
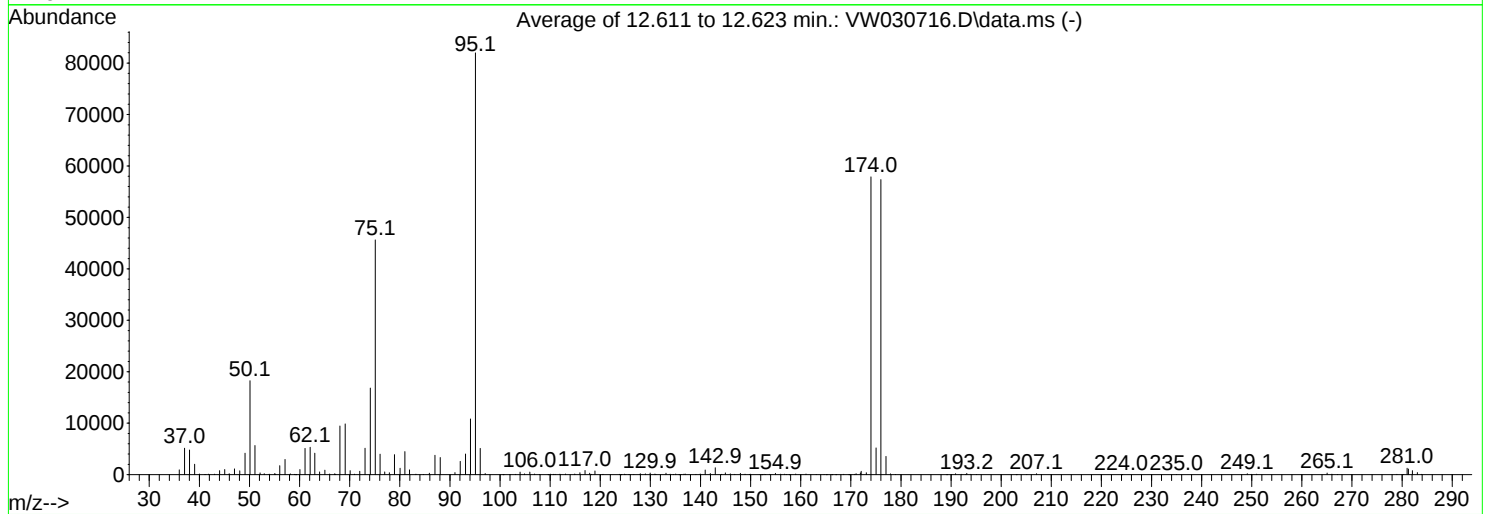


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102324\
Data File : VW030716.D
Acq On : 23 Oct 2024 09:16
Operator : SY/MD
Sample : BFB582
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB582

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Title : SFAM01.0
Last Update : Thu Oct 24 01:34:36 2024

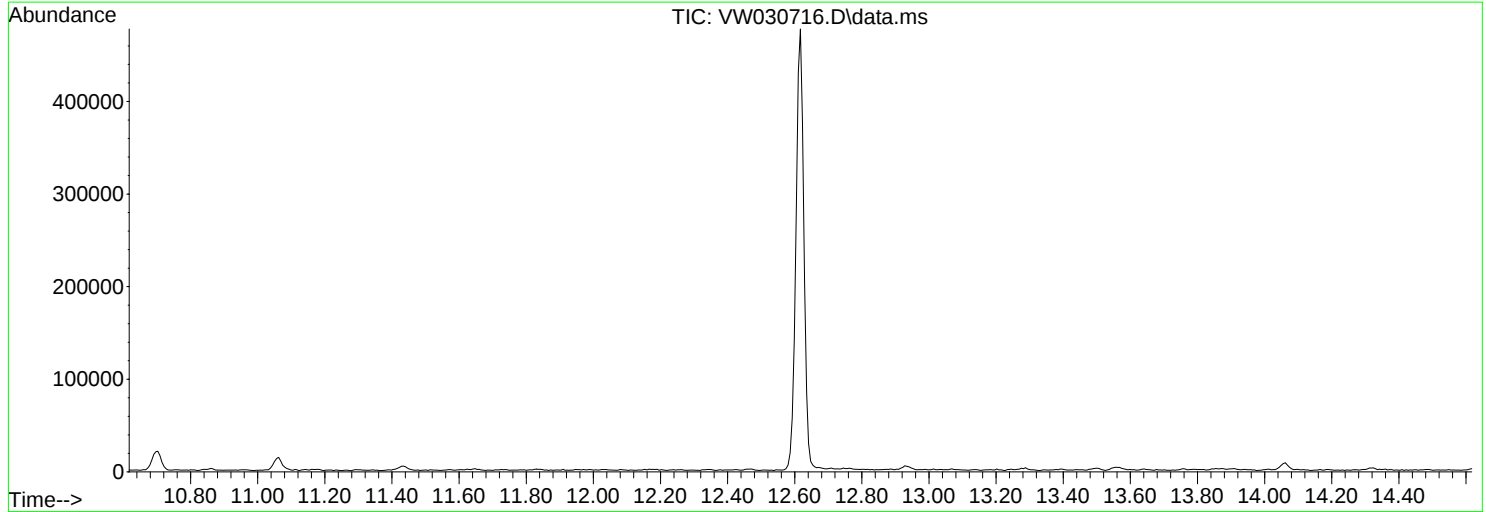

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	18257	PASS
75	95	30	80	55.7	45627	PASS
95	95	100	100	100.0	81989	PASS
96	95	5	9	6.2	5105	PASS
173	174	0.00	2	0.6	361	PASS
174	95	50	120	70.6	57885	PASS
175	174	5	9	9.0	5192	PASS
176	174	95	101	99.1	57341	PASS
177	176	5	9	6.2	3541	PASS

m/z	Abundance
35.30	114.0
35.70	84.0
36.20	76.0
37.50	66.0
38.20	59.0
40.00	261.0
43.30	107.0
44.20	154.0
45.10	60.0
46.10	77.0
47.40	88.0
51.50	116.0
55.10	85.0
57.30	77.0
62.90	62.0
63.90	60.0
65.70	64.0
68.80	65.0
69.20	66.0
70.30	74.0
72.70	52.0
76.00	52.0
81.50	61.0
91.10	72.0
102.90	51.0
146.90	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582

m/z	Abundance
36.00	1058.0
37.00	5377.0
38.00	5039.0
39.10	2494.0
40.00	518.0
41.10	94.0
42.00	100.0
43.00	160.0
44.00	1064.0
45.10	1182.0
46.00	174.0
47.00	1172.0
48.00	789.0
49.10	4717.0
50.10	19264.0
51.10	5973.0
52.10	334.0
53.00	241.0
54.00	115.0
55.00	492.0
56.00	1978.0
57.10	3303.0
58.10	190.0
59.00	163.0
60.00	1222.0
61.10	5142.0
62.10	5757.0
63.10	4628.0
64.10	643.0
65.00	873.0
66.10	207.0
67.00	348.0
68.00	9902.0
69.10	10049.0
70.10	914.0
70.90	61.0
72.00	906.0
73.00	5694.0
74.10	17336.0
75.10	47488.0
76.10	4271.0
77.10	590.0
78.00	420.0
79.00	4246.0
80.00	1347.0
81.00	4606.0
82.00	1055.0
83.20	104.0
86.00	388.0
87.00	4027.0
88.00	3425.0
91.00	583.0
92.00	2698.0
93.10	3736.0
94.10	10340.0
95.10	81872.0
96.10	5372.0
97.10	202.0
102.80	123.0
104.00	572.0
105.00	132.0
106.00	488.0
106.90	134.0
110.10	96.0
110.70	150.0
112.00	81.0
113.10	97.0
114.90	147.0
115.90	379.0
116.90	802.0
117.90	392.0
119.00	782.0
120.50	85.0
124.10	53.0
124.90	154.0
125.70	128.0
127.90	327.0
129.00	185.0
129.90	302.0
130.90	182.0
133.10	380.0
134.00	94.0
135.00	105.0
135.70	53.0
136.10	72.0
137.00	161.0
139.10	69.0
139.90	102.0
141.00	821.0
142.00	215.0
142.90	1283.0
144.20	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582

145.00	554.0
145.90	192.0
146.90	145.0
147.90	238.0
148.90	115.0
149.80	69.0
151.90	87.0
152.70	77.0
153.90	100.0
155.00	218.0
156.10	119.0
157.20	130.0
159.00	146.0
161.00	205.0
163.10	141.0
164.70	64.0
165.10	50.0
166.20	51.0
168.60	105.0
170.80	165.0
171.90	985.0
174.00	56248.0
175.00	4571.0
176.00	48584.0
177.00	3134.0
177.90	196.0
178.90	113.0
189.10	55.0
190.90	236.0
192.10	190.0
193.20	504.0
194.00	112.0
195.10	72.0
203.00	57.0
205.10	132.0
207.00	270.0
208.00	85.0
224.00	51.0
235.00	64.0
249.10	351.0
249.90	135.0
251.00	233.0
265.10	548.0
266.00	151.0
267.10	86.0
279.00	117.0
280.30	128.0
281.00	3728.0
282.10	922.0
283.10	552.0
283.90	214.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582

m/z	Abundance
36.00	1244.0
37.10	5944.0
38.10	5324.0
39.10	2023.0
40.00	353.0
41.30	96.0
41.80	89.0
43.10	139.0
44.10	909.0
45.00	1177.0
45.90	197.0
46.20	194.0
47.00	1280.0
48.00	805.0
49.10	4532.0
50.10	20544.0
51.10	6525.0
52.10	404.0
52.90	157.0
53.90	98.0
55.20	379.0
56.10	1981.0
57.10	3214.0
58.10	129.0
59.20	55.0
60.10	898.0
61.10	6163.0
62.10	5848.0
63.10	4676.0
64.00	660.0
65.00	972.0
66.00	108.0
67.20	313.0
68.10	11008.0
69.10	10981.0
70.10	987.0
71.00	133.0
72.00	588.0
73.10	5642.0
74.10	18488.0
75.10	50728.0
76.10	4307.0
76.90	638.0
77.80	426.0
79.00	4238.0
80.00	1377.0
81.00	5082.0
82.00	939.0
83.10	78.0
85.80	370.0
87.00	4563.0
88.00	3673.0
91.00	485.0
92.10	2779.0
93.10	4691.0
94.10	11993.0
95.10	91768.0
96.00	5245.0
97.00	256.0
100.60	58.0
103.10	144.0
104.00	621.0
104.80	151.0
105.90	547.0
106.90	145.0
107.90	73.0
110.10	84.0
111.00	137.0
112.00	89.0
113.00	186.0
114.80	131.0
116.00	501.0
117.00	879.0
117.90	433.0
119.00	827.0
120.60	67.0
123.80	99.0
125.10	133.0
125.90	87.0
126.80	61.0
128.10	202.0
128.90	191.0
130.00	315.0
130.90	153.0
133.10	387.0
133.90	104.0
135.10	197.0
136.90	201.0
139.10	81.0
140.00	159.0
141.00	969.0
141.90	205.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582

142.90	1611.0
144.20	76.0
144.90	301.0
146.00	140.0
146.80	83.0
148.00	193.0
148.90	118.0
150.00	188.0
152.70	82.0
153.80	89.0
155.00	282.0
156.00	127.0
156.80	184.0
159.10	112.0
161.10	82.0
164.60	78.0
168.60	77.0
171.00	306.0
172.10	1135.0
174.00	61344.0
175.10	6003.0
176.00	68520.0
177.00	4336.0
177.90	222.0
190.10	57.0
190.90	228.0
193.00	213.0
193.90	56.0
207.10	108.0
249.00	115.0
249.90	59.0
250.90	71.0
265.00	203.0
266.00	108.0
278.90	50.0
281.30	2090.0
281.90	585.0
282.20	569.0
283.00	507.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582

m/z	Abundance
36.10	744.0
37.10	4086.0
38.10	4195.0
39.00	1582.0
40.10	332.0
41.80	87.0
44.10	840.0
45.10	849.0
46.00	180.0
47.00	952.0
48.10	637.0
49.10	3285.0
50.10	14962.0
51.10	4474.0
52.10	274.0
53.00	175.0
54.00	91.0
55.00	309.0
56.00	1268.0
57.10	2546.0
58.20	145.0
60.00	851.0
61.10	4012.0
62.10	4334.0
63.10	3437.0
64.10	466.0
65.10	814.0
65.90	85.0
66.80	128.0
68.00	7499.0
69.10	8756.0
70.10	637.0
70.90	129.0
71.90	441.0
73.10	4084.0
74.10	14626.0
75.10	38664.0
76.10	3550.0
77.10	407.0
77.90	243.0
78.90	3176.0
80.10	982.0
81.00	3718.0
81.90	773.0
83.30	115.0
84.70	102.0
85.80	114.0
87.00	2709.0
88.10	2936.0
91.00	383.0
92.00	2297.0
93.10	3647.0
94.10	10156.0
95.10	72328.0
96.10	4699.0
97.00	188.0
102.00	63.0
103.90	333.0
104.90	180.0
106.00	456.0
106.90	108.0
109.60	56.0
110.00	101.0
111.00	92.0
111.90	103.0
113.00	102.0
115.00	90.0
115.90	239.0
116.90	755.0
118.20	229.0
118.90	551.0
123.90	85.0
124.80	97.0
126.60	51.0
128.00	272.0
129.10	143.0
129.90	361.0
131.10	114.0
133.00	97.0
133.90	74.0
134.60	86.0
135.00	103.0
136.70	266.0
139.90	75.0
140.90	903.0
141.90	251.0
143.00	1100.0
144.90	214.0
146.00	112.0
146.90	173.0
148.00	299.0
149.00	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582

149.90	111.0
152.20	58.0
153.00	135.0
154.90	237.0
155.90	71.0
156.80	132.0
157.70	56.0
158.90	126.0
161.10	115.0
167.00	51.0
169.60	54.0
171.10	274.0
172.00	876.0
173.10	1083.0
174.00	56064.0
175.00	5002.0
176.00	54920.0
177.00	3152.0
177.80	95.0
190.10	58.0
191.00	134.0
192.90	91.0
207.10	149.0
249.00	116.0
265.00	229.0
281.20	1209.0
282.10	249.0
282.90	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB582