

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102418\
 Data File : VW006313.D
 Acq On : 24 Oct 2018 12:34
 Operator : SY/AP
 Sample : J5635-06
 Misc : 5.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40E5

Quant Time: Oct 25 07:47:37 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 25 07:32:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	406428	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	385654	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	205439	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	79887	17.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.72%
7) Chloroethane-d5	2.89	69	79099	20.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.20%
10) 1,1-Dichloroethene-d2	4.01	63	128052	14.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.20%
20) 2-Butanone-d5	7.08	46	62294	41.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.00%
24) Chloroform-d	7.65	84	192617	21.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.52%
26) 1,2-Dichloroethane-d4	8.31	65	113733	23.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.40%
29) Benzene-d6	8.27	84	384518	21.96	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.84%
33) 1,2-Dichloropropane-d6	9.27	67	115059	21.77	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.08%
37) Toluene-d8	10.33	98	376556	21.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.04%
38) trans-1,3-Dichloropropene-	10.58	79	49112	19.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.48%
39) 2-Hexanone-d5	10.93	63	51236	40.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	113027	22.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	165669	23.53	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.12%


Target Compounds					Ovalue
13) Acetone	4.13	43	39396	25.667 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102418\
Data File : VW006313.D
Acq On : 24 Oct 2018 12:34
Operator : SY/AP
Sample : J5635-06
Misc : 5.09G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40E5

Quant Time: Oct 25 07:47:37 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 25 07:32:16 2018
Response via : Initial Calibration

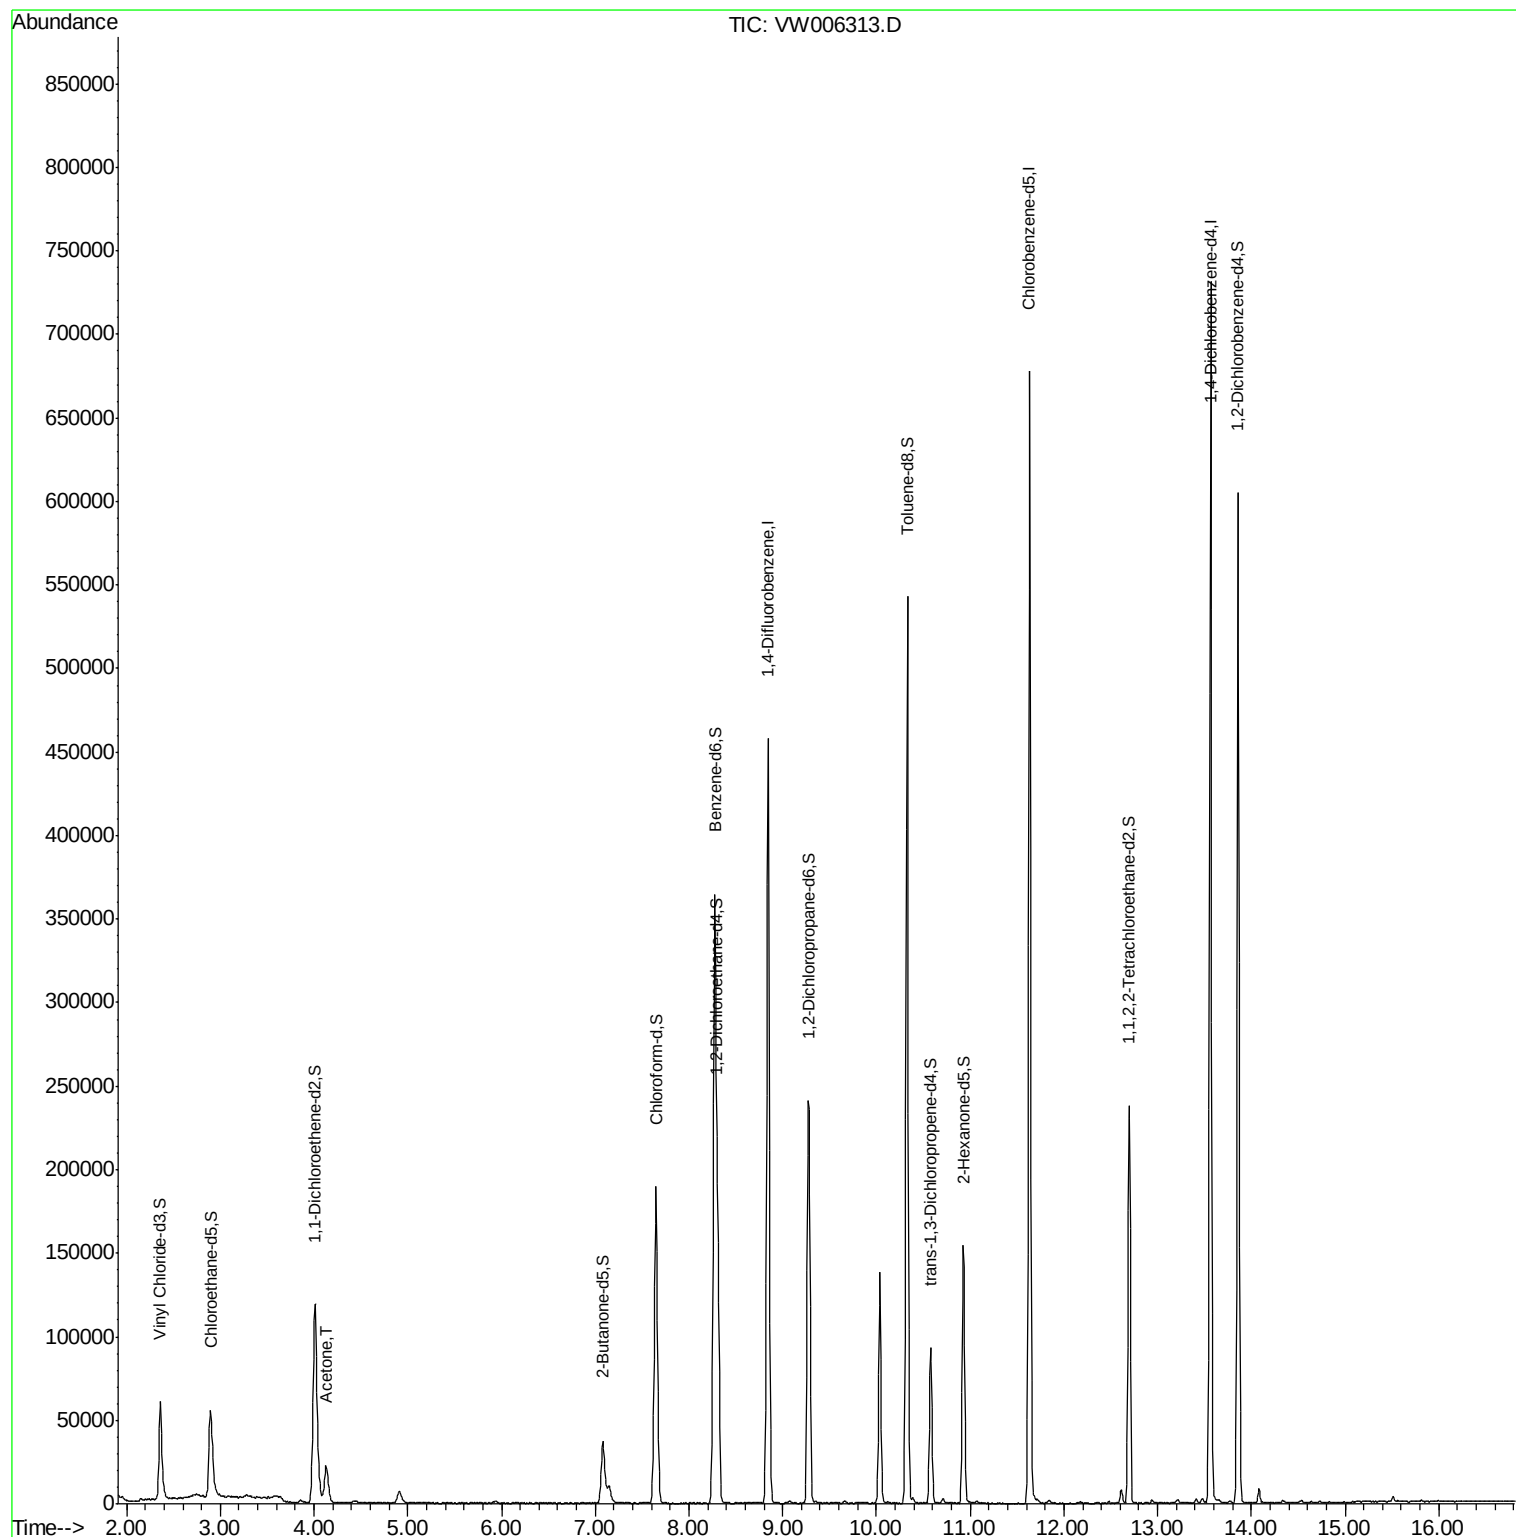

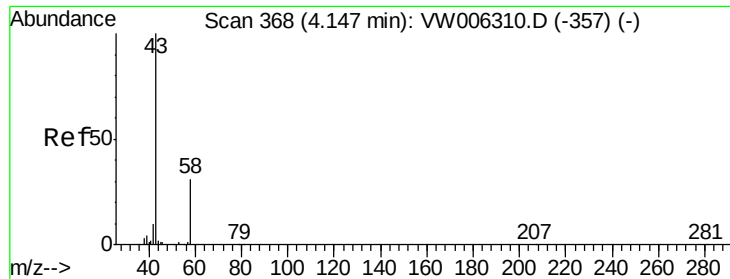

#13

Acetone

Concen: 25.667 ug/L

RT: 4.13 min Scan# 365

Delta R.T. -0.01 min

Lab File: VW006313.D

Acq: 24 Oct 2018 12:34

Instrument :

MSVOA_W

ClientSampleId :

A40E5

Tot Ion: 43 Resp: 39396

Ion Ratio Lower Upper

43 100

58 30.4 0.0 61.2

