


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102418\
 Data File : VW006309.D
 Acq On : 24 Oct 2018 08:54
 Operator : SY/AP
 Sample : BFB92
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB92

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Title : VOC Analysis
 Last Update : Fri Oct 26 23:43:44 2018

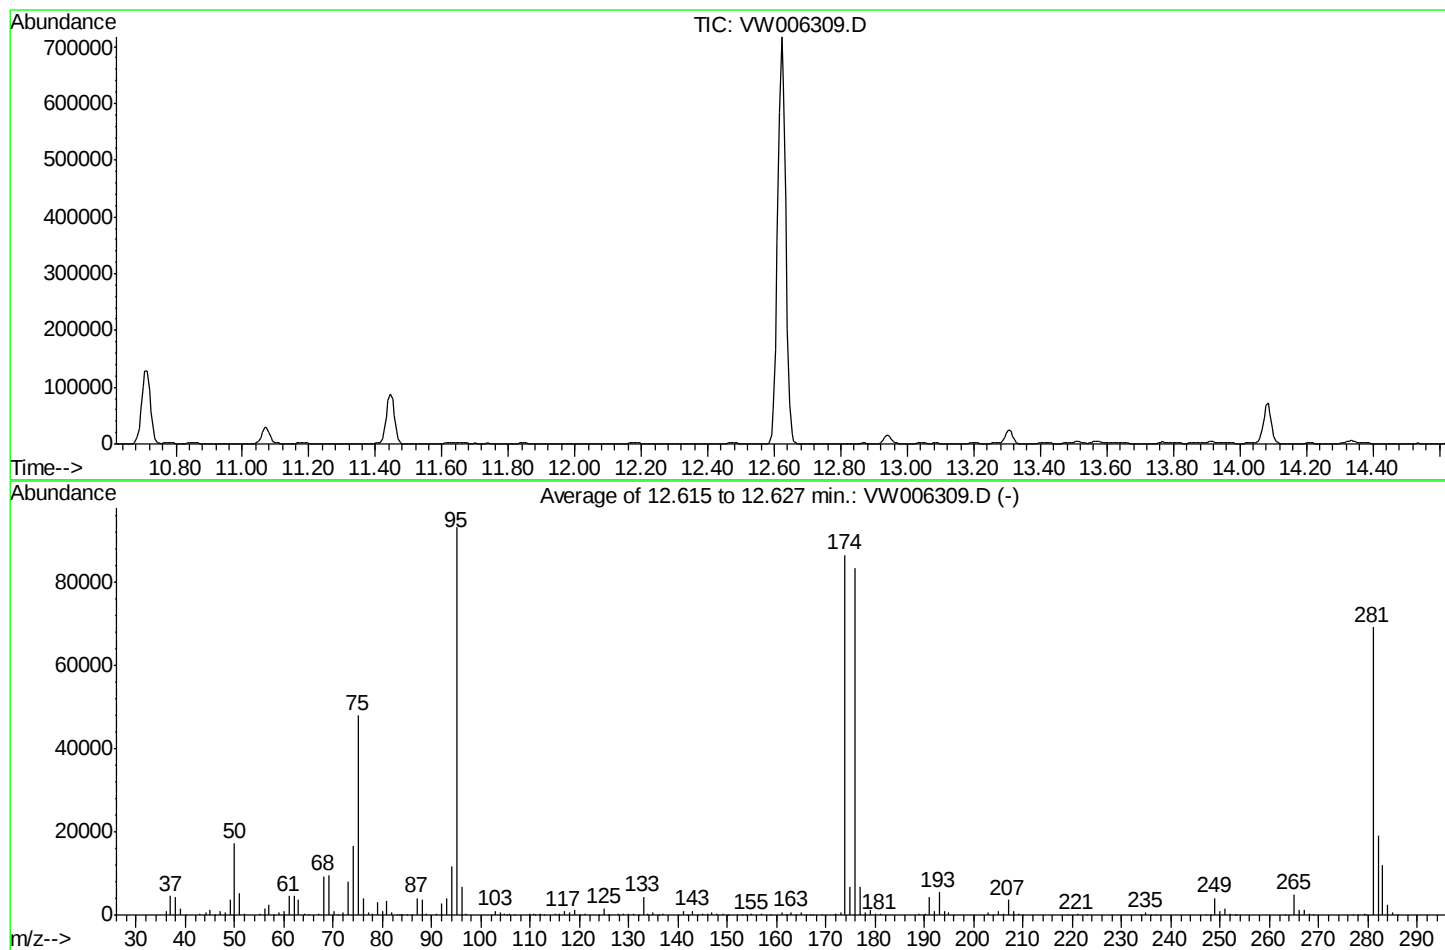

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	17103	PASS
75	95	30	80	51.4	47880	PASS
95	95	100	100	100.0	93168	PASS
96	95	5	9	7.4	6874	PASS
173	174	0.00	2	0.8	695	PASS
174	95	50	120	92.9	86592	PASS
175	174	5	9	7.8	6749	PASS
176	174	95	101	96.1	83224	PASS
177	176	5	9	8.2	6815	PASS

Scan 1750 (12.573 min): VW006309.D
BFB92

m/z	Abundance
40.10	91.0
40.90	88.0
44.10	178.0
57.00	71.0
73.10	56.0
206.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92

m/z	Abundance
36.00	698.0
37.00	4028.0
38.10	3499.0
39.00	1562.0
40.10	129.0
41.00	58.0
43.00	277.0
44.10	774.0
45.00	1677.0
45.90	97.0
47.10	883.0
47.90	446.0
49.00	3533.0
50.00	14957.0
51.10	4814.0
52.00	250.0
55.00	308.0
56.00	1393.0
57.00	2120.0
58.00	162.0
59.00	810.0
60.00	824.0
61.00	3786.0
62.00	3912.0
63.00	2963.0
64.00	278.0
65.00	163.0
66.90	271.0
68.00	7833.0
69.00	8466.0
70.10	755.0
71.10	92.0
72.00	505.0
73.10	8958.0
74.00	14440.0
75.00	41136.0
76.00	3259.0
77.00	527.0
78.00	348.0
78.90	2624.0
79.90	795.0
80.90	2942.0
81.90	697.0
82.90	108.0
83.50	95.0
84.00	63.0
85.00	66.0
85.80	127.0
87.00	3413.0
88.00	3231.0
88.90	406.0
91.00	286.0
92.00	2341.0
93.00	3350.0
94.00	10412.0
95.00	77704.0
96.00	5894.0
97.00	247.0
102.90	1139.0
103.80	732.0
104.80	324.0
105.80	373.0
106.80	136.0
110.00	401.0
110.90	347.0
111.90	374.0
112.80	146.0
115.00	497.0
115.90	366.0
116.90	738.0
118.00	851.0
118.90	1385.0
119.90	176.0
121.00	169.0
123.90	55.0
125.00	1674.0
127.80	245.0
128.90	221.0
130.00	249.0
130.90	275.0
132.00	125.0
133.00	5608.0
135.00	702.0
136.00	60.0
137.00	151.0
140.00	51.0
141.00	632.0
141.90	93.0
142.90	875.0
144.10	99.0
145.00	222.0
145.90	133.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92

146.90	717.0
148.00	303.0
149.00	480.0
150.10	105.0
153.10	59.0
154.90	269.0
156.80	183.0
158.80	119.0
161.00	480.0
161.90	61.0
162.10	63.0
162.90	1103.0
164.10	106.0
164.90	602.0
166.00	121.0
166.70	89.0
171.80	218.0
173.00	836.0
173.90	64312.0
175.00	5325.0
175.90	62008.0
177.00	6323.0
178.00	706.0
179.00	1534.0
180.10	199.0
181.00	261.0
189.00	589.0
190.20	219.0
191.00	5726.0
192.00	1364.0
193.00	6714.0
194.00	1261.0
194.90	965.0
196.00	125.0
203.00	697.0
204.00	200.0
205.00	1341.0
205.90	341.0
207.10	4448.0
208.00	1083.0
209.00	515.0
210.00	67.0
218.90	214.0
220.90	238.0
222.80	82.0
235.00	594.0
236.00	190.0
237.00	187.0
246.90	100.0
249.00	4752.0
250.00	1154.0
251.00	2015.0
251.90	617.0
253.20	227.0
263.20	66.0
265.00	5552.0
266.00	1596.0
267.10	1295.0
268.00	358.0
269.00	144.0
277.10	91.0
278.00	62.0
279.20	347.0
281.10	76704.0
282.10	22184.0
283.00	13792.0
284.10	2818.0
285.00	960.0
285.90	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92

m/z	Abundance
36.00	1020.0
37.00	5119.0
38.00	4761.0
39.00	1837.0
39.90	189.0
41.00	56.0
43.00	275.0
44.00	898.0
45.10	1391.0
46.00	127.0
47.00	1107.0
47.90	682.0
49.00	4044.0
50.00	19216.0
51.00	6091.0
52.10	286.0
55.00	312.0
56.00	1787.0
57.00	3075.0
57.90	139.0
59.00	677.0
60.00	912.0
61.00	5203.0
62.00	4949.0
63.00	4002.0
64.00	407.0
65.10	120.0
67.00	320.0
68.00	10414.0
69.00	10592.0
70.00	917.0
70.90	83.0
71.10	87.0
72.00	681.0
73.00	8514.0
74.00	18768.0
75.00	53880.0
76.10	4533.0
77.10	782.0
77.90	451.0
78.90	3515.0
79.90	1047.0
80.90	4040.0
81.90	798.0
83.00	82.0
83.70	119.0
85.00	95.0
85.90	83.0
86.90	4357.0
87.90	4156.0
89.00	282.0
90.90	427.0
92.00	3305.0
93.00	4211.0
94.00	13040.0
95.00	103424.0
96.00	7536.0
97.10	474.0
102.90	1089.0
103.90	798.0
104.80	385.0
105.90	525.0
106.80	116.0
109.90	334.0
110.70	275.0
112.10	218.0
112.90	126.0
115.00	489.0
115.90	546.0
116.90	830.0
118.00	893.0
118.90	1286.0
119.90	165.0
121.00	222.0
123.90	116.0
125.00	1775.0
125.70	386.0
127.90	379.0
128.90	279.0
129.90	379.0
130.90	303.0
131.80	150.0
133.00	4671.0
134.90	539.0
136.10	67.0
136.80	233.0
140.00	115.0
140.90	1150.0
142.00	139.0
143.00	1115.0
143.90	118.0
145.00	182.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92

146.00	229.0
146.90	621.0
147.80	326.0
149.00	372.0
150.00	167.0
153.10	74.0
154.90	212.0
156.80	326.0
158.90	178.0
160.90	616.0
161.90	73.0
163.00	693.0
164.00	162.0
164.90	708.0
165.90	146.0
166.70	68.0
167.20	80.0
169.10	76.0
172.00	287.0
173.90	97216.0
174.90	7529.0
175.90	92112.0
177.00	7611.0
178.00	648.0
179.00	1378.0
179.90	190.0
181.00	155.0
188.90	506.0
190.00	233.0
191.00	4257.0
192.00	1094.0
193.00	6045.0
194.00	1041.0
195.00	692.0
195.80	155.0
203.00	591.0
204.00	184.0
205.00	1084.0
205.90	341.0
207.00	3966.0
208.00	755.0
209.00	385.0
209.90	63.0
218.90	168.0
221.00	256.0
222.90	76.0
233.80	111.0
234.90	550.0
236.00	113.0
237.00	170.0
247.00	70.0
249.00	4659.0
250.00	1312.0
251.00	1731.0
252.00	466.0
252.90	240.0
265.00	5388.0
266.00	1496.0
267.00	1362.0
268.00	246.0
269.00	130.0
276.90	63.0
278.10	107.0
279.40	309.0
281.00	76824.0
282.00	20408.0
283.00	13607.0
284.00	2504.0
285.10	831.0
286.00	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92

m/z	Abundance
36.00	820.0
37.00	4444.0
38.00	4436.0
39.10	1552.0
40.00	179.0
43.00	215.0
44.00	732.0
45.00	1106.0
46.10	101.0
47.00	1150.0
48.00	561.0
49.00	3963.0
50.00	17136.0
51.00	5249.0
52.00	248.0
55.10	305.0
56.00	1516.0
57.00	2621.0
57.90	118.0
59.00	421.0
60.00	931.0
61.00	4568.0
62.00	4599.0
63.00	3747.0
64.10	329.0
65.00	120.0
66.90	308.0
68.00	9656.0
69.00	9978.0
70.10	751.0
71.00	102.0
72.00	547.0
73.00	6535.0
74.00	16824.0
75.00	48624.0
76.00	4001.0
77.10	581.0
77.90	360.0
78.90	3318.0
79.90	759.0
80.90	3643.0
81.90	692.0
83.00	76.0
85.00	61.0
86.00	109.0
87.00	4422.0
87.90	3621.0
88.80	213.0
90.90	495.0
92.00	2874.0
93.00	4221.0
94.00	11978.0
95.00	98376.0
96.00	7194.0
96.90	260.0
102.10	60.0
102.90	591.0
103.90	559.0
105.10	275.0
105.90	413.0
106.90	140.0
110.10	216.0
111.00	272.0
111.90	141.0
112.80	100.0
115.00	295.0
115.90	381.0
116.90	828.0
118.00	515.0
118.90	954.0
120.00	76.0
121.00	120.0
123.90	54.0
125.10	839.0
126.10	254.0
127.90	413.0
129.00	234.0
129.90	430.0
130.90	220.0
133.10	2647.0
133.80	594.0
134.90	403.0
137.00	232.0
141.00	1045.0
141.90	162.0
142.90	927.0
143.90	76.0
145.00	154.0
146.00	147.0
146.90	419.0
147.90	334.0
149.00	228.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92

150.00	163.0
152.00	57.0
152.90	69.0
153.80	63.0
154.90	361.0
156.90	179.0
158.90	118.0
160.90	379.0
161.80	85.0
163.00	490.0
163.90	120.0
164.90	382.0
166.00	94.0
172.00	386.0
173.10	1250.0
173.90	98248.0
175.00	7395.0
175.90	95552.0
177.00	6512.0
177.90	487.0
179.00	971.0
179.90	153.0
180.80	95.0
189.00	302.0
190.20	125.0
191.00	2727.0
192.10	611.0
193.00	3558.0
194.00	628.0
195.00	342.0
203.00	324.0
204.10	61.0
205.00	747.0
205.90	146.0
207.00	2628.0
208.00	645.0
209.00	355.0
219.00	93.0
221.00	169.0
223.00	64.0
234.90	365.0
236.10	80.0
237.00	107.0
247.10	112.0
248.00	83.0
249.00	2880.0
249.90	785.0
251.10	1095.0
252.10	273.0
253.00	179.0
265.00	3597.0
266.00	992.0
267.00	904.0
268.10	173.0
269.00	86.0
278.10	68.0
279.20	191.0
281.00	53760.0
282.10	14214.0
283.00	8866.0
284.10	1689.0
285.00	521.0
286.00	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB92