

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
 Data File : VW030739.D
 Acq On : 24 Oct 2024 12:31
 Operator : SY/MD
 Sample : VW1024SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 25 01:43:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 01:42:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	268481	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	256812	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	113086	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	52381	12.412	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	49.640%		
7) Chloroethane-d5	2.899	69	51191	16.025	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.080%		
11) 1,1-Dichloroethene-d2	4.021	65	23199	13.217	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.880%		
21) 2-Butanone-d5	7.081	46	34433	45.339	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.680%		
24) Chloroform-d	7.654	84	141407	18.417	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	73.680%		
26) 1,2-Dichloroethane-d4	8.307	65	77117	19.315	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	77.280%		
32) Benzene-d6	8.276	84	239814	16.089	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	64.360%		
36) 1,2-Dichloropropane-d6	9.276	67	80139	18.318	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	73.280%		
41) Toluene-d8	10.325	98	205479	15.101	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	60.400%		
43) trans-1,3-Dichloroprop...	10.581	79	28795	15.719	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	62.880%		
47) 2-Hexanone-d5	10.922	63	23878	42.376	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	84.760%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	70756	22.023	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.080%		
66) 1,2-Dichlorobenzene-d4	13.854	152	78086	20.407	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.640%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3246	0.516	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
Data File : VW030739.D
Acq On : 24 Oct 2024 12:31
Operator : SY/MD
Sample : VW1024SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 25 01:43:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 01:42:56 2024
Response via : Initial Calibration

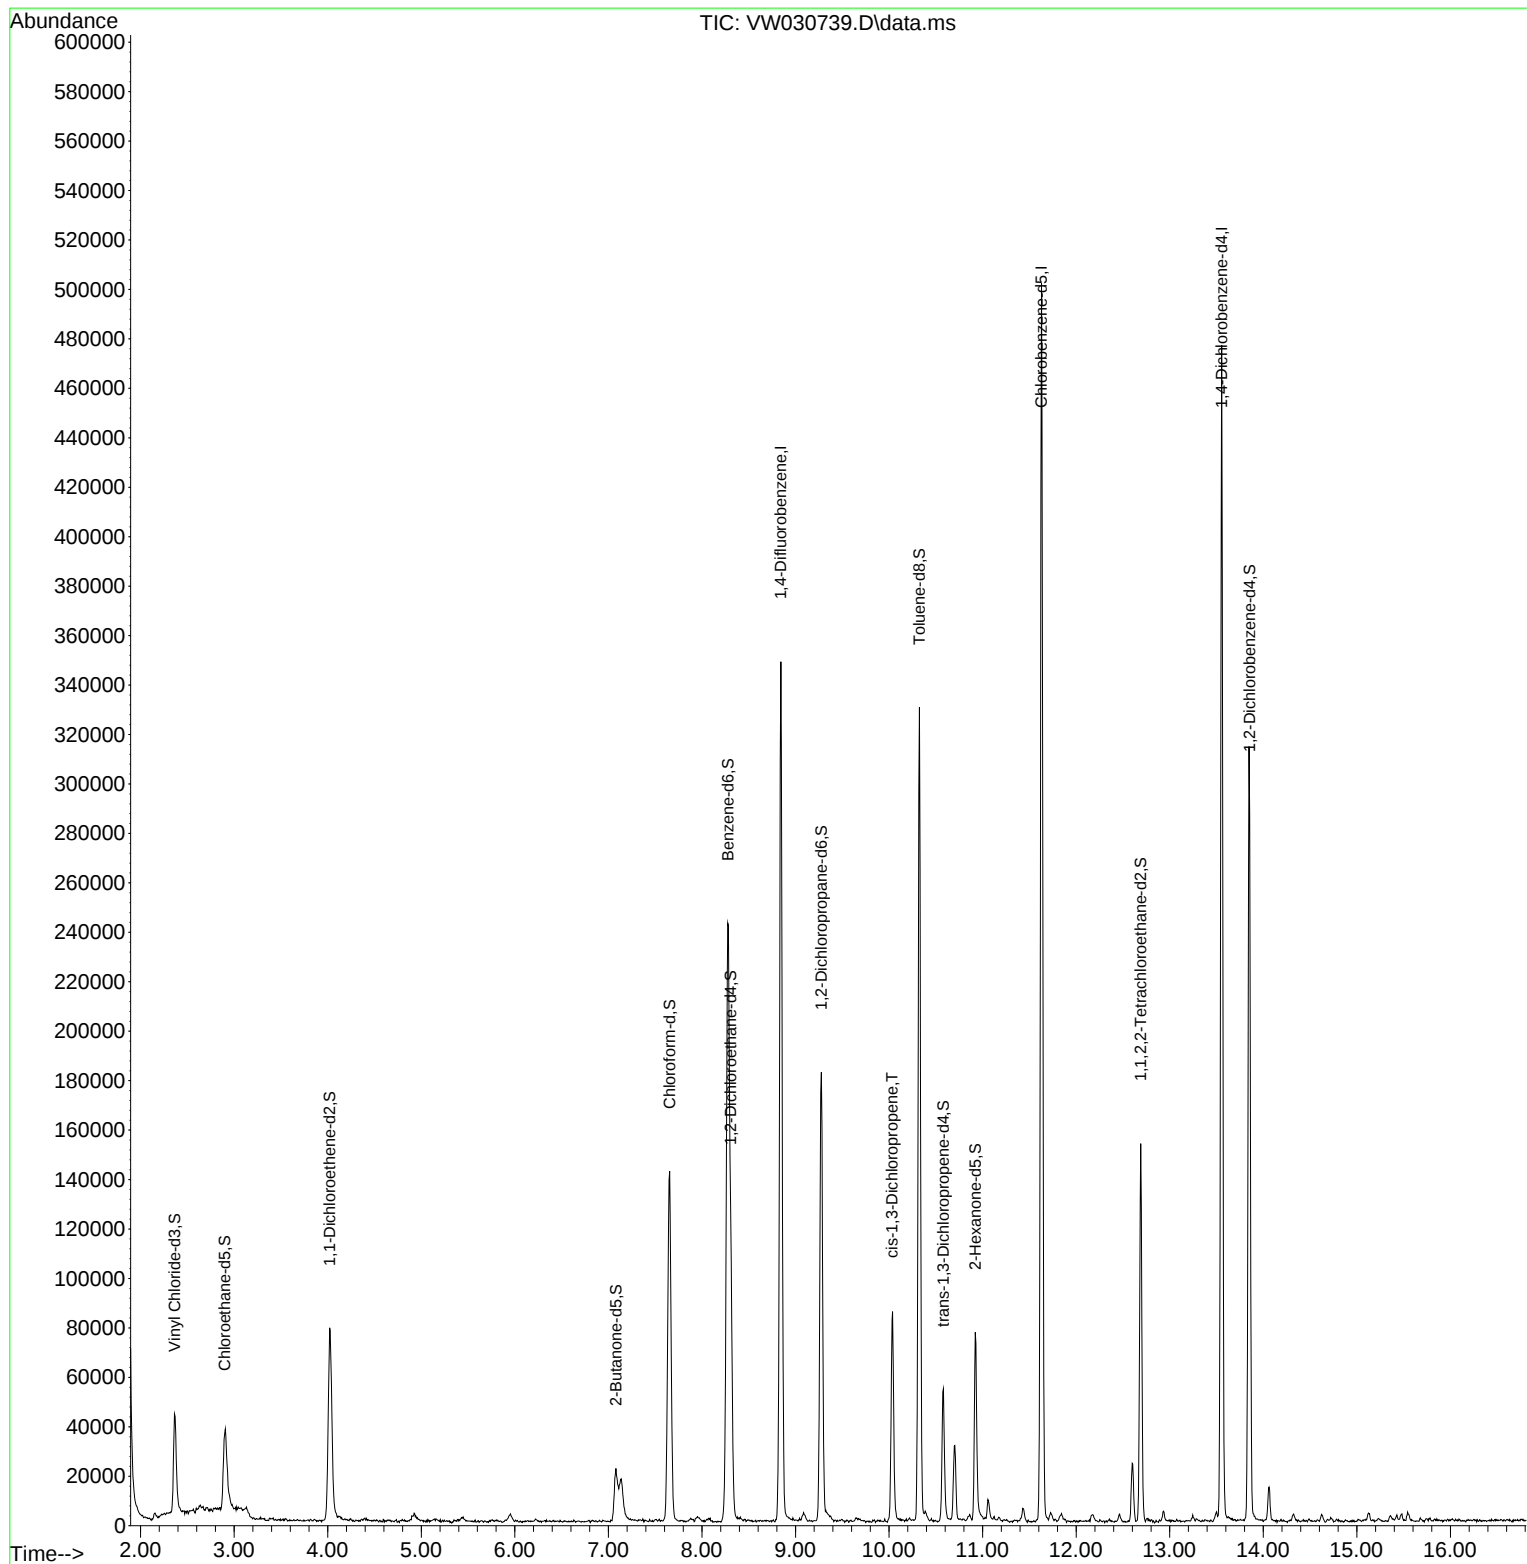

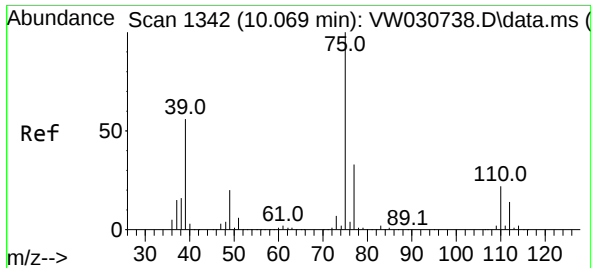

#39
 cis-1,3-Dichloropropene
 Concen: 0.516 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030739.D
 Acq: 24 Oct 2024 12:31

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3246
 Ion Ratio Lower Upper
 75 100
 77 34.5 21.1 39.1

