

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
 Data File : VW030740.D
 Acq On : 24 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4436-16
 Misc : 5.27g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 25 01:43:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 01:42:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	256019	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	242721	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	104822	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	104622	25.998	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.000%
7) Chloroethane-d5	2.899	69	83590	27.441	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.760%
11) 1,1-Dichloroethene-d2	4.021	65	42748	25.540	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	102.160%
21) 2-Butanone-d5	7.075	46	34584	47.754	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.500%
24) Chloroform-d	7.654	84	186529	25.476	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.920%
26) 1,2-Dichloroethane-d4	8.307	65	99542	26.145	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.600%
32) Benzene-d6	8.276	84	359543	25.522	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.080%
36) 1,2-Dichloropropane-d6	9.270	67	106785	25.826	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.320%
41) Toluene-d8	10.325	98	328622	25.553	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.200%
43) trans-1,3-Dichloroprop...	10.575	79	40578	23.437	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.760%
47) 2-Hexanone-d5	10.922	63	26810	50.342	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	76255	25.112	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.440%
66) 1,2-Dichlorobenzene-d4	13.854	152	99506	28.056	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	112.240%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4005	0.673	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
Data File : VW030740.D
Acq On : 24 Oct 2024 14:42
Operator : SY/MD
Sample : P4436-16
Misc : 5.27g/10mL/MSVOA_W/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 25 01:43:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 01:42:56 2024
Response via : Initial Calibration

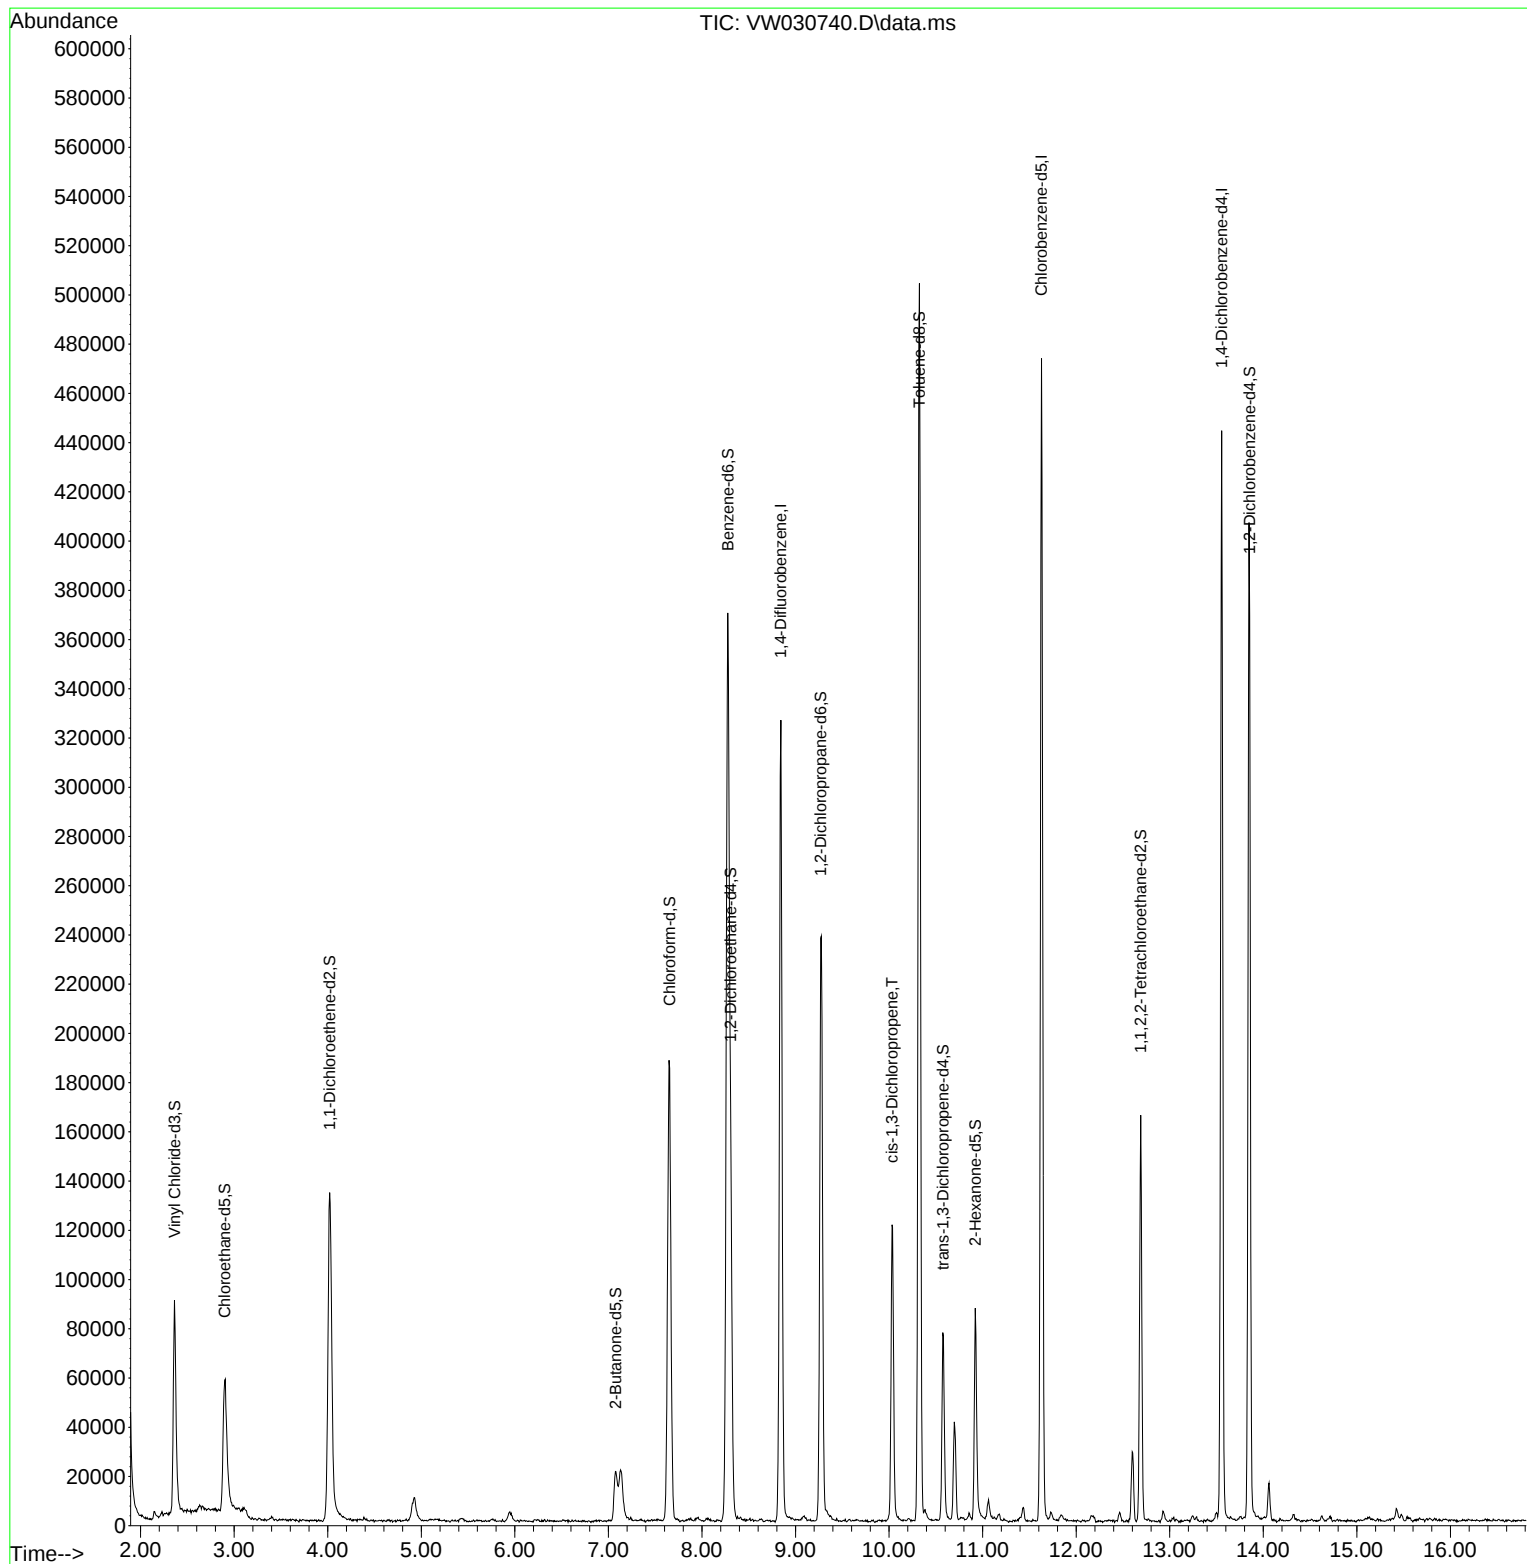

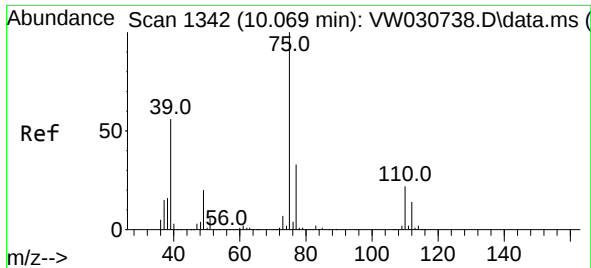

#39
cis-1,3-Dichloropropene
Concen: 0.673 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW030740.D
Acq: 24 Oct 2024 14:42

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 4005
Ion Ratio Lower Upper
75 100
77 45.6 21.1 39.1#

