

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
 Data File : VW030742.D
 Acq On : 24 Oct 2024 13:55
 Operator : SY/MD
 Sample : P4493-04
 Misc : 5.22g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 25 01:44:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 01:42:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	236217	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	203714	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	66663	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	40670	10.953	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	43.800%		
7) Chloroethane-d5	2.893	69	42491	15.118	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.480%		
11) 1,1-Dichloroethene-d2	4.021	65	17943	11.619	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.480%		
21) 2-Butanone-d5	7.075	46	35266	52.778	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.560%		
24) Chloroform-d	7.648	84	137933	20.418	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.680%		
26) 1,2-Dichloroethane-d4	8.307	65	77814	22.152	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.600%		
32) Benzene-d6	8.276	84	199145	16.843	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	67.360%		
36) 1,2-Dichloropropane-d6	9.276	67	77062	22.206	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.840%		
41) Toluene-d8	10.325	98	144506	13.388	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	53.560%		
43) trans-1,3-Dichloroprop...	10.581	79	25896	17.821	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.280%		
47) 2-Hexanone-d5	10.922	63	24196	54.133	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.260%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66108	25.939	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.760%		
66) 1,2-Dichlorobenzene-d4	13.848	152	47335	20.986	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.960%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2283	0.457	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
Data File : VW030742.D
Acq On : 24 Oct 2024 13:55
Operator : SY/MD
Sample : P4493-04
Misc : 5.22g/10mL/MSVOA_W/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 25 01:44:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 01:42:56 2024
Response via : Initial Calibration

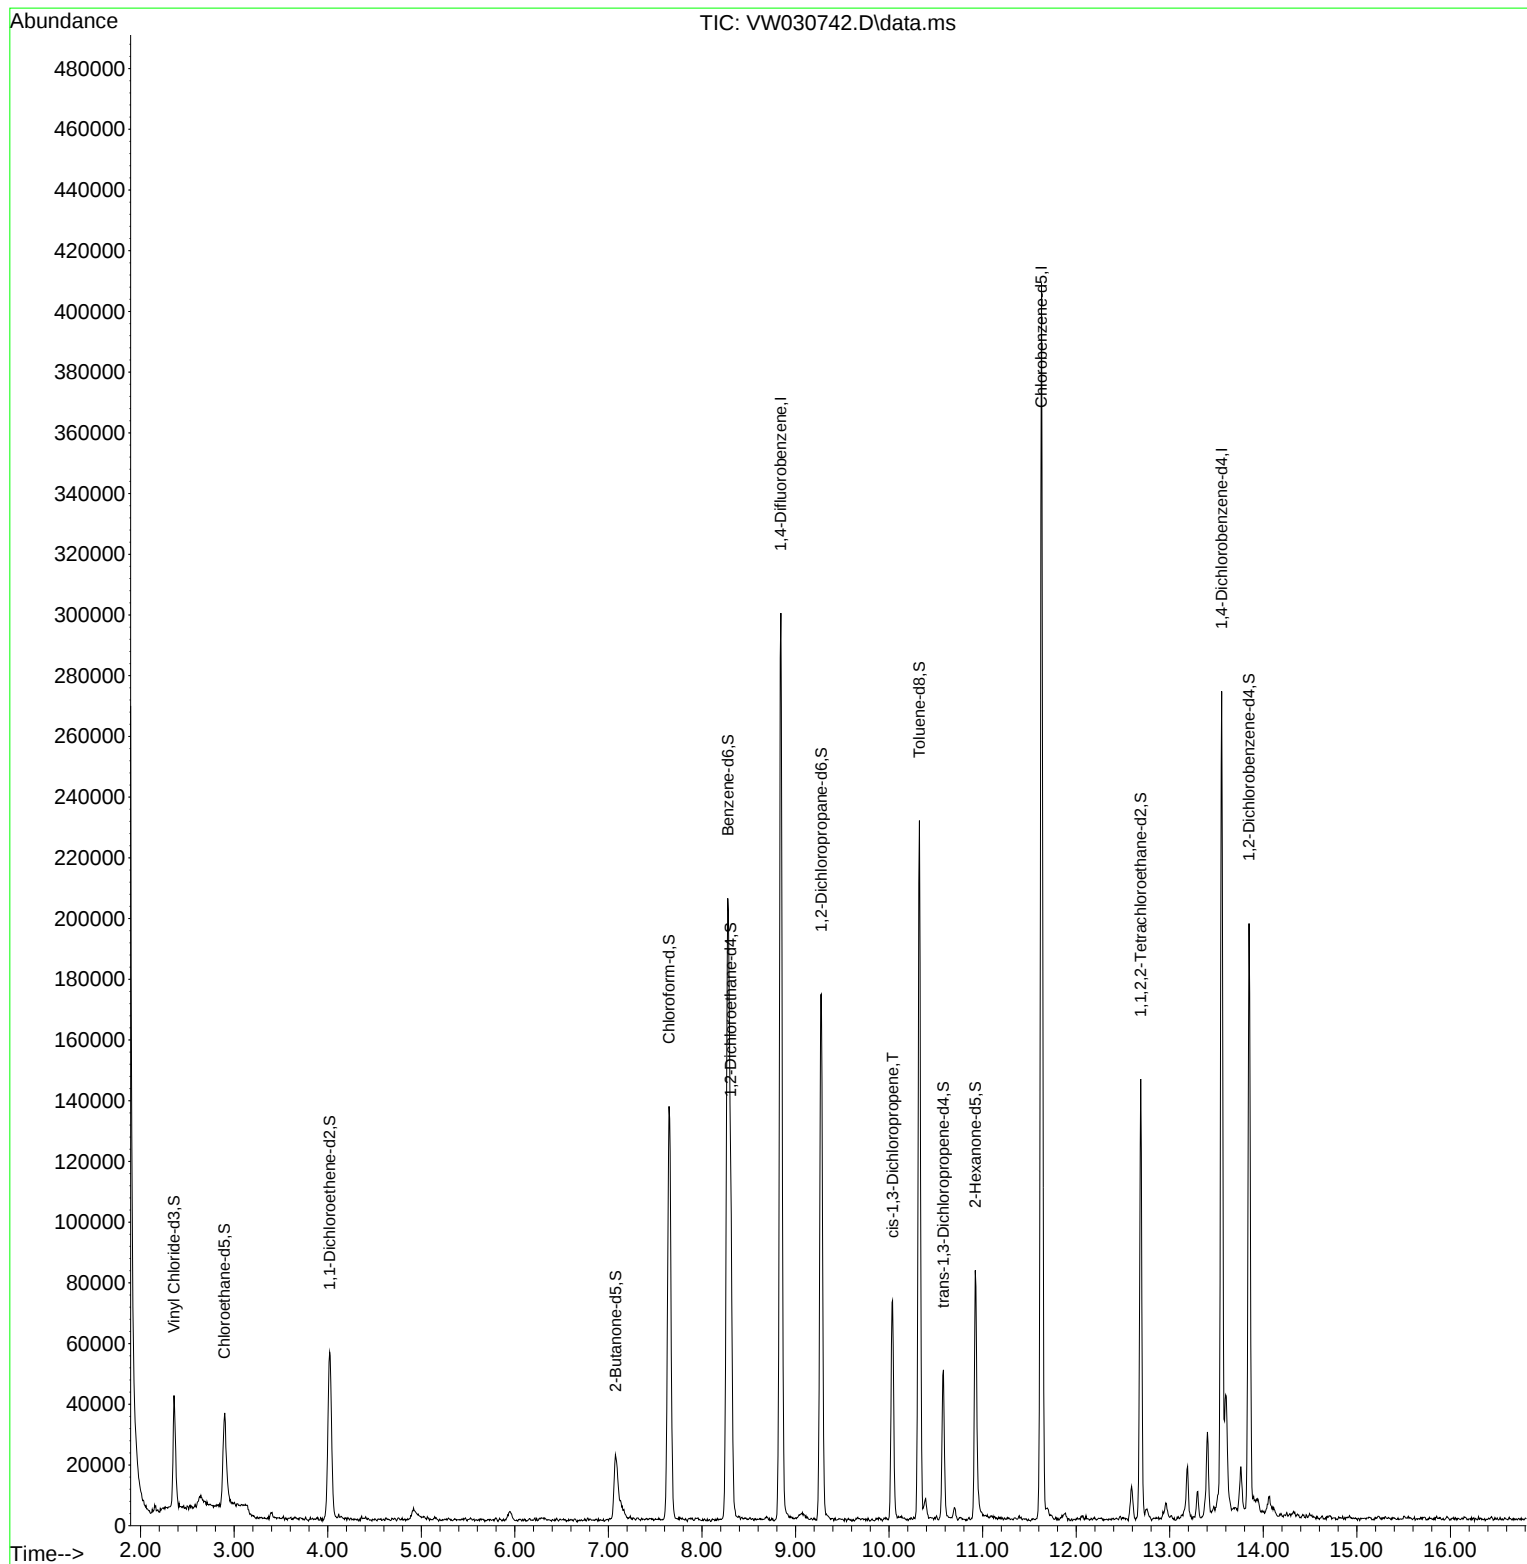

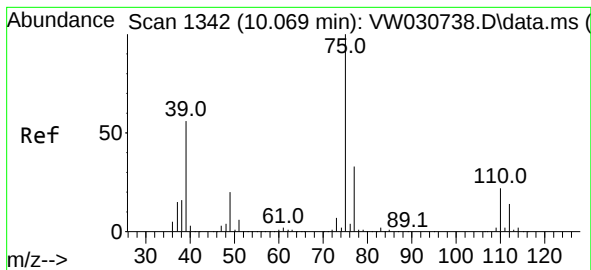

#39
 cis-1,3-Dichloropropene
 Concen: 0.457 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW030742.D
 Acq: 24 Oct 2024 13:55

Instrument :
 MSVOA_W
 ClientSampleId :

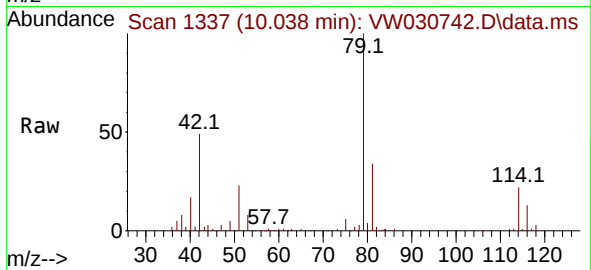

Tgt Ion: 75 Resp: 2283
 Ion Ratio Lower Upper
 75 100
 77 32.1 21.1 39.1

