

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
 Data File : VW030743.D
 Acq On : 24 Oct 2024 14:19
 Operator : SY/MD
 Sample : P4493-05
 Misc : 5.60g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 25 01:44:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 01:42:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	423748	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	344837	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	113094	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	75919	11.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.600%
7) Chloroethane-d5	2.905	69	83396	16.541	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.160%
11) 1,1-Dichloroethene-d2	4.027	65	32300	11.659	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.640%
21) 2-Butanone-d5	7.075	46	47560	39.677	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.360%
24) Chloroform-d	7.654	84	252220	20.813	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.240%
26) 1,2-Dichloroethane-d4	8.307	65	125908	19.981	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.920%
32) Benzene-d6	8.276	84	368963	18.435	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.720%
36) 1,2-Dichloropropane-d6	9.276	67	139191	23.695	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.760%
41) Toluene-d8	10.325	98	285335	15.617	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	62.480%
43) trans-1,3-Dichloroprop...	10.581	79	45629	18.550	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.200%
47) 2-Hexanone-d5	10.922	63	35981	47.555	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	104135	24.138	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.560%
66) 1,2-Dichlorobenzene-d4	13.855	152	93378	24.402	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.600%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3825	0.452	ug/L	Qvalue # 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
Data File : VW030743.D
Acq On : 24 Oct 2024 14:19
Operator : SY/MD
Sample : P4493-05
Misc : 5.60g/10mL/MSVOA_W/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 25 01:44:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 01:42:56 2024
Response via : Initial Calibration

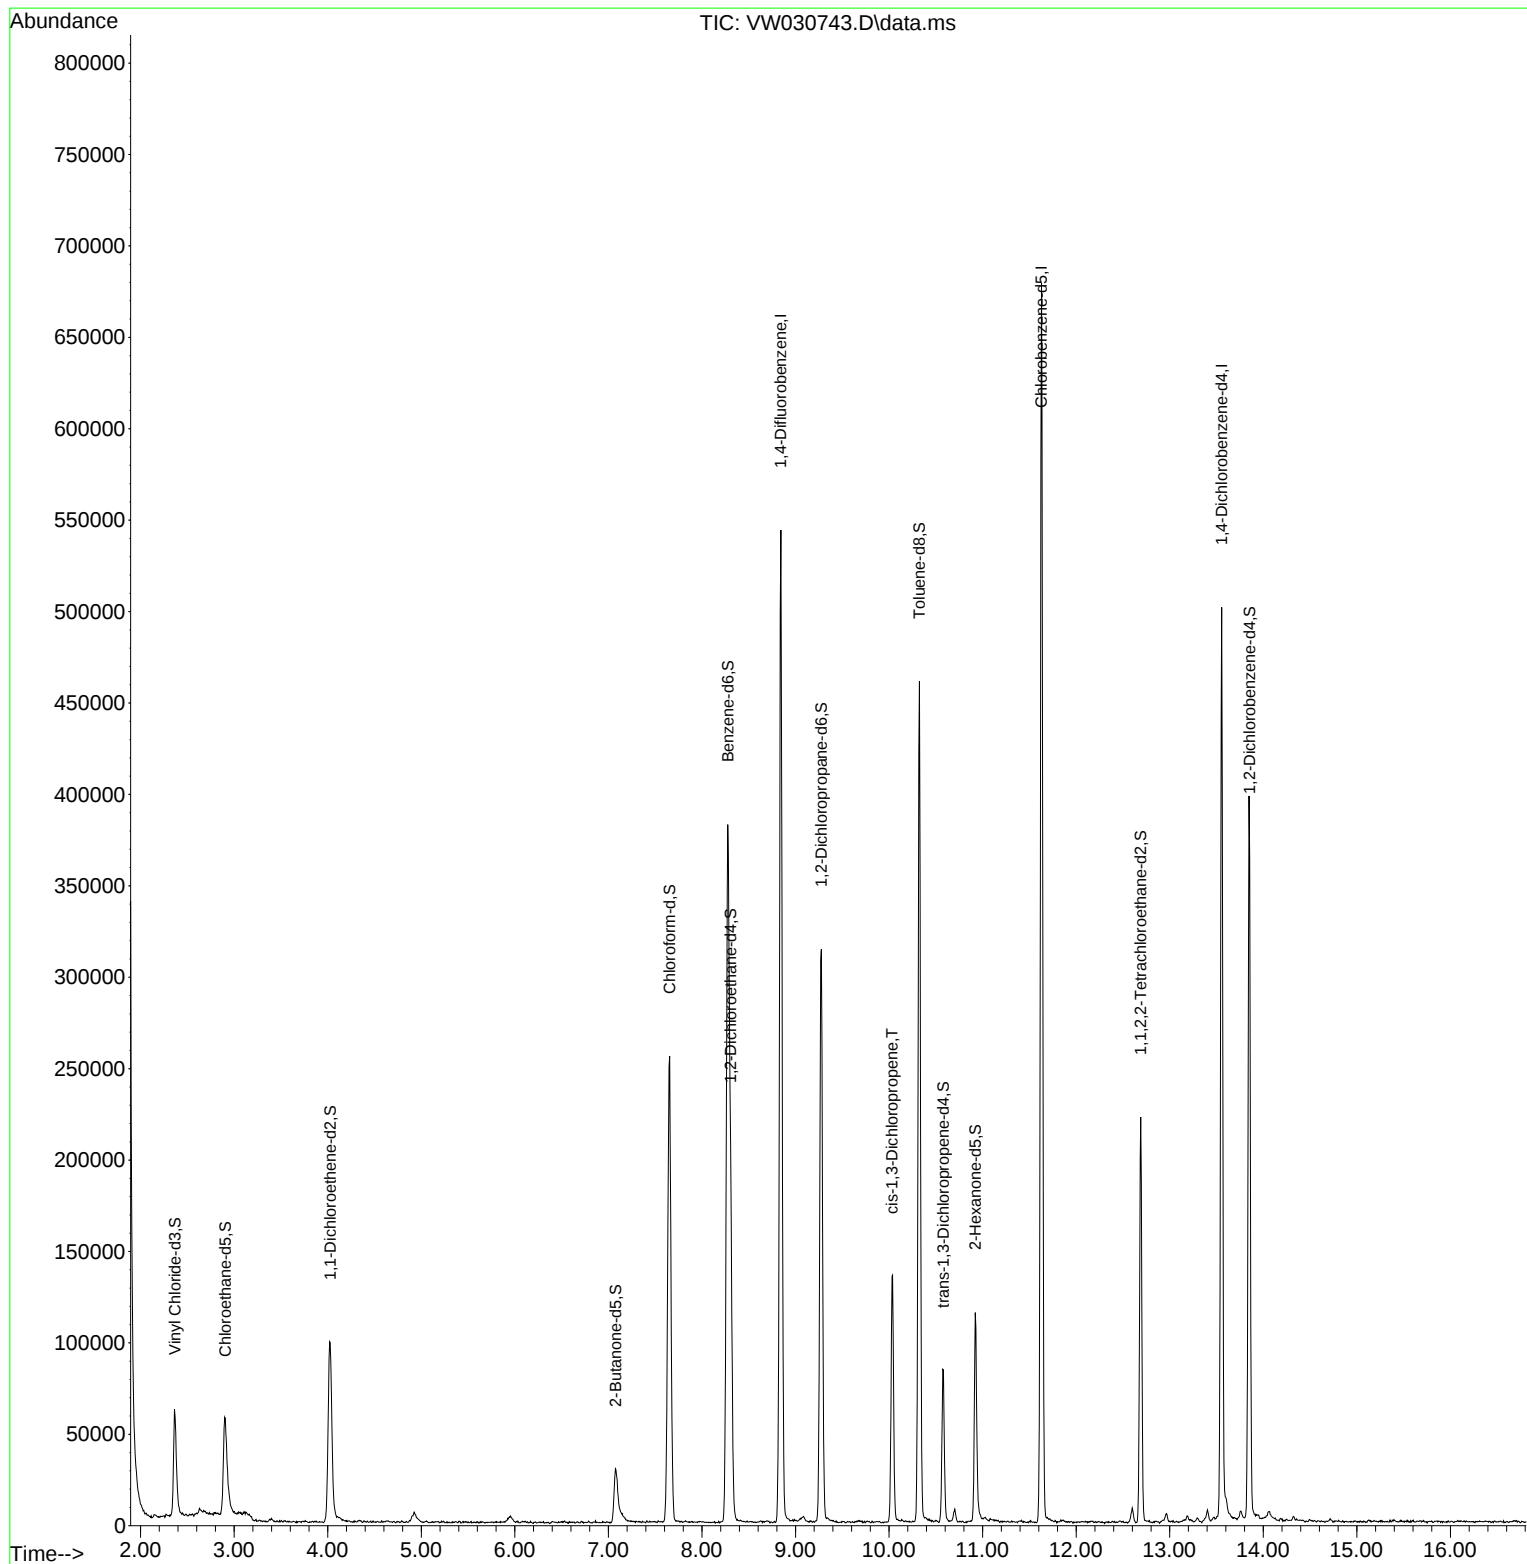

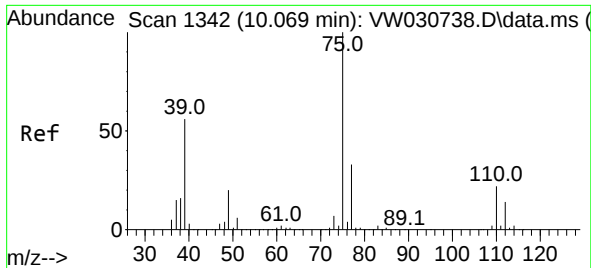

#39
 cis-1,3-Dichloropropene
 Concen: 0.452 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030743.D
 Acq: 24 Oct 2024 14:19

Instrument :
 MSVOA_W
 ClientSampleId :

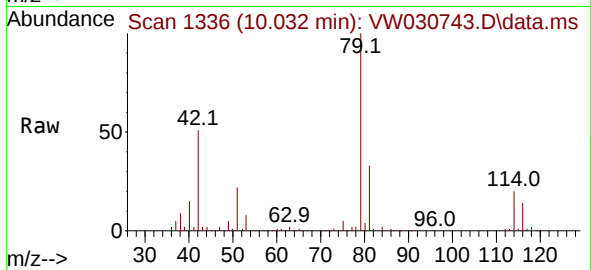

Tgt Ion: 75 Resp: 3825
 Ion Ratio Lower Upper
 75 100
 77 45.0 21.1 39.1#

