

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
 Data File : VW030744.D
 Acq On : 24 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4492-03
 Misc : 4.64g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 25 01:44:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 25 01:42:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	399168	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	315970	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	98934	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	66211	10.553	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.200%
7) Chloroethane-d5	2.905	69	72070	15.175	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.680%
11) 1,1-Dichloroethene-d2	4.027	65	28052	10.749	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.000%#
21) 2-Butanone-d5	7.075	46	48395	42.860	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.720%
24) Chloroform-d	7.648	84	222724	19.511	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.040%
26) 1,2-Dichloroethane-d4	8.307	65	114599	19.306	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	77.240%
32) Benzene-d6	8.276	84	328565	17.916	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.680%
36) 1,2-Dichloropropane-d6	9.276	67	124117	23.059	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.240%
41) Toluene-d8	10.325	98	246020	14.695	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	58.800%
43) trans-1,3-Dichloroprop...	10.575	79	39982	17.739	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.960%
47) 2-Hexanone-d5	10.922	63	36992	53.358	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91436	23.131	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.520%
66) 1,2-Dichlorobenzene-d4	13.855	152	75511	22.557	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.240%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	6112	3.029	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102424\
Data File : VW030744.D
Acq On : 24 Oct 2024 15:06
Operator : SY/MD
Sample : P4492-03
Misc : 4.64g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 25 01:44:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 25 01:42:56 2024
Response via : Initial Calibration

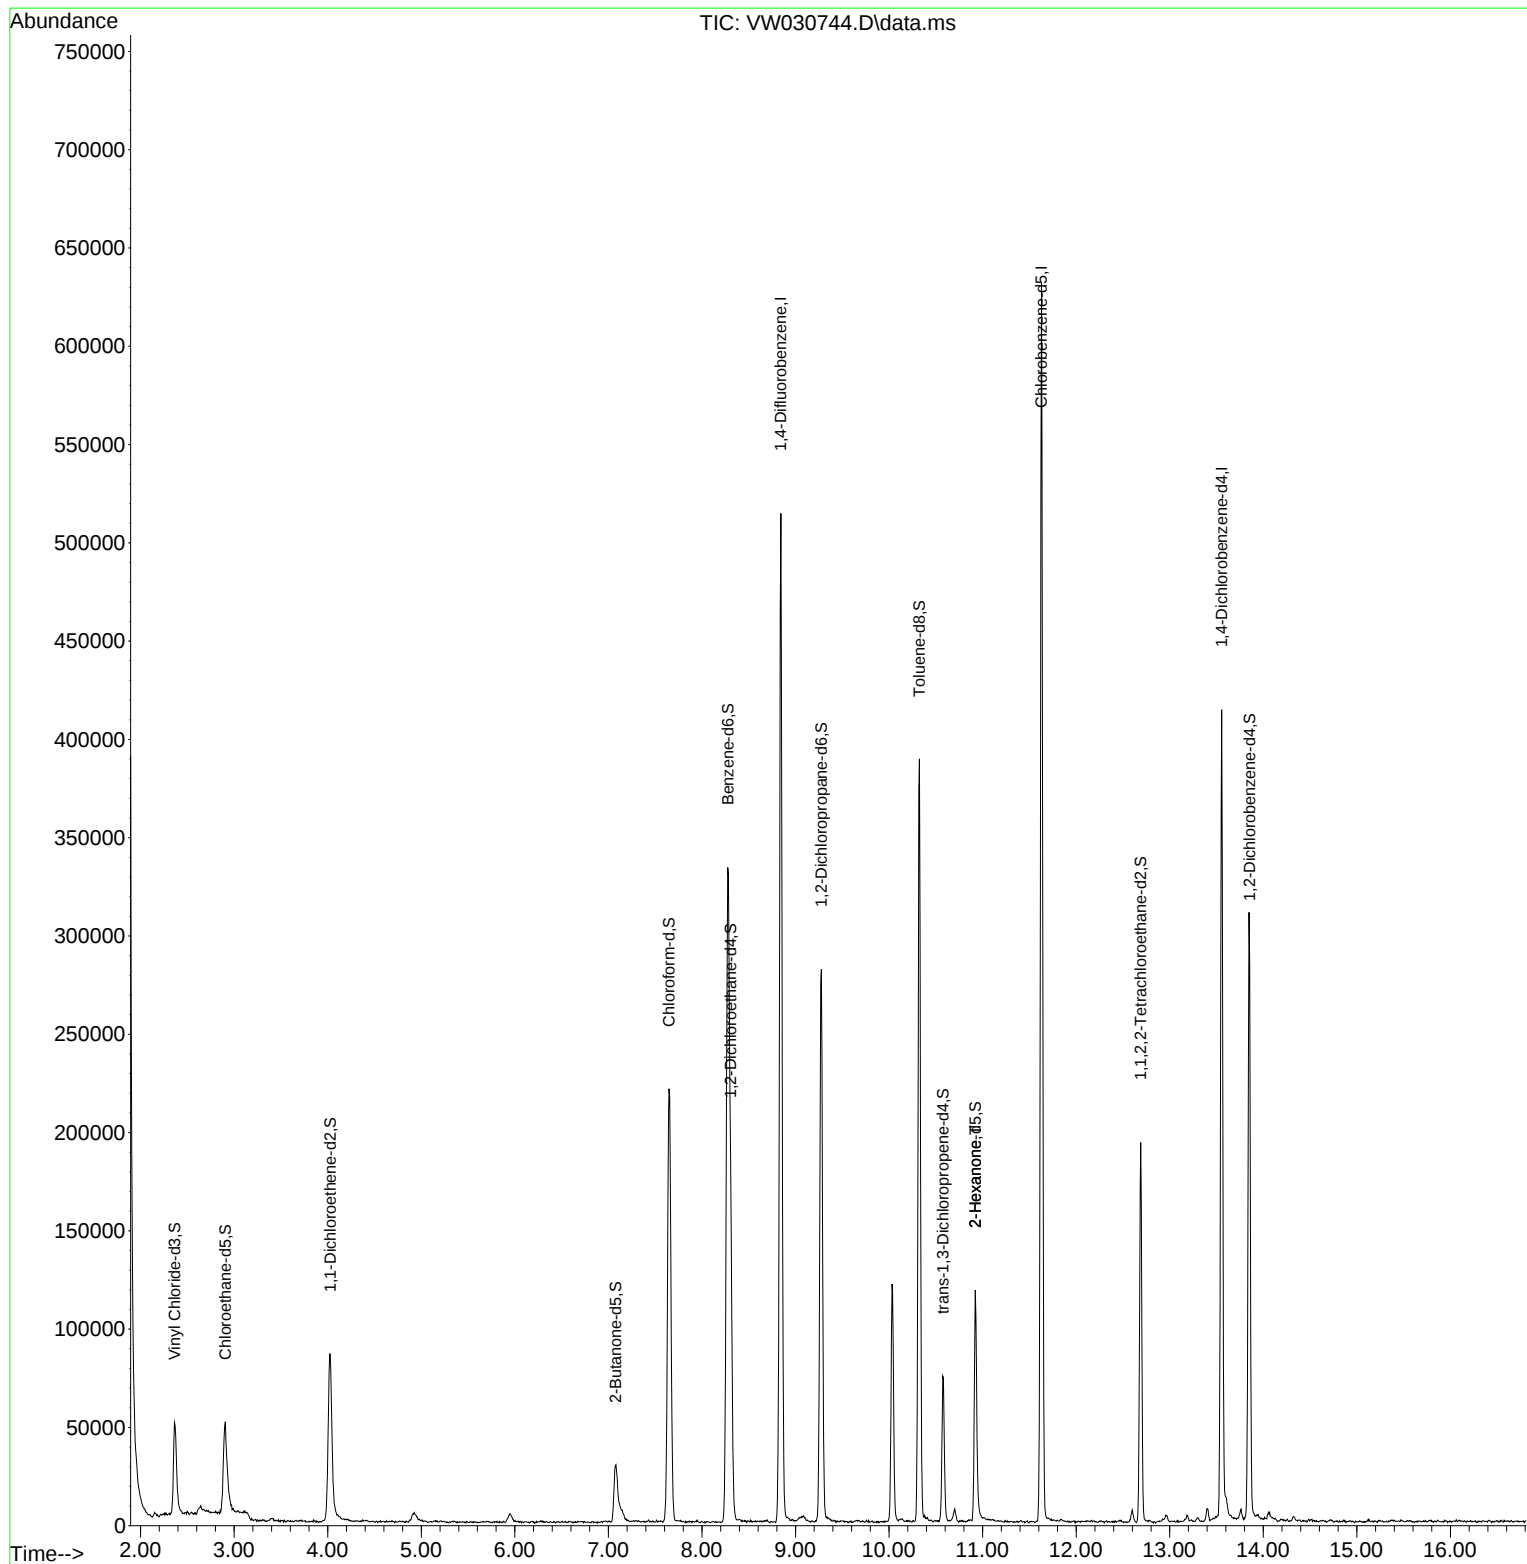

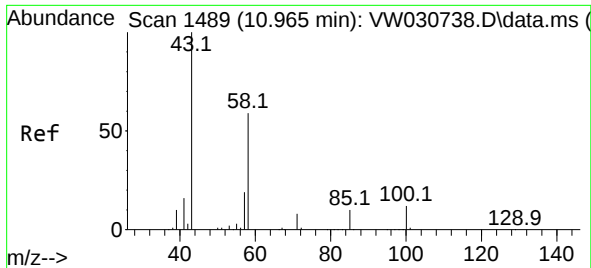

#48
 2-Hexanone
 Concen: 3.029 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW030744.D
 Acq: 24 Oct 2024 15:06

Instrument :
 MSVOA_W
 ClientSampleId :

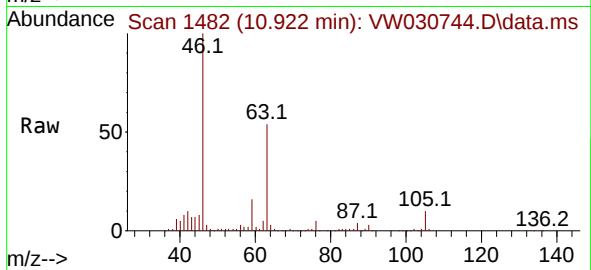

Tgt Ion: 43	Resp: 6112
Ion Ratio	Lower Upper
43	100
58	28.6 44.6 67.0#
57	0.0 15.8 23.8#
100	1.4 10.2 15.2#

