


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102621\
Data File : VW020692.D
Acq On : 26 Oct 2021 09:24
Operator : SY/VA
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W102221S.M
Title : SW846 8260
Last Update : Sat Oct 23 05:58:59 2021

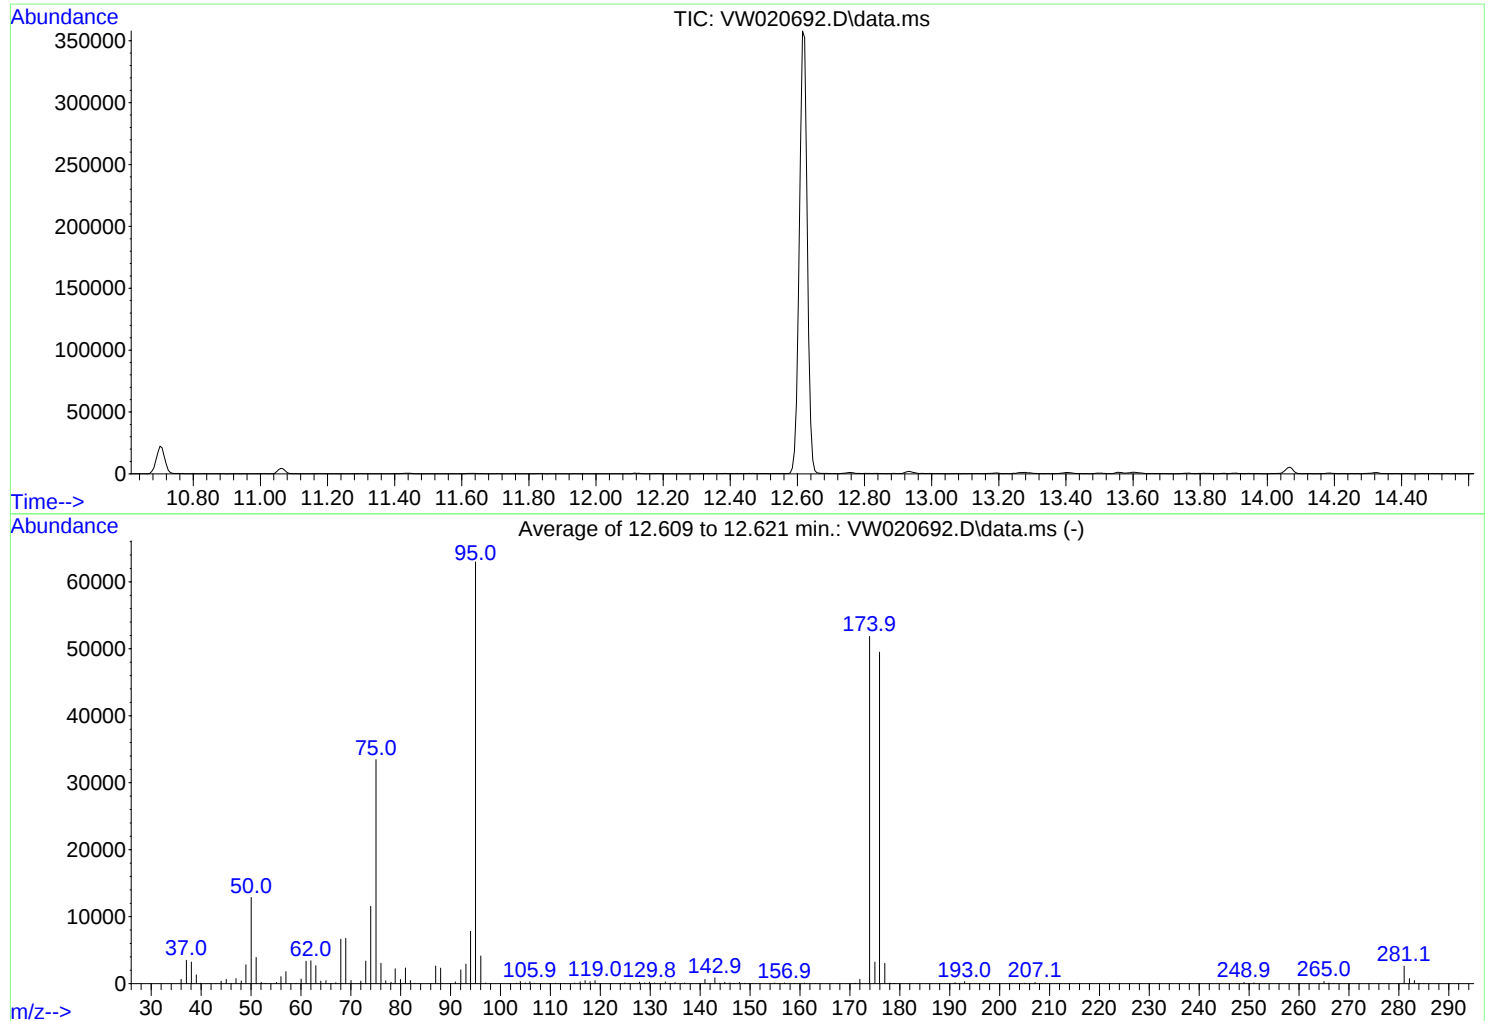

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	12870	PASS
75	95	30	60	53.1	33451	PASS
95	95	100	100	100.0	62989	PASS
96	95	5	9	6.6	4145	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.3	51851	PASS
175	174	5	9	6.2	3236	PASS
176	174	95	101	95.5	49509	PASS
177	176	5	9	6.1	3042	PASS