

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
 Data File : VW024985.D
 Acq On : 26 Oct 2022 14:22
 Operator : SY/VA
 Sample : VW1026SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK432

Quant Time: Oct 27 04:49:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 04:48:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	350702	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	317519	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	151198	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	101383	25.756	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.040%
7) Chloroethane-d5	2.891	69	57957	25.134	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.520%
11) 1,1-Dichloroethene-d2	4.019	63	196746	20.065	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.240%
21) 2-Butanone-d5	7.080	46	71994	54.191	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.380%
24) Chloroform-d	7.647	84	277436	26.067	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.280%
26) 1,2-Dichloroethane-d4	8.305	65	158022	26.524	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.080%
32) Benzene-d6	8.275	84	560801	27.556	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.240%
36) 1,2-Dichloropropane-d6	9.274	67	163592	27.434	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.720%
41) Toluene-d8	10.323	98	512023	27.023	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.080%
43) trans-1,3-Dichloroprop...	10.579	79	71561	27.063	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	108.240%
47) 2-Hexanone-d5	10.921	63	58823	57.104	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.200%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	130288	27.363	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	155876	26.827	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.320%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	11301	2.233	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
Data File : VW024985.D
Acq On : 26 Oct 2022 14:22
Operator : SY/VA
Sample : VW1026SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK432

Quant Time: Oct 27 04:49:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 04:48:47 2022
Response via : Initial Calibration

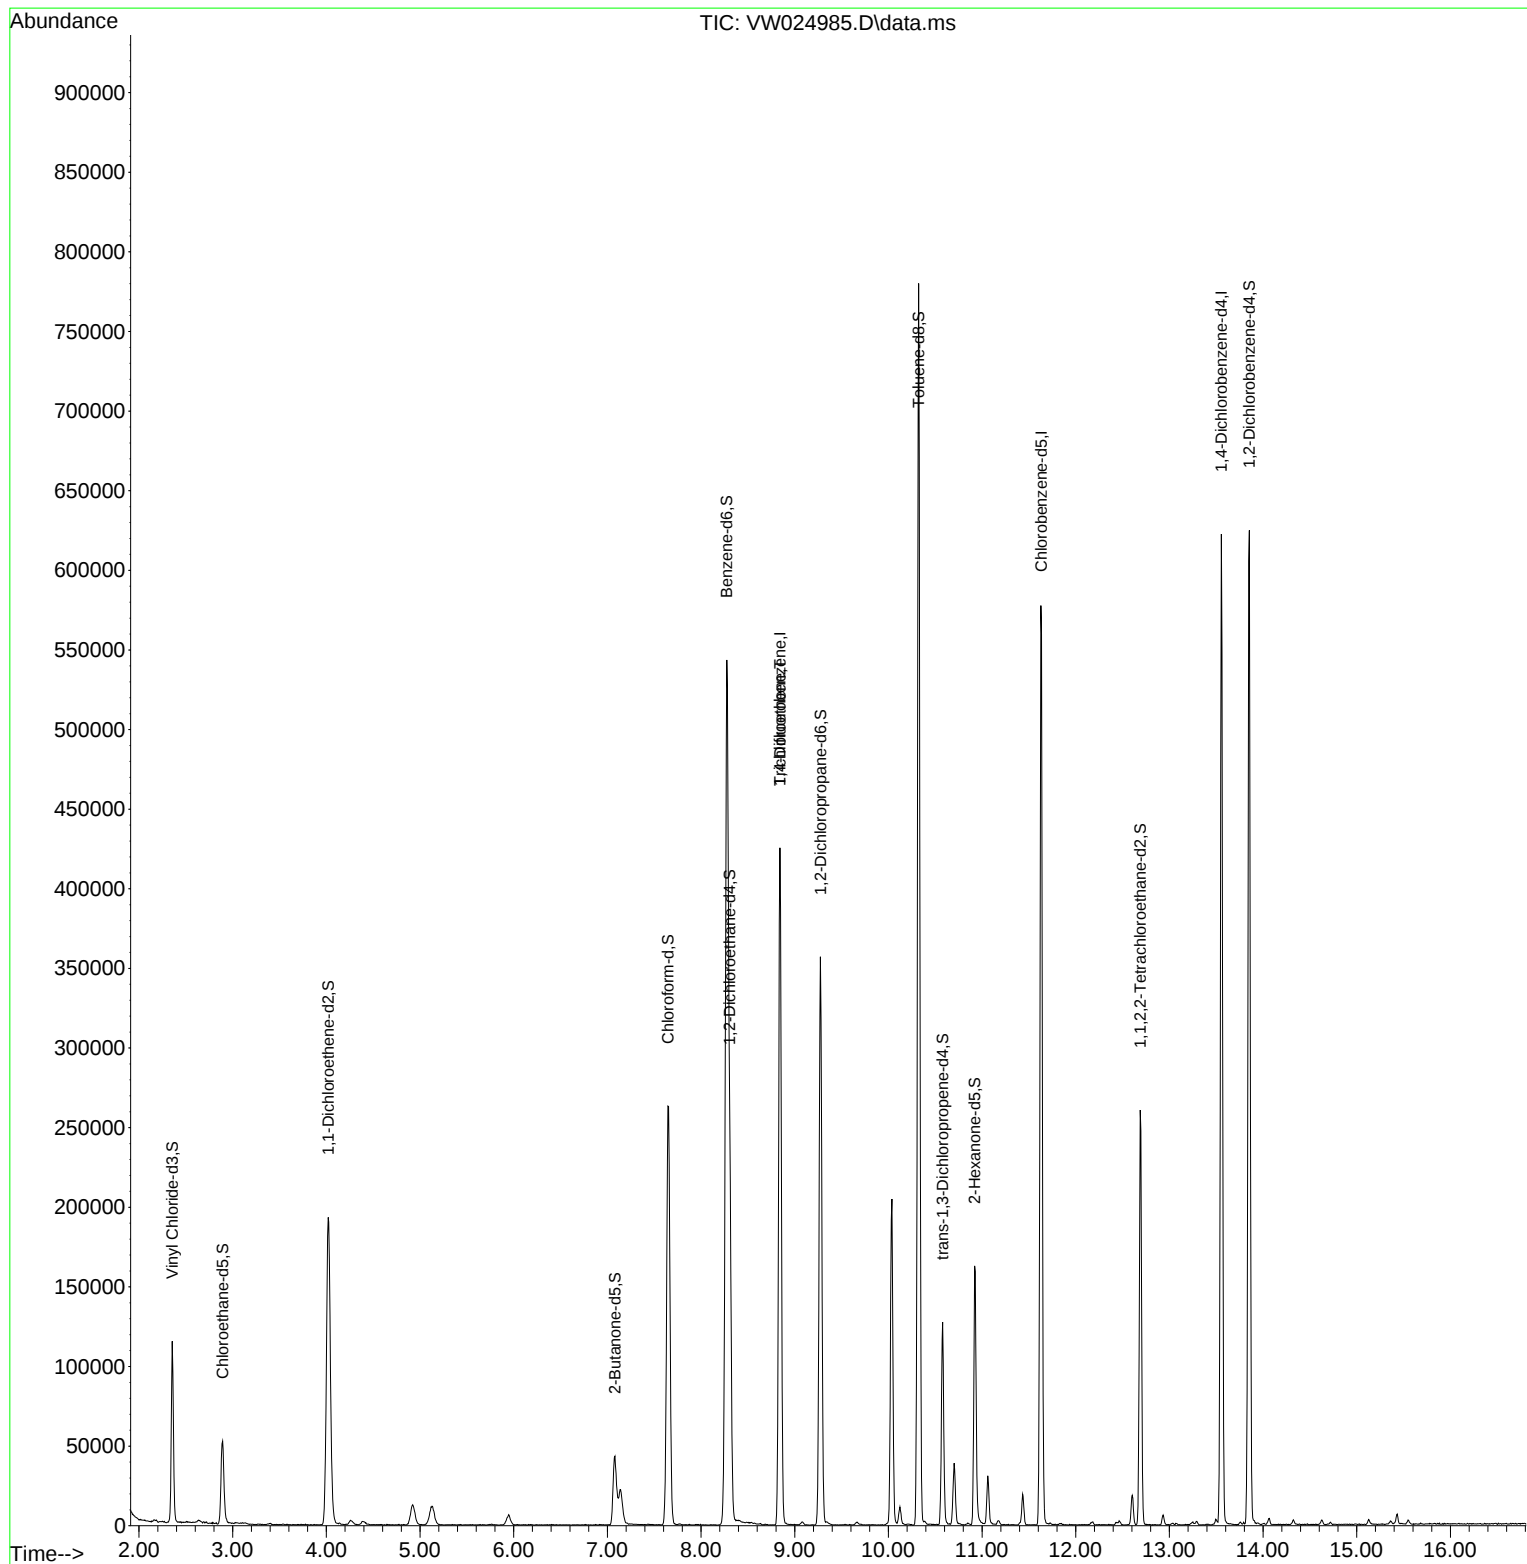

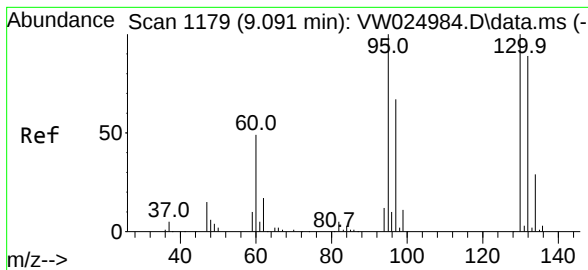

#34

Trichloroethene

Concen: 2.233 ug/L

RT: 8.842 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW024985.D


Acq: 26 Oct 2022 14:22

Instrument :

MSVOA_W

ClientSampleId :

VBLK432

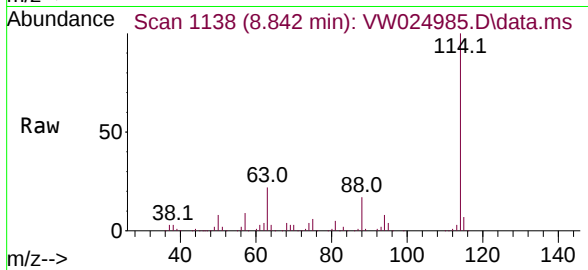

Tgt Ion: 95 Resp: 11301

Ion Ratio Lower Upper

95 100

97 0.0 44.7 83.1#

132 0.0 62.6 116.2#

130 0.0 69.1 128.3#

