

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
 Data File : VW024989.D
 Acq On : 26 Oct 2022 15:59
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK572

Quant Time: Oct 27 04:50:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 04:48:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	338286	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	309973	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	146122	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	85716	22.575	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.280%		
7) Chloroethane-d5	2.885	69	47343	21.285	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.120%		
11) 1,1-Dichloroethene-d2	4.019	63	160658	16.986	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.960%		
21) 2-Butanone-d5	7.080	46	60927	47.544	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.080%		
24) Chloroform-d	7.653	84	242222	23.594	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.360%		
26) 1,2-Dichloroethane-d4	8.305	65	137557	23.936	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.760%		
32) Benzene-d6	8.275	84	488457	24.585	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	98.360%		
36) 1,2-Dichloropropane-d6	9.274	67	143810	24.703	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.800%		
41) Toluene-d8	10.323	98	448957	24.272	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	97.080%		
43) trans-1,3-Dichloroprop...	10.579	79	60364	23.385	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	93.520%		
47) 2-Hexanone-d5	10.921	63	48011	47.743	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.480%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	110672	23.809	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.240%		
66) 1,2-Dichlorobenzene-d4	13.853	152	139118	24.774	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.080%		
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	11103	2.247	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
Data File : VW024989.D
Acq On : 26 Oct 2022 15:59
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK572

Quant Time: Oct 27 04:50:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 04:48:47 2022
Response via : Initial Calibration

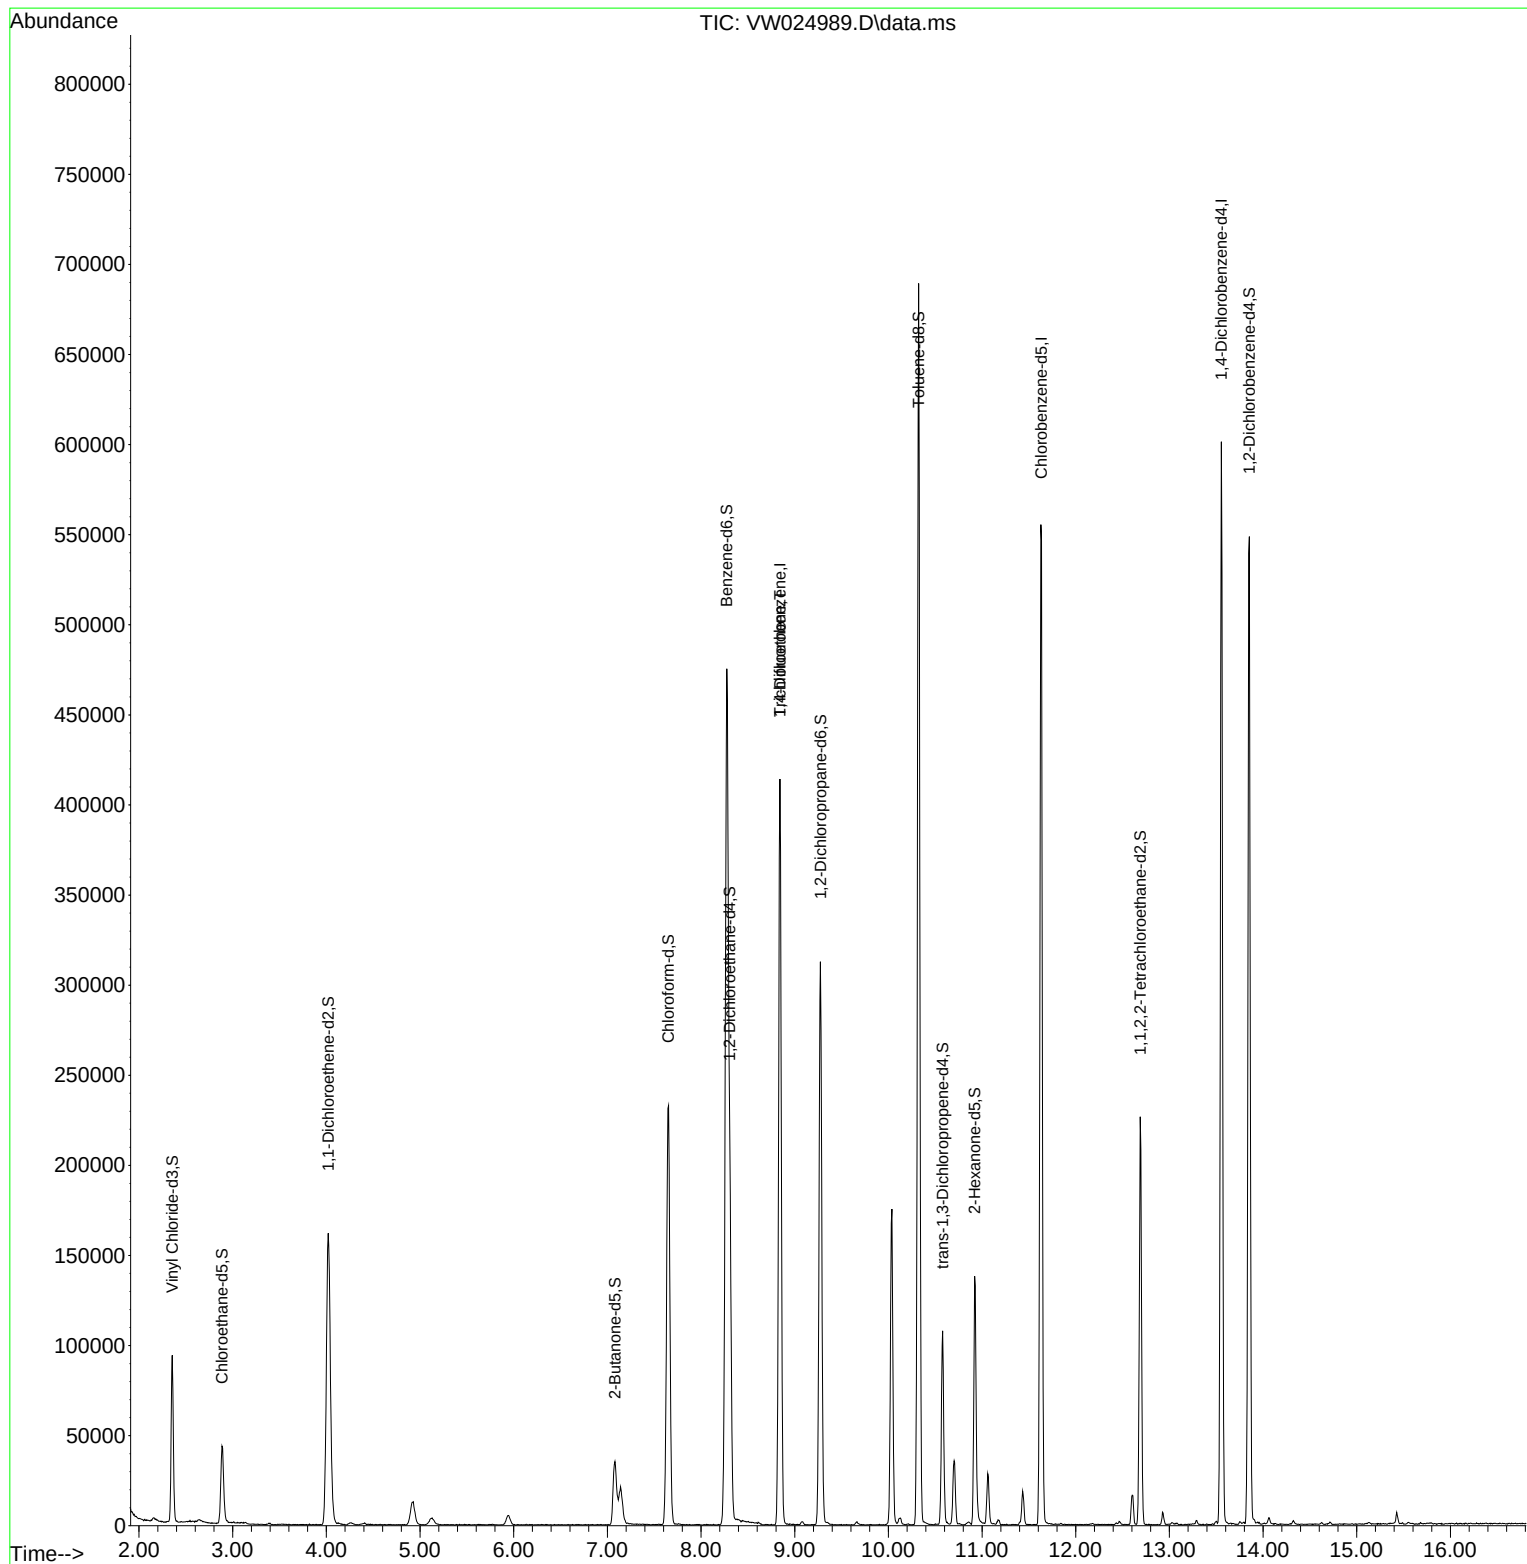

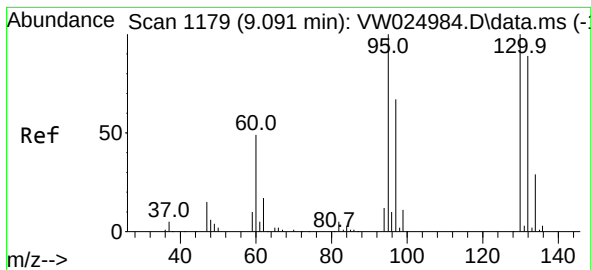

#34

Trichloroethene

Concen: 2.247 ug/L

RT: 8.842 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW024989.D


Acq: 26 Oct 2022 15:59

Instrument :

MSVOA_W

ClientSampleId :

VIBLK572

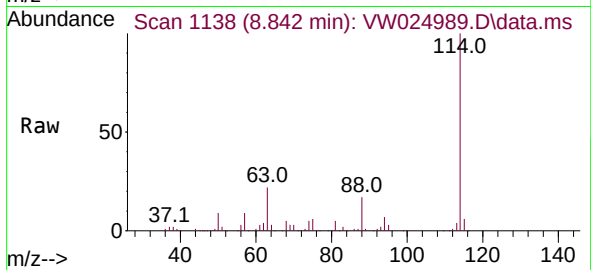

Tgt Ion: 95 Resp: 11103

Ion Ratio Lower Upper

95 100

97 0.0 44.7 83.1#

132 0.0 62.6 116.2#

130 0.0 69.1 128.3#

