
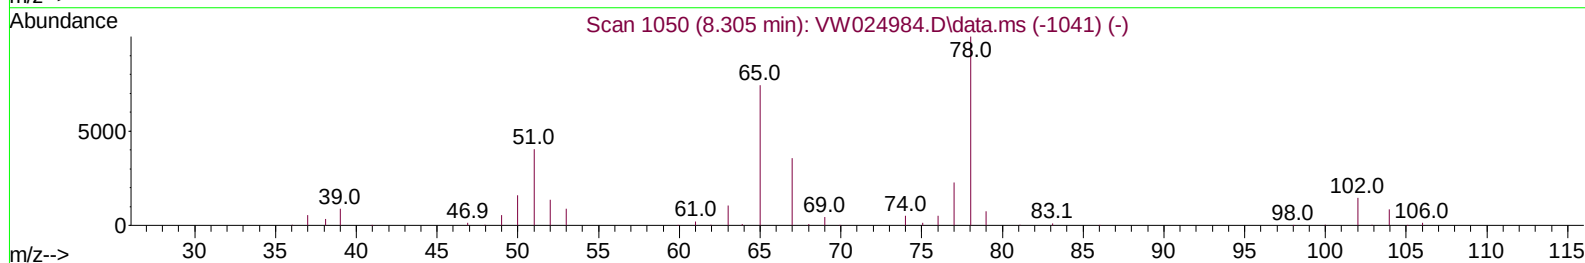
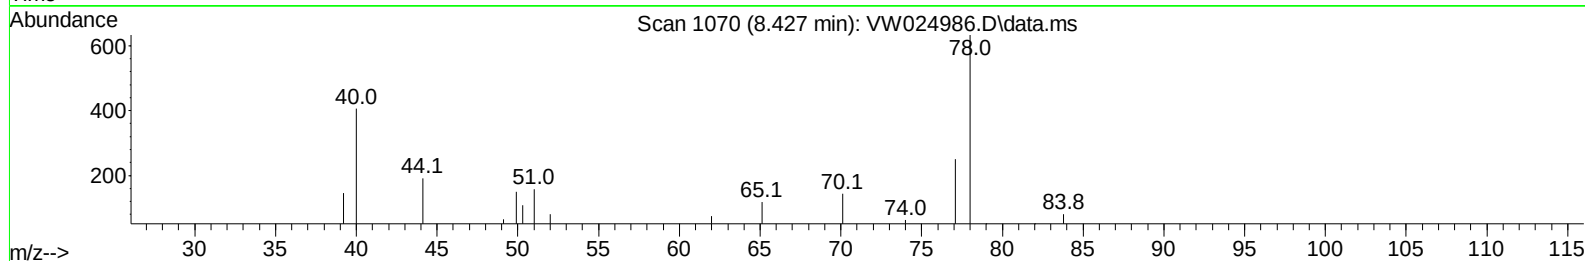


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
Data File : VW024986.D
Acq On : 26 Oct 2022 14:46
Operator : SY/VA
Sample : N5258-07RE
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 04:49:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 04:48:47 2022
Response via : Initial Calibration

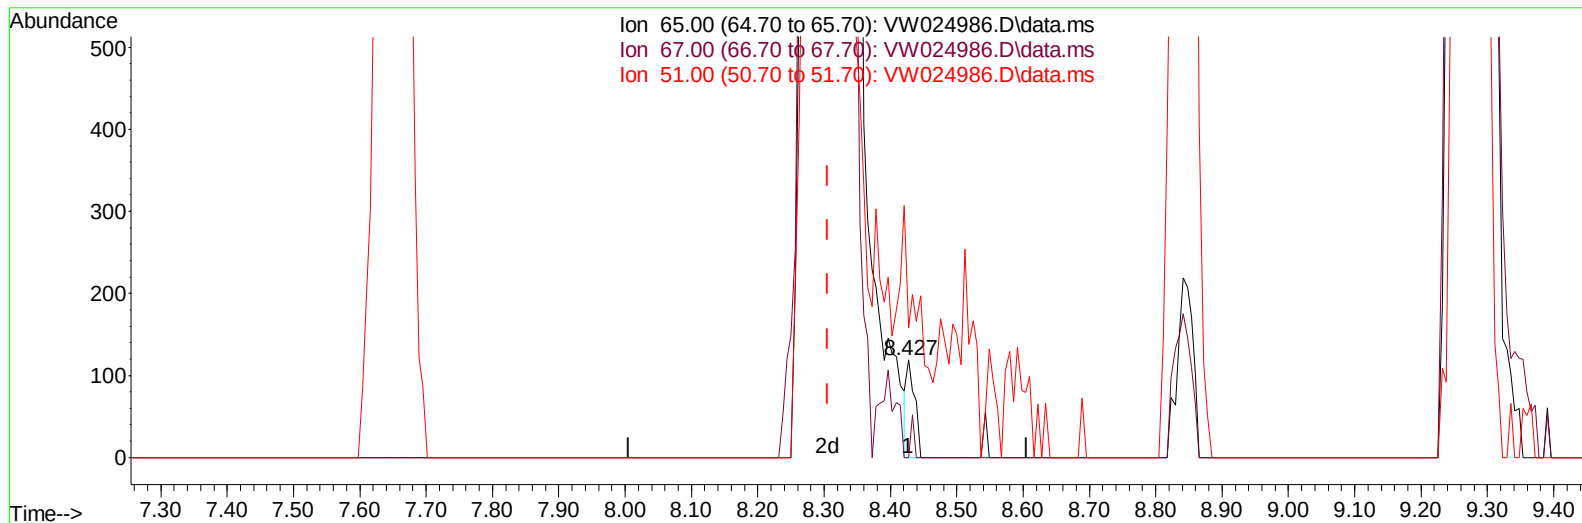

TIC: VW024986.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)


8.427min (+ 0.122) 0.02 ug/L

response 98

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.00	48.98
51.00	84.80	108.16
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
Data File : VW024986.D
Acq On : 26 Oct 2022 14:46
Operator : SY/VA
Sample : N5258-07RE
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 04:49:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 04:48:47 2022
Response via : Initial Calibration

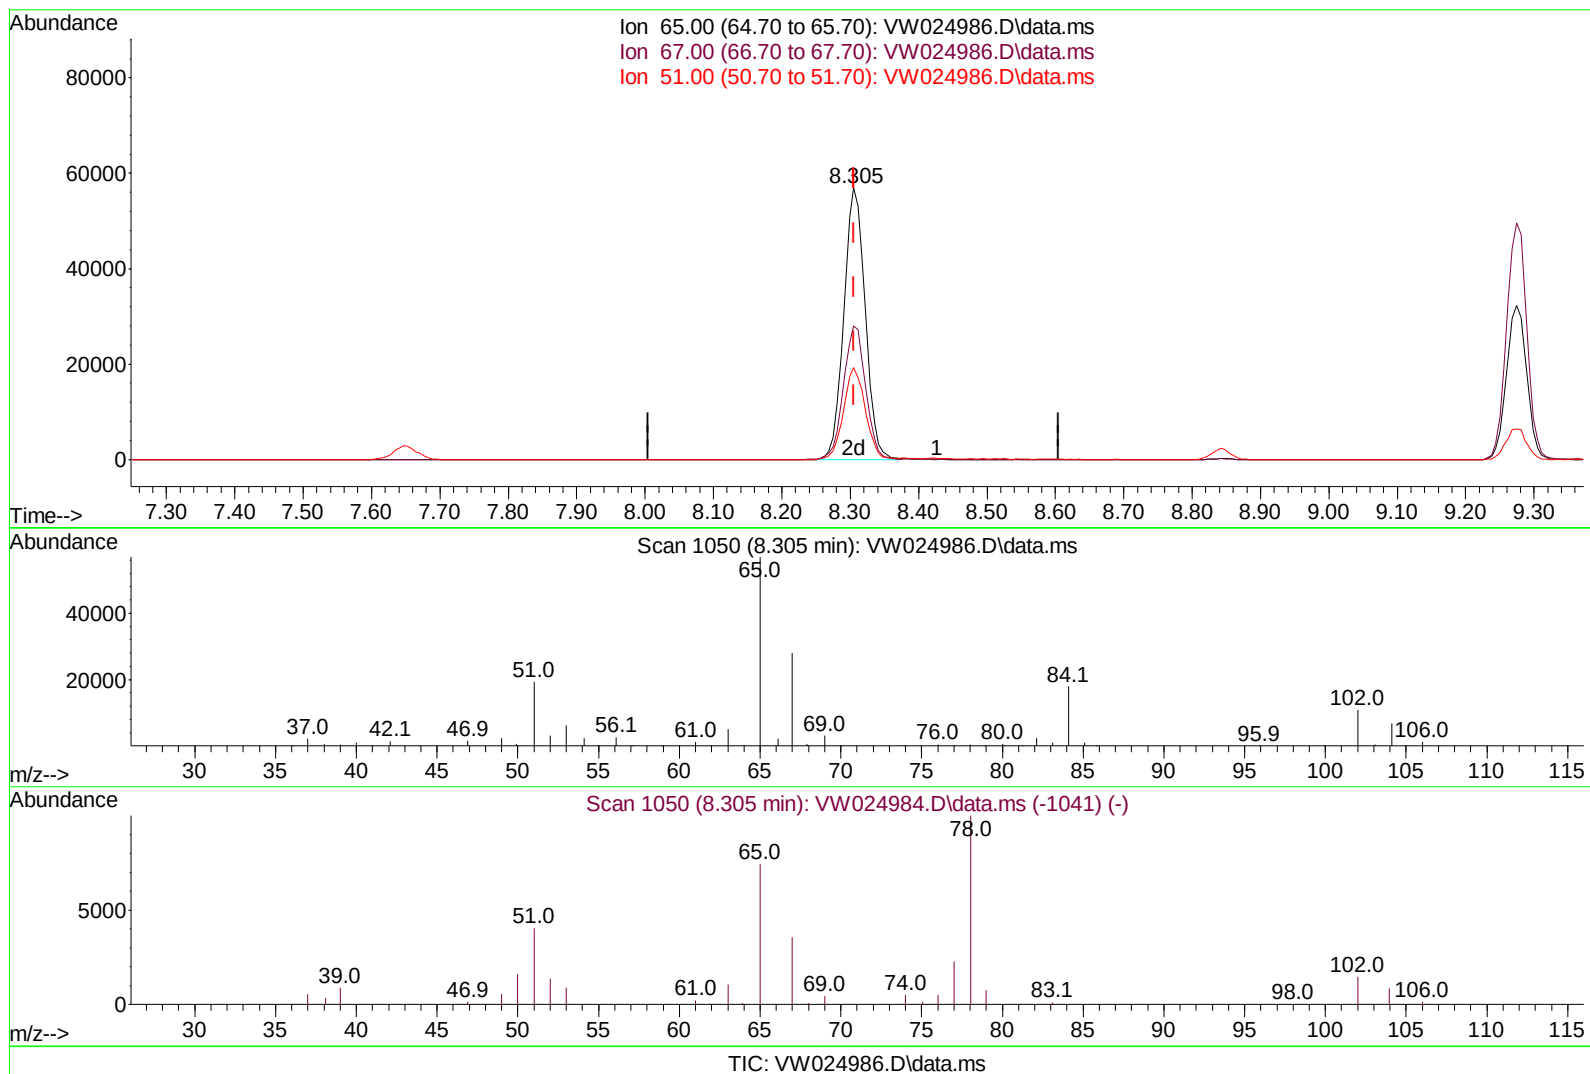

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 31.15 ug/L m

response 123509

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.00	0.04#
51.00	84.80	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw102622\
 Data File : VW024986.D
 Acq On : 26 Oct 2022 14:46
 Operator : SY/VA
 Sample : N5258-07RE
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 04:49:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 27 04:48:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	233383	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	112371	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	20886	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	57054	21.780	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.120%	
7) Chloroethane-d5	2.885	69	36242	23.618	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.480%	
11) 1,1-Dichloroethene-d2	4.019	63	92125	14.118	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	56.480%	
21) 2-Butanone-d5	7.074	46	112561	127.317	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	254.640%#	
24) Chloroform-d	7.653	84	177736	25.094	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	100.360%	
26) 1,2-Dichloroethane-d4	8.305	65	123509m	31.152	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	124.600%	
32) Benzene-d6	8.275	84	304842	42.324	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	169.280%#	
36) 1,2-Dichloropropane-d6	9.274	67	100885	47.804	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	191.200%#	
41) Toluene-d8	10.323	98	171508	25.577	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	102.320%	
43) trans-1,3-Dichloroprop...	10.579	79	33800	36.119	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	144.480%#	
47) 2-Hexanone-d5	10.920	63	75596	207.366	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	414.740%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98856	58.666	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	234.680%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	18890	23.535	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	94.120%	
Target Compounds						
13) Acetone	4.129	43	11286	17.969	ug/L	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
Data File : VW024986.D
Acq On : 26 Oct 2022 14:46
Operator : SY/VA
Sample : N5258-07RE
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 04:49:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 27 04:48:47 2022
Response via : Initial Calibration

