
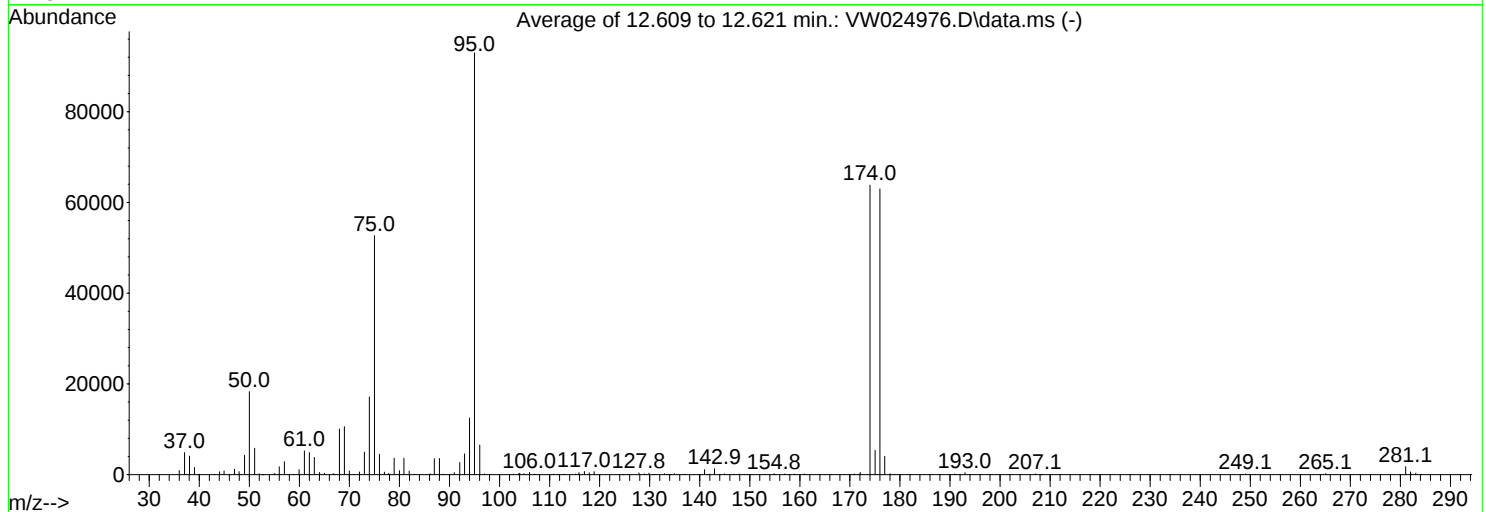


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102622\
Data File : VW024976.D
Acq On : 26 Oct 2022 08:34
Operator : SY/VA
Sample : BFB447
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB447

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Title : SFAM01.0
Last Update : Thu Oct 27 23:51:01 2022

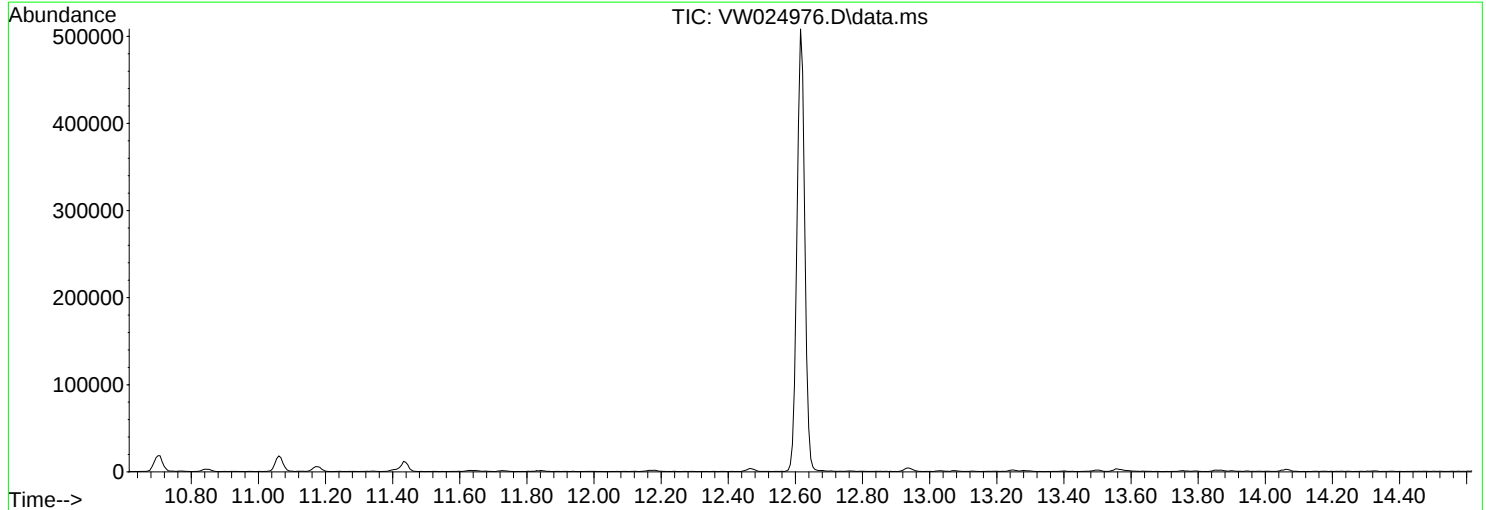

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	18291	PASS
75	95	30	80	56.7	52685	PASS
95	95	100	100	100.0	92971	PASS
96	95	5	9	7.0	6508	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.7	63829	PASS
175	174	5	9	8.4	5348	PASS
176	174	95	105	98.7	62981	PASS
177	176	5	10	6.4	4008	PASS

Scan 1749 (12.567 min): VW024976.D\data.ms
BFB447

m/z	Abundance
39.90	300.0
44.20	68.0
280.90	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	793.0
37.00	5023.0
38.10	3980.0
39.00	1717.0
40.00	454.0
44.10	927.0
44.90	838.0
46.20	140.0
47.00	1051.0
48.00	804.0
49.00	3993.0
50.00	17064.0
51.00	6199.0
52.00	164.0
52.70	58.0
55.10	332.0
56.00	1708.0
57.00	2645.0
57.90	121.0
58.90	98.0
60.00	1166.0
61.00	5173.0
62.00	3993.0
63.00	3271.0
64.00	470.0
65.10	312.0
66.80	261.0
68.00	9050.0
69.00	10187.0
70.00	739.0
71.00	85.0
71.90	588.0
73.00	4869.0
74.00	15224.0
75.00	48472.0
76.00	3956.0
77.00	513.0
78.90	3508.0
80.00	721.0
80.90	3124.0
81.90	831.0
83.00	143.0
86.10	170.0
87.00	3305.0
88.00	3119.0
90.90	393.0
92.10	2374.0
93.00	3730.0
94.00	10955.0
95.00	82088.0
96.00	5891.0
97.00	228.0
102.70	59.0
104.10	398.0
104.90	196.0
106.00	427.0
107.00	124.0
110.00	63.0
110.80	131.0
111.80	135.0
112.90	89.0
115.10	113.0
115.80	371.0
116.90	576.0
117.90	334.0
118.90	569.0
124.70	58.0
125.60	93.0
127.80	381.0
128.90	169.0
129.90	273.0
130.90	106.0
133.00	329.0
135.00	164.0
136.80	161.0
138.80	77.0
139.70	55.0
141.00	941.0
141.70	128.0
143.00	966.0
144.10	67.0
145.00	189.0
146.10	127.0
146.90	114.0
147.80	213.0
148.90	68.0
149.60	69.0
149.90	61.0
152.80	75.0
154.80	156.0
155.10	154.0
157.00	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

161.00	133.0
165.00	134.0
170.70	66.0
171.80	283.0
172.10	294.0
174.00	52032.0
175.00	4631.0
176.00	46360.0
177.00	3564.0
178.00	129.0
178.90	81.0
191.00	264.0
191.90	77.0
193.10	609.0
194.00	79.0
195.00	66.0
207.10	337.0
249.10	247.0
249.80	107.0
251.00	141.0
265.00	275.0
265.90	59.0
281.10	2583.0
282.00	960.0
283.10	387.0
284.30	120.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	1094.0
37.10	5316.0
38.00	4966.0
39.00	1701.0
40.00	377.0
43.00	101.0
44.00	591.0
44.90	922.0
46.00	111.0
47.10	1169.0
47.90	550.0
49.10	4843.0
50.00	20936.0
51.10	5755.0
52.00	244.0
55.00	277.0
56.00	1723.0
57.00	3184.0
58.10	142.0
58.90	79.0
60.00	1114.0
61.00	6008.0
62.00	5703.0
63.00	4422.0
64.10	512.0
64.90	361.0
66.80	381.0
68.00	11674.0
69.00	11446.0
70.00	950.0
70.90	109.0
72.00	685.0
73.00	5608.0
74.00	19560.0
75.00	59784.0
76.00	4881.0
77.00	659.0
77.90	466.0
79.00	3760.0
80.00	890.0
80.90	4082.0
81.90	843.0
82.90	98.0
86.10	253.0
86.90	3843.0
88.00	4036.0
88.70	327.0
90.90	488.0
92.00	3034.0
93.00	5120.0
94.00	14522.0
95.00	103488.0
96.10	6753.0
97.00	203.0
102.80	119.0
103.80	611.0
104.90	235.0
106.00	584.0
106.90	149.0
110.80	87.0
112.00	152.0
112.90	106.0
115.20	141.0
115.80	509.0
117.00	900.0
117.90	541.0
118.90	816.0
123.90	52.0
125.70	65.0
127.90	419.0
128.90	201.0
129.70	349.0
130.60	93.0
131.00	125.0
132.90	238.0
133.80	122.0
134.90	261.0
137.10	202.0
138.90	68.0
140.90	1278.0
141.90	141.0
142.90	1577.0
144.10	72.0
145.00	185.0
145.90	90.0
146.90	85.0
148.00	233.0
149.00	105.0
149.50	56.0
152.90	57.0
154.80	165.0
156.10	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

156.90	241.0
159.00	209.0
160.90	160.0
170.90	200.0
172.00	624.0
174.00	66400.0
175.10	5624.0
176.00	74384.0
177.00	4416.0
178.00	223.0
191.20	107.0
192.10	108.0
193.00	341.0
194.00	72.0
207.00	175.0
249.00	181.0
249.80	75.0
250.90	68.0
265.10	204.0
267.10	73.0
280.00	75.0
281.10	1765.0
282.00	823.0
283.10	342.0
284.20	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

m/z	Abundance
36.00	875.0
37.10	4313.0
38.00	3356.0
39.10	1330.0
40.10	362.0
43.10	86.0
44.00	605.0
45.00	643.0
46.00	84.0
47.10	1425.0
47.90	717.0
49.00	3973.0
50.00	16872.0
51.00	5472.0
51.90	189.0
52.20	166.0
55.20	197.0
56.00	1805.0
57.00	2718.0
58.00	181.0
59.90	1043.0
61.00	4444.0
62.00	4915.0
63.00	3753.0
64.00	465.0
65.00	310.0
67.00	275.0
68.00	9426.0
69.00	10104.0
70.00	743.0
72.10	555.0
73.00	4408.0
74.00	16632.0
75.00	49800.0
76.00	4757.0
77.00	545.0
77.80	381.0
78.90	3663.0
80.00	1076.0
80.90	3704.0
82.00	702.0
82.90	74.0
86.00	91.0
87.00	3474.0
88.00	3530.0
91.00	494.0
92.00	2667.0
93.00	4956.0
94.00	11978.0
95.00	93336.0
96.10	6881.0
97.00	137.0
104.00	526.0
104.90	239.0
106.00	464.0
107.00	51.0
110.00	56.0
110.80	99.0
112.00	105.0
112.90	88.0
115.10	134.0
115.90	465.0
116.90	629.0
117.90	428.0
118.90	667.0
125.70	56.0
127.90	401.0
128.90	153.0
129.90	449.0
130.70	150.0
132.80	90.0
133.40	63.0
134.10	53.0
134.90	177.0
136.90	162.0
138.90	52.0
140.10	73.0
140.90	1092.0
142.00	174.0
142.90	1381.0
144.00	58.0
144.80	120.0
145.70	151.0
146.70	69.0
148.00	226.0
148.80	62.0
150.10	90.0
152.80	93.0
154.90	305.0
157.10	143.0
157.80	65.0
159.00	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447

160.80	177.0
170.90	202.0
172.00	610.0
174.00	73056.0
175.00	5789.0
176.00	68200.0
176.90	4043.0
178.10	142.0
190.90	136.0
192.90	278.0
207.20	72.0
208.20	53.0
249.10	148.0
265.10	123.0
281.10	1189.0
282.20	314.0
283.00	250.0

Instrument :
MSVOA_W
ClientSampleId :
BFB447