

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006409.D
 Acq On : 26 Oct 2018 16:32
 Operator : SY/AP
 Sample : VIBLK91
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK91

Quant Time: Oct 27 01:31:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	310908	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	289248	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	159699	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	65768	18.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.04%
7) Chloroethane-d5	2.90	69	64973	21.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.12%
10) 1,1-Dichloroethene-d2	4.01	63	103001	15.30	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.20%
20) 2-Butanone-d5	7.09	46	65639	56.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.96%
24) Chloroform-d	7.65	84	158251	23.50	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	8.31	65	92732	24.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.56%
29) Benzene-d6	8.28	84	315160	24.00	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.00%
33) 1,2-Dichloropropane-d6	9.28	67	93988	23.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.84%
37) Toluene-d8	10.33	98	307891	23.44	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.76%
38) trans-1,3-Dichloropropene-	10.58	79	38290	19.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.52%
39) 2-Hexanone-d5	10.93	63	53974	56.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	116596	30.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.00%#
61) 1,2-Dichlorobenzene-d4	13.86	152	140132	25.60	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.40%


Target Compounds					Ovalue
13) Acetone	4.14	43	3213	2.736 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006409.D
Acq On : 26 Oct 2018 16:32
Operator : SY/AP
Sample : VIBLK91
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK91

Quant Time: Oct 27 01:31:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration

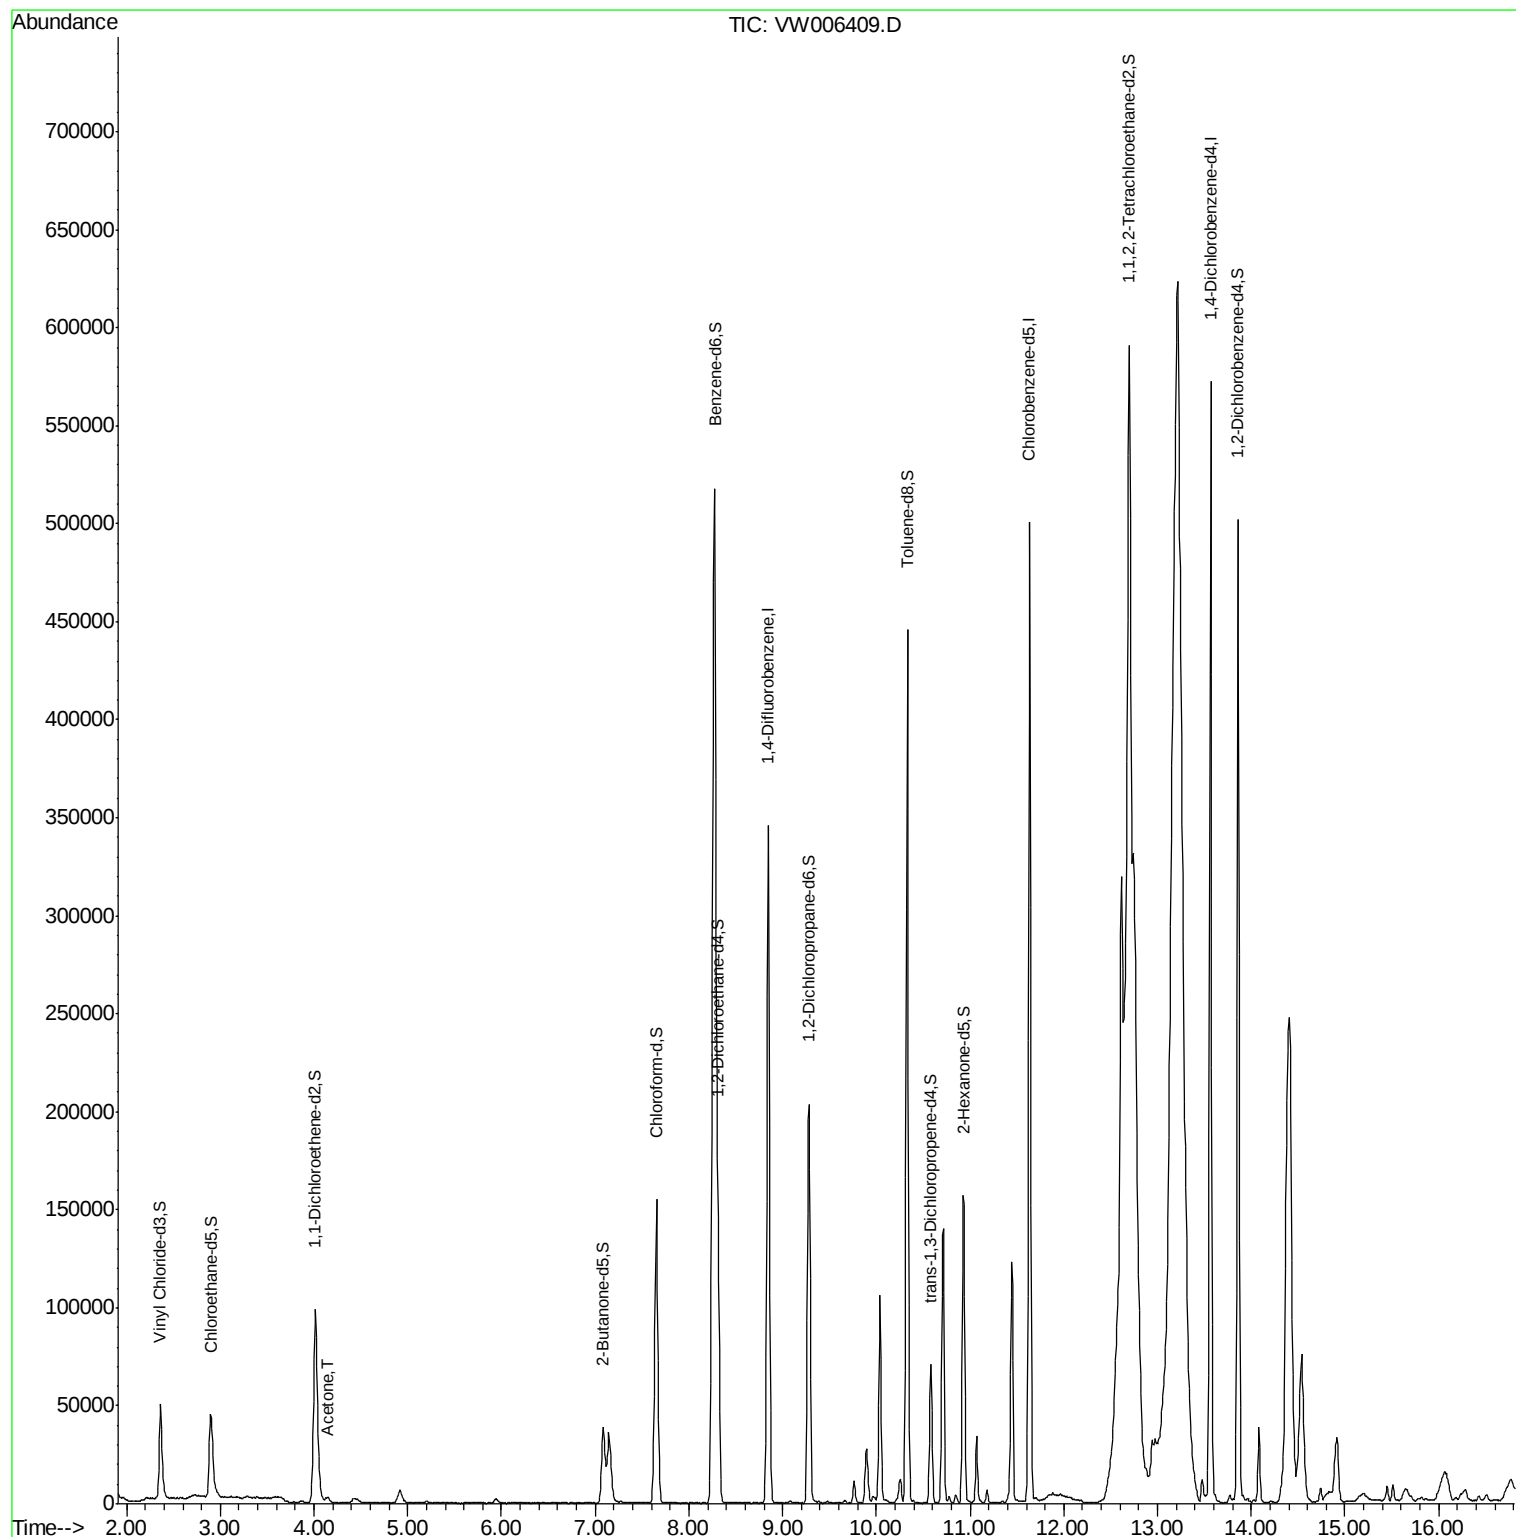

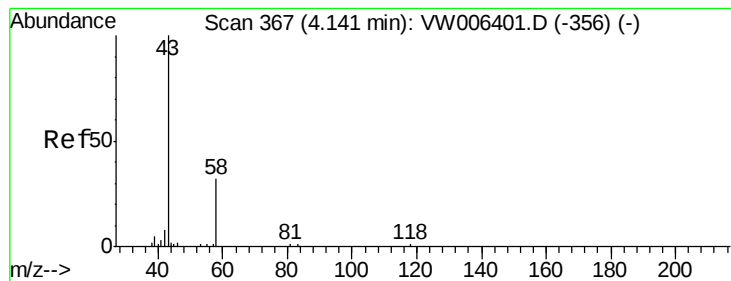

#13

Acetone

Concen: 2.736 ug/L

RT: 4.14 min Scan# 367

Delta R.T. 0.00 min

Lab File: VW006409.D

Acq: 26 Oct 2018 16:32

Instrument :

MSVOA_W

ClientSampleId :

VIBLK91

Tot Ion: 43 Resp: 3213

Ion Ratio Lower Upper

43 100

58 30.6 0.0 61.2

