

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006410.D
 Acq On : 26 Oct 2018 17:13
 Operator : SY/AP
 Sample : J5657-20
 Misc : 5.57G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40G5

Quant Time: Oct 27 01:34:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	374049	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	331407	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	154617	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	73640	17.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.84%
7) Chloroethane-d5	2.90	69	74255	20.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.80%
10) 1,1-Dichloroethene-d2	4.01	63	116249	14.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.40%
20) 2-Butanone-d5	7.09	46	50959	36.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.88%
24) Chloroform-d	7.65	84	186501	23.02	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.08%
26) 1,2-Dichloroethane-d4	8.31	65	104602	23.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.32%
29) Benzene-d6	8.27	84	363105	24.13	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.52%
33) 1,2-Dichloropropane-d6	9.28	67	110016	24.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.92%
37) Toluene-d8	10.33	98	345967	22.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.96%
38) trans-1,3-Dichloropropene-	10.58	79	40880	18.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.08%
39) 2-Hexanone-d5	10.93	63	40901	37.28	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.56%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104178	23.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.36%
61) 1,2-Dichlorobenzene-d4	13.86	152	125304	23.64	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.56%


Target Compounds					Ovalue
13) Acetone	4.14	43	34405	24.356 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006410.D
Acq On : 26 Oct 2018 17:13
Operator : SY/AP
Sample : J5657-20
Misc : 5.57G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40G5

Quant Time: Oct 27 01:34:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration

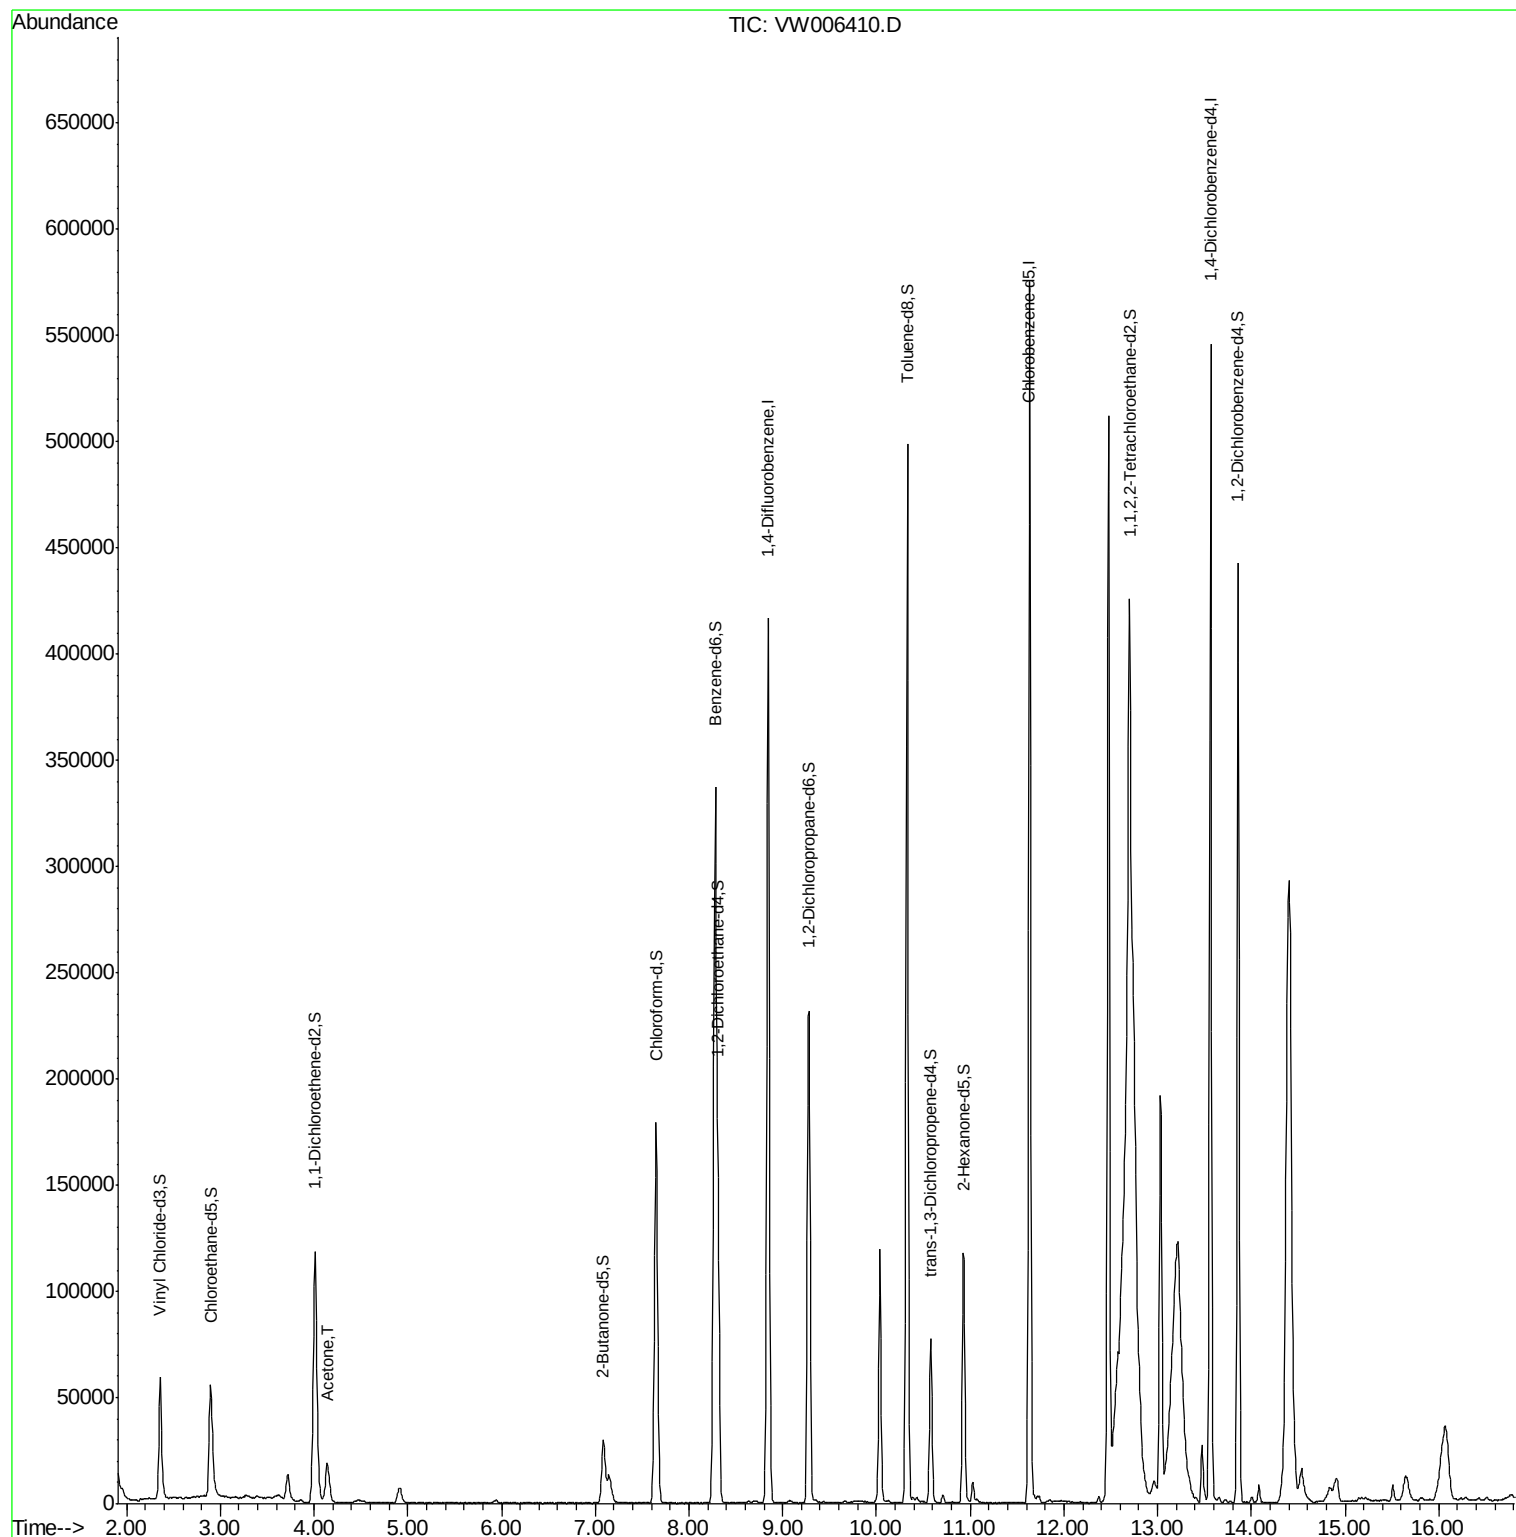

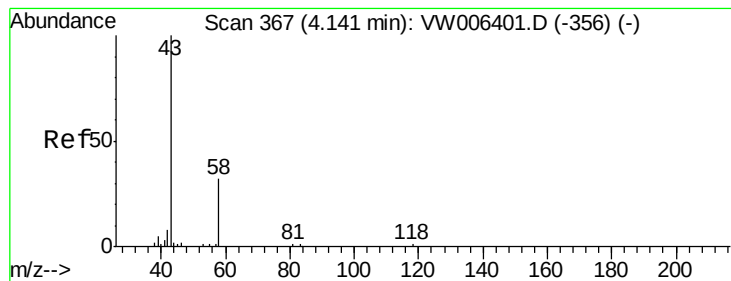

#13
 Acetone
 Concen: 24.356 ug/L
 RT: 4.14 min Scan# 366
 Delta R.T. -0.01 min
 Lab File: VW006410.D
 Acq: 26 Oct 2018 17:13

Instrument :
 MSVOA_W
 ClientSampleId :
 A40G5

Tot Ion: 43 Resp: 34405
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 61.2

