

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006411.D
 Acq On : 26 Oct 2018 17:38
 Operator : SY/AP
 Sample : J5657-21
 Misc : 5.04G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40H1

Quant Time: Oct 27 01:40:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	314128	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	270747	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	116580	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	61099	17.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.00%
7) Chloroethane-d5	2.90	69	59731	19.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.36%
10) 1,1-Dichloroethene-d2	4.01	63	95462	14.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.12%
20) 2-Butanone-d5	7.09	46	46555	39.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.30%
24) Chloroform-d	7.65	84	149668	21.99	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.96%
26) 1,2-Dichloroethane-d4	8.31	65	86361	22.94	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.76%
29) Benzene-d6	8.28	84	288590	23.48	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.92%
33) 1,2-Dichloropropane-d6	9.28	67	88535	23.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.44%
37) Toluene-d8	10.33	98	272213	22.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.56%
38) trans-1,3-Dichloropropene-	10.58	79	31522	17.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.92%
39) 2-Hexanone-d5	10.93	63	37127	41.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.84%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	86934	24.10	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	92656	23.19	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.76%


Target Compounds					Ovalue
13) Acetone	4.14	43	2141	1.805 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006411.D
Acq On : 26 Oct 2018 17:38
Operator : SY/AP
Sample : J5657-21
Misc : 5.04G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40H1

Quant Time: Oct 27 01:40:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration

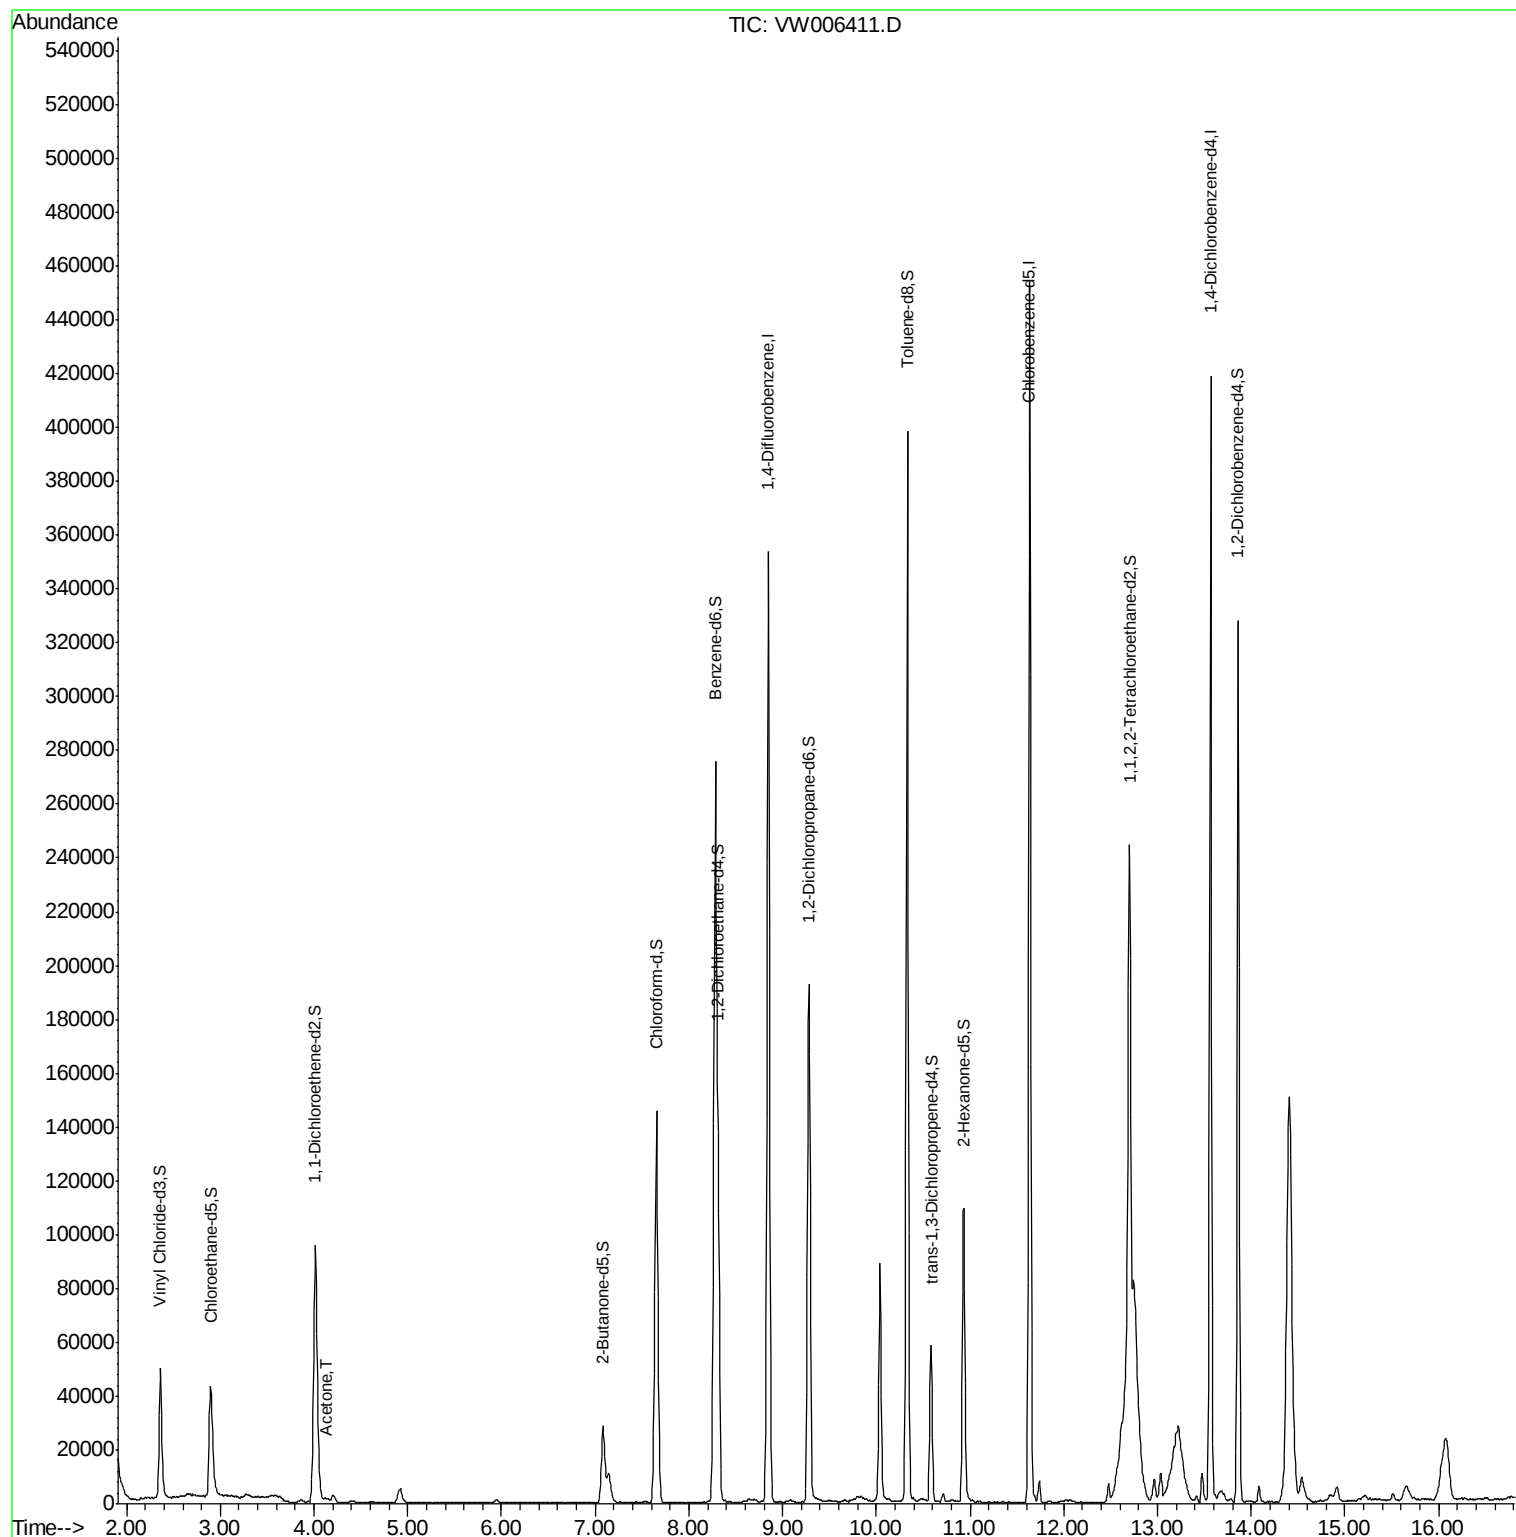

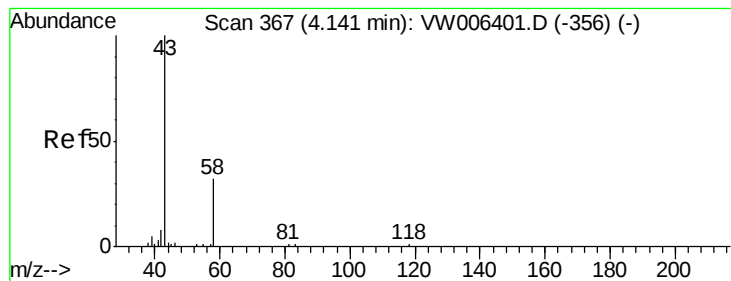

#13

Acetone

Concen: 1.805 ug/L

RT: 4.14 min Scan# 366

Delta R.T. -0.01 min

Lab File: VW006411.D

Acq: 26 Oct 2018 17:38

Instrument :
MSVOA_W
ClientSampleId :
A40H1

Tot Ion: 43 Resp: 2141

Ion Ratio Lower Upper

43 100

58 25.4 0.0 61.2

