

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006412.D
 Acq On : 26 Oct 2018 18:04
 Operator : SY/AP
 Sample : J5657-22
 Misc : 5.03G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40J3

Quant Time: Oct 27 01:43:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	353033	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	327591	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	166400	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	74678	18.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.04%
7) Chloroethane-d5	2.90	69	78435	22.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.56%
10) 1,1-Dichloroethene-d2	4.01	63	118768	15.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.12%
20) 2-Butanone-d5	7.09	46	56134	42.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.06%
24) Chloroform-d	7.65	84	191036	24.98	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.92%
26) 1,2-Dichloroethane-d4	8.31	65	107818	25.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.92%
29) Benzene-d6	8.27	84	373422	25.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.44%
33) 1,2-Dichloropropane-d6	9.27	67	112302	25.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.08%
37) Toluene-d8	10.33	98	360903	24.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.04%
38) trans-1,3-Dichloropropene-	10.58	79	43972	20.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.64%
39) 2-Hexanone-d5	10.93	63	47188	43.51	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.02%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	107116	24.54	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	152892	26.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.24%


Target Compounds					Ovalue
13) Acetone	4.14	43	32017	24.014 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006412.D
Acq On : 26 Oct 2018 18:04
Operator : SY/AP
Sample : J5657-22
Misc : 5.03G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40J3

Quant Time: Oct 27 01:43:06 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration

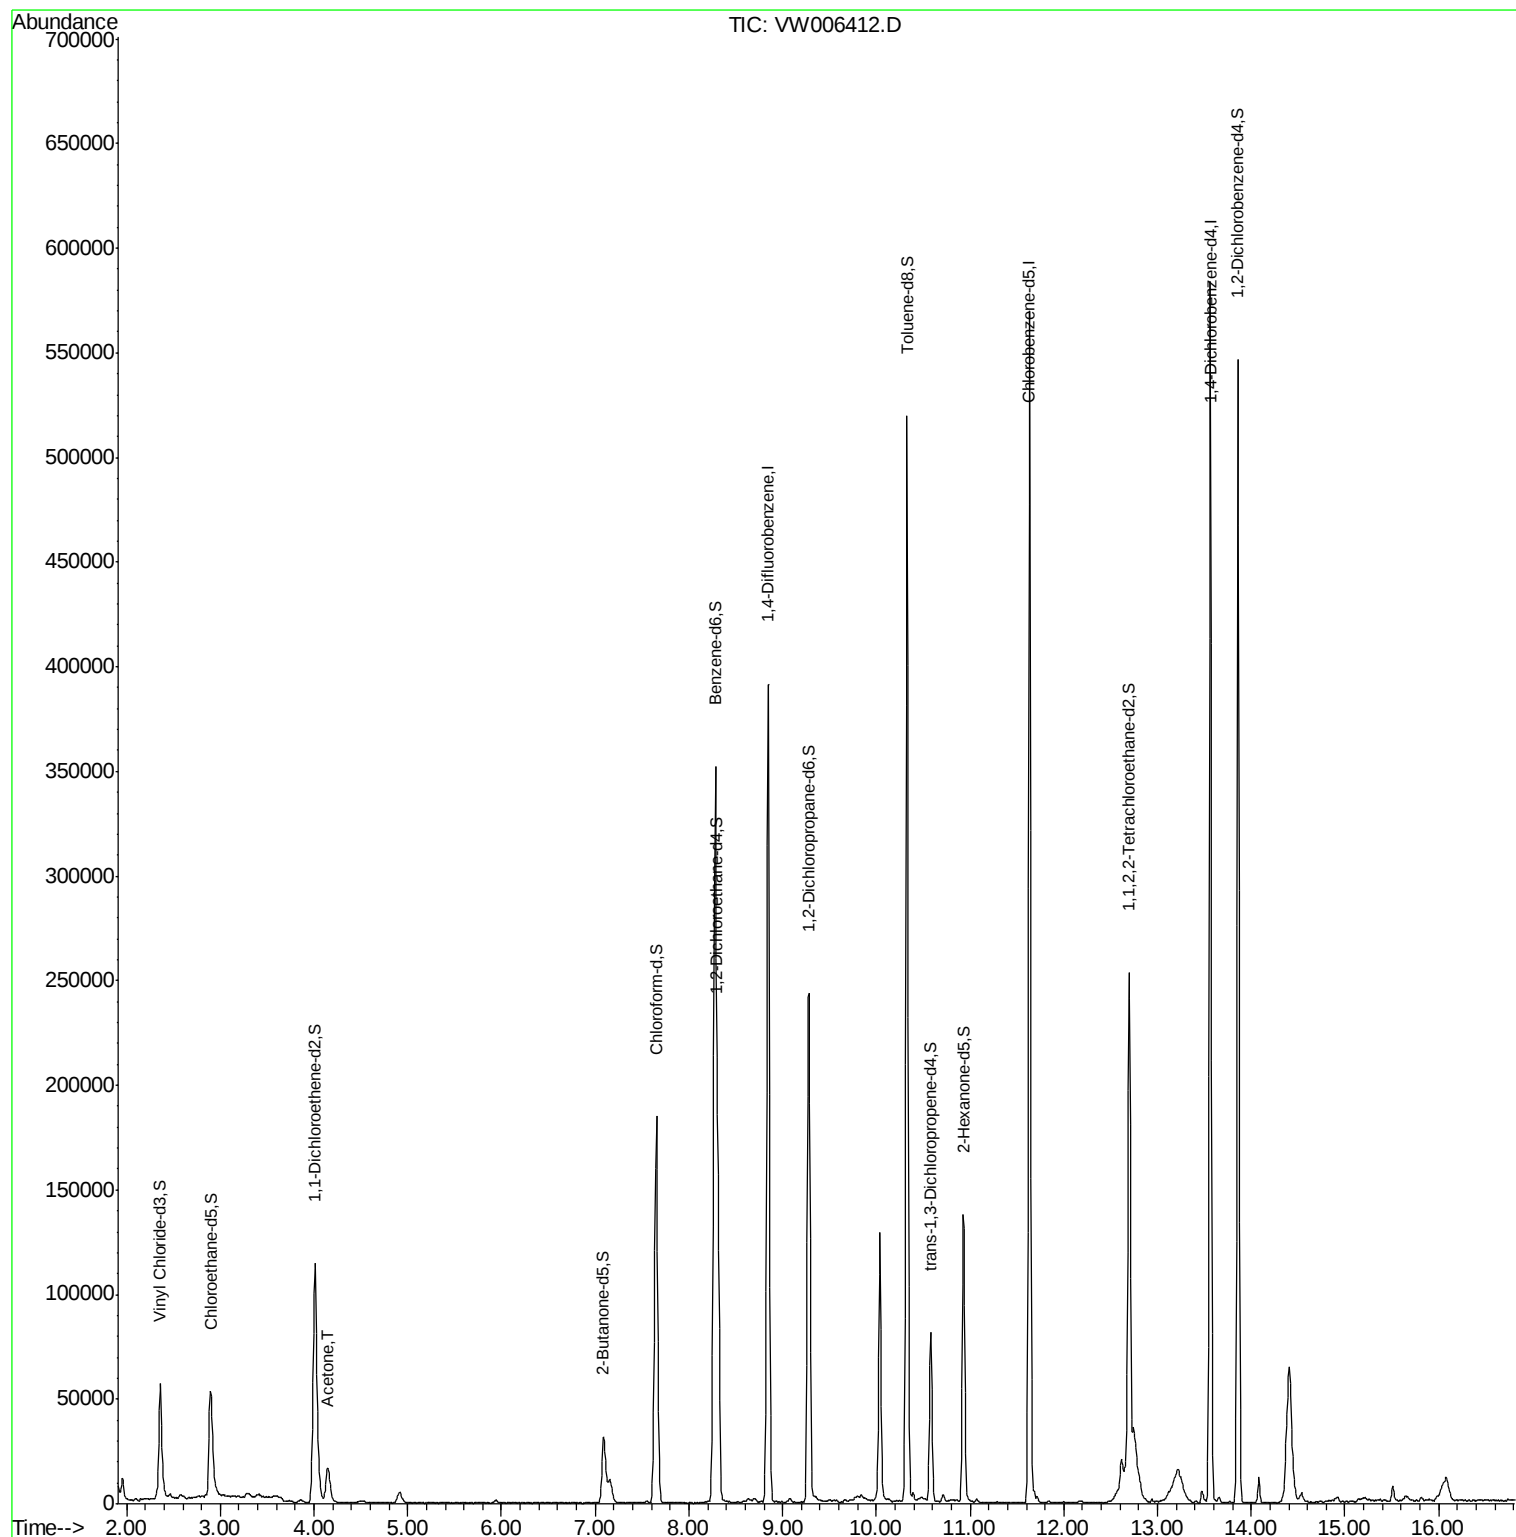

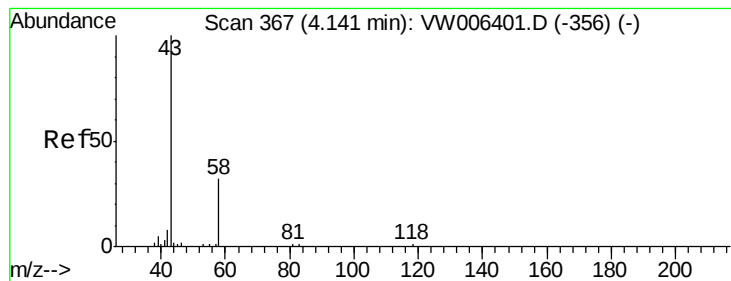

#13
 Acetone
 Concen: 24.014 ug/L
 RT: 4.14 min Scan# 367
 Delta R.T. 0.00 min
 Lab File: VW006412.D
 Acq: 26 Oct 2018 18:04

Instrument :
 MSVOA_W
 ClientSampleId :
 A40J3

Tot Ion: 43 Resp: 32017
 Ion Ratio Lower Upper
 43 100
 58 29.7 0.0 61.2

