

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006413.D
 Acq On : 26 Oct 2018 18:30
 Operator : SY/AP
 Sample : J5657-23
 Misc : 4.96G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40K0

Quant Time: Oct 27 01:45:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	314855	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	264363	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	112028	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	59735	16.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.28%
7) Chloroethane-d5	2.90	69	62806	20.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.20%
10) 1,1-Dichloroethene-d2	4.01	63	94760	13.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.60%
20) 2-Butanone-d5	7.09	46	51126	43.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.88%
24) Chloroform-d	7.65	84	153045	22.44	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.76%
26) 1,2-Dichloroethane-d4	8.31	65	88934	23.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.28%
29) Benzene-d6	8.28	84	296970	24.74	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.96%
33) 1,2-Dichloropropane-d6	9.28	67	90646	25.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.08%
37) Toluene-d8	10.33	98	273671	22.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.20%
38) trans-1,3-Dichloropropene-	10.58	79	33148	18.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.32%
39) 2-Hexanone-d5	10.93	63	41112	46.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.94%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	83932	23.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.32%
61) 1,2-Dichlorobenzene-d4	13.86	152	88313	23.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.00%


Target Compounds					Ovalue
13) Acetone	4.14	43	25054	21.070 ug/L	99
21) 2-Butanone	7.18	43	8278	5.239 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006413.D
Acq On : 26 Oct 2018 18:30
Operator : SY/AP
Sample : J5657-23
Misc : 4.96G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40K0

Quant Time: Oct 27 01:45:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration




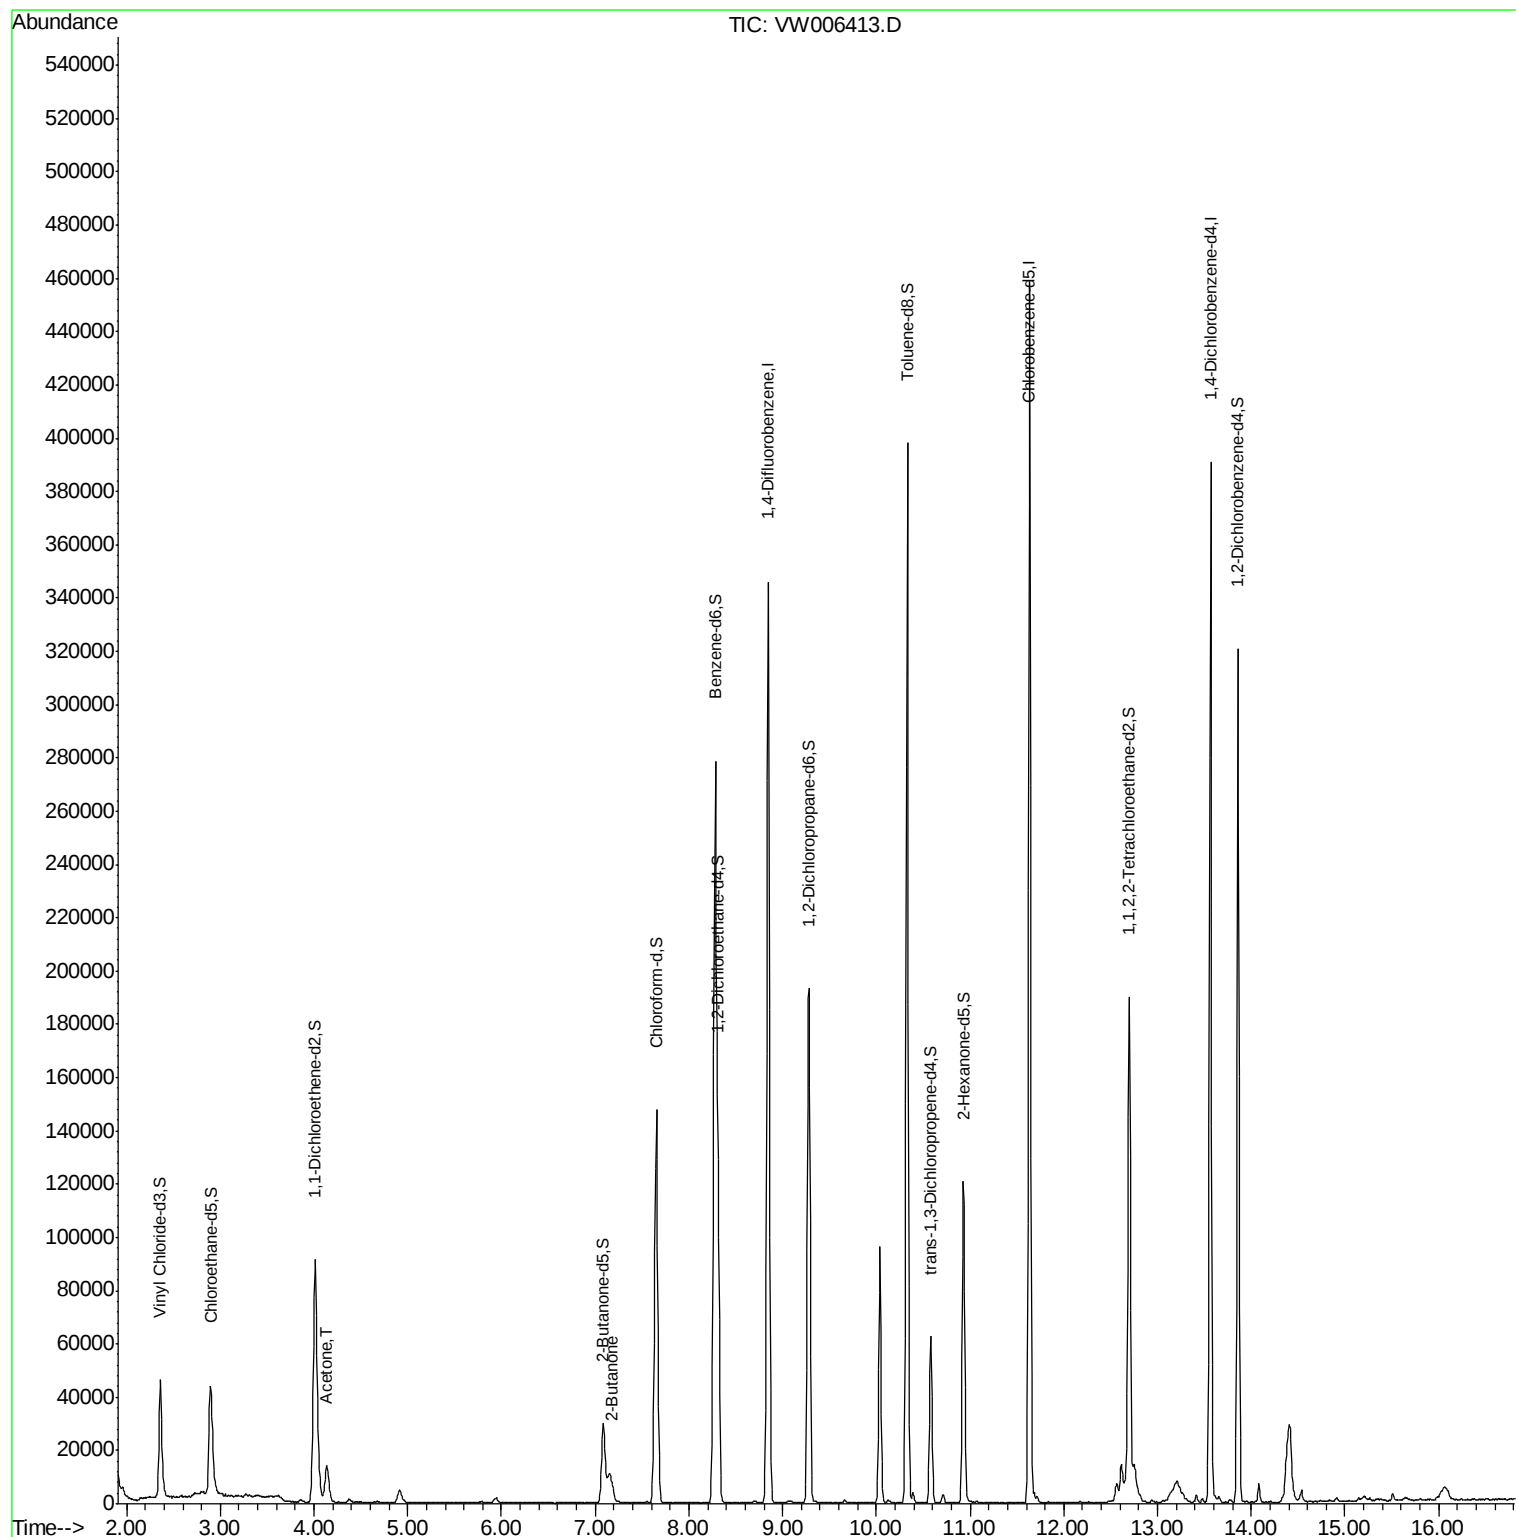


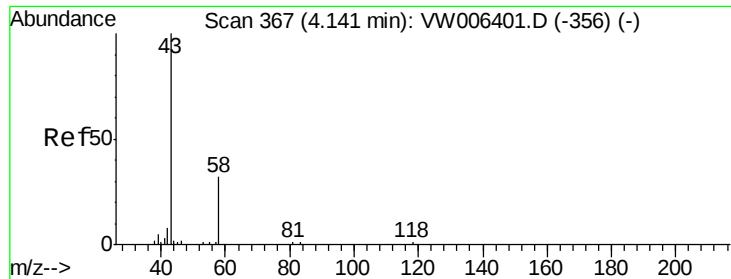

#13
Acetone
Concen: 21.070 ug/L
RT: 4.14 min Scan# 366
Delta R.T. -0.01 min
Lab File: VW006413.D
Acq: 26 Oct 2018 18:30

Instrument :
MSVOA_W
ClientSampleId :
A40K0

Tot Ion: 43 Resp: 25054
Ion Ratio Lower Upper
43 100
58 30.0 0.0 61.2

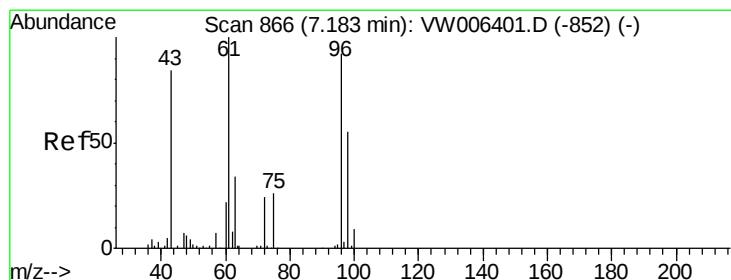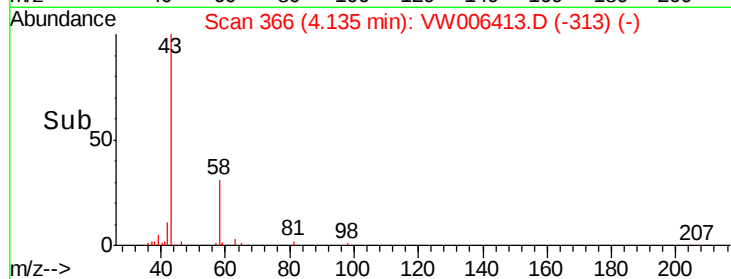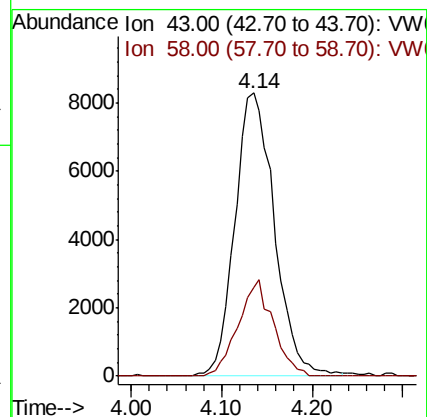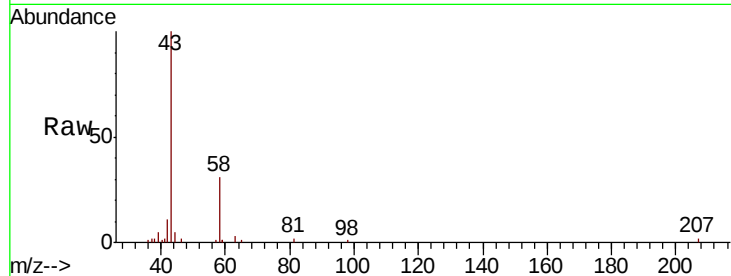

#21
2-Butanone
Concen: 5.239 ug/L
RT: 7.18 min Scan# 866
Delta R.T. 0.00 min
Lab File: VW006413.D
Acq: 26 Oct 2018 18:30

Tgt Ion: 43 Resp: 8278
Ion Ratio Lower Upper
43 100
72 24.6 13.8 41.4

