

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006415.D
 Acq On : 26 Oct 2018 19:21
 Operator : SY/AP
 Sample : VIBLK92
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK92

Quant Time: Oct 27 01:50:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	296556	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	277772	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	147613	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	58902	17.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.44%
7) Chloroethane-d5	2.90	69	61479	21.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.44%
10) 1,1-Dichloroethene-d2	4.01	63	94805	14.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.04%
20) 2-Butanone-d5	7.09	46	59938	54.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.14%
24) Chloroform-d	7.65	84	146478	22.80	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.20%
26) 1,2-Dichloroethane-d4	8.31	65	86906	24.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.80%
29) Benzene-d6	8.27	84	290839	23.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.24%
33) 1,2-Dichloropropane-d6	9.28	67	86261	22.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.64%
37) Toluene-d8	10.33	98	282069	22.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.48%
38) trans-1,3-Dichloropropene-	10.58	79	35091	18.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.88%
39) 2-Hexanone-d5	10.93	63	48720	52.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	97978	26.47	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.88%
61) 1,2-Dichlorobenzene-d4	13.86	152	127602	25.22	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.88%


Target Compounds					Ovalue
13) Acetone	4.14	43	3035	2.710 ug/L	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006415.D
Acq On : 26 Oct 2018 19:21
Operator : SY/AP
Sample : VIBLK92
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK92

Quant Time: Oct 27 01:50:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration

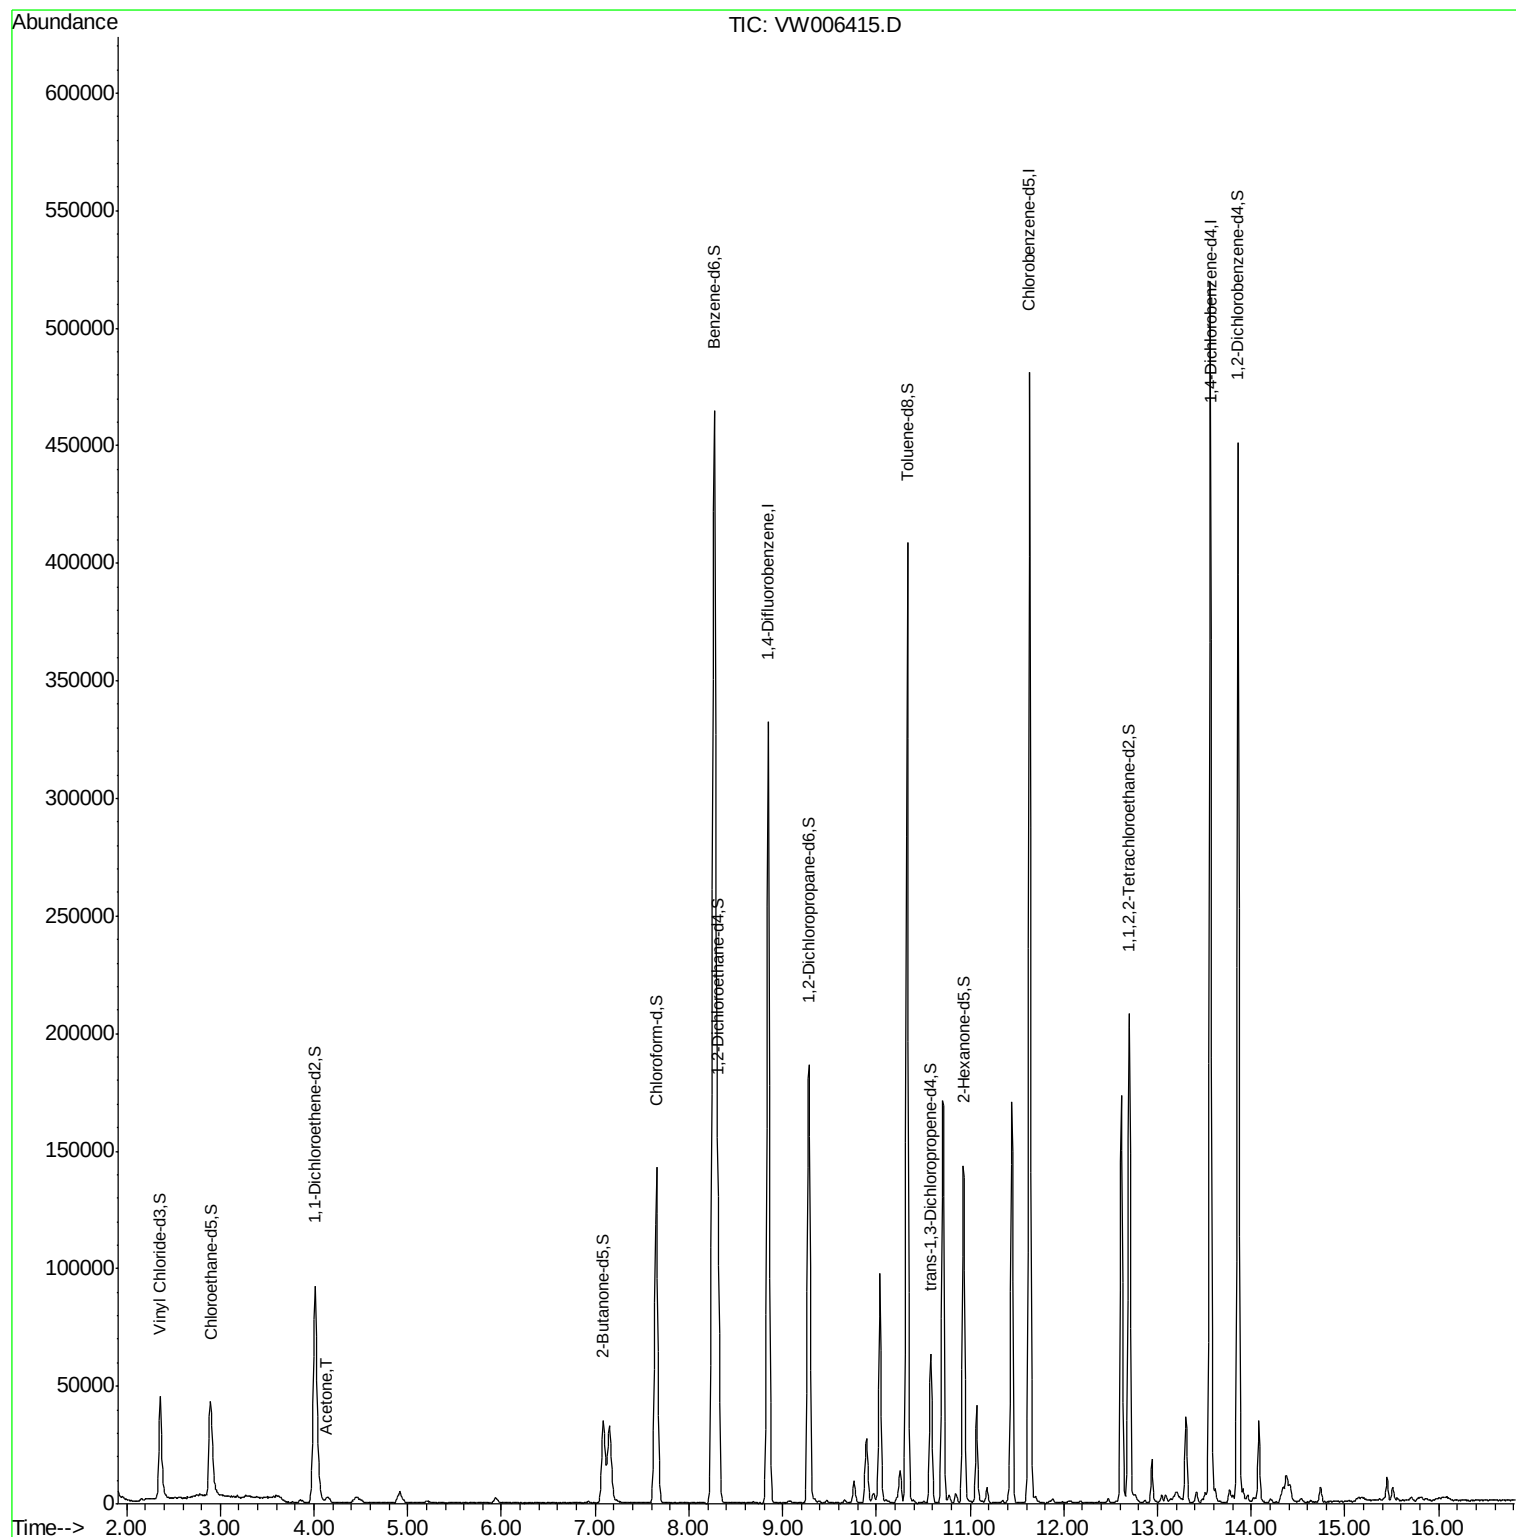

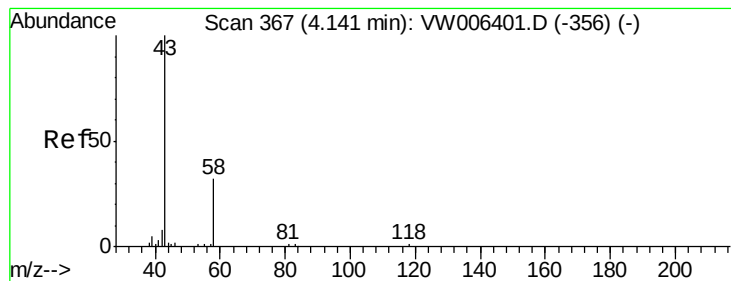

#13
 Acetone
 Concen: 2.710 ug/L
 RT: 4.14 min Scan# 366
 Delta R.T. -0.01 min
 Lab File: VW006415.D
 Acq: 26 Oct 2018 19:21

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK92

Tot Ion: 43 Resp: 3035
 Ion Ratio Lower Upper
 43 100
 58 14.1 0.0 61.2

