

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
 Data File : VW006416.D
 Acq On : 26 Oct 2018 19:47
 Operator : SY/AP
 Sample : J5635-27
 Misc : 5.44G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A40H7

Quant Time: Oct 27 01:52:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 26 23:43:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	353589	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	322737	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	155470	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	72664	18.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.88%
7) Chloroethane-d5	2.90	69	75392	21.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.88%
10) 1,1-Dichloroethene-d2	4.01	63	118524	15.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.92%
20) 2-Butanone-d5	7.09	46	47082	35.62	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.24%
24) Chloroform-d	7.65	84	191463	25.00	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.00%
26) 1,2-Dichloroethane-d4	8.31	65	107695	25.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.68%
29) Benzene-d6	8.28	84	374066	25.53	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.12%
33) 1,2-Dichloropropane-d6	9.28	67	113626	25.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.76%
37) Toluene-d8	10.33	98	357952	24.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.72%
38) trans-1,3-Dichloropropene-	10.58	79	41815	19.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.84%
39) 2-Hexanone-d5	10.93	63	37004	34.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	102663	23.87	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.48%
61) 1,2-Dichlorobenzene-d4	13.86	152	140935	26.45	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.80%


Target Compounds					Ovalue
13) Acetone	4.13	43	26075	19.527 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006416.D
Acq On : 26 Oct 2018 19:47
Operator : SY/AP
Sample : J5635-27
Misc : 5.44G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A40H7

Quant Time: Oct 27 01:52:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 26 23:43:44 2018
Response via : Initial Calibration

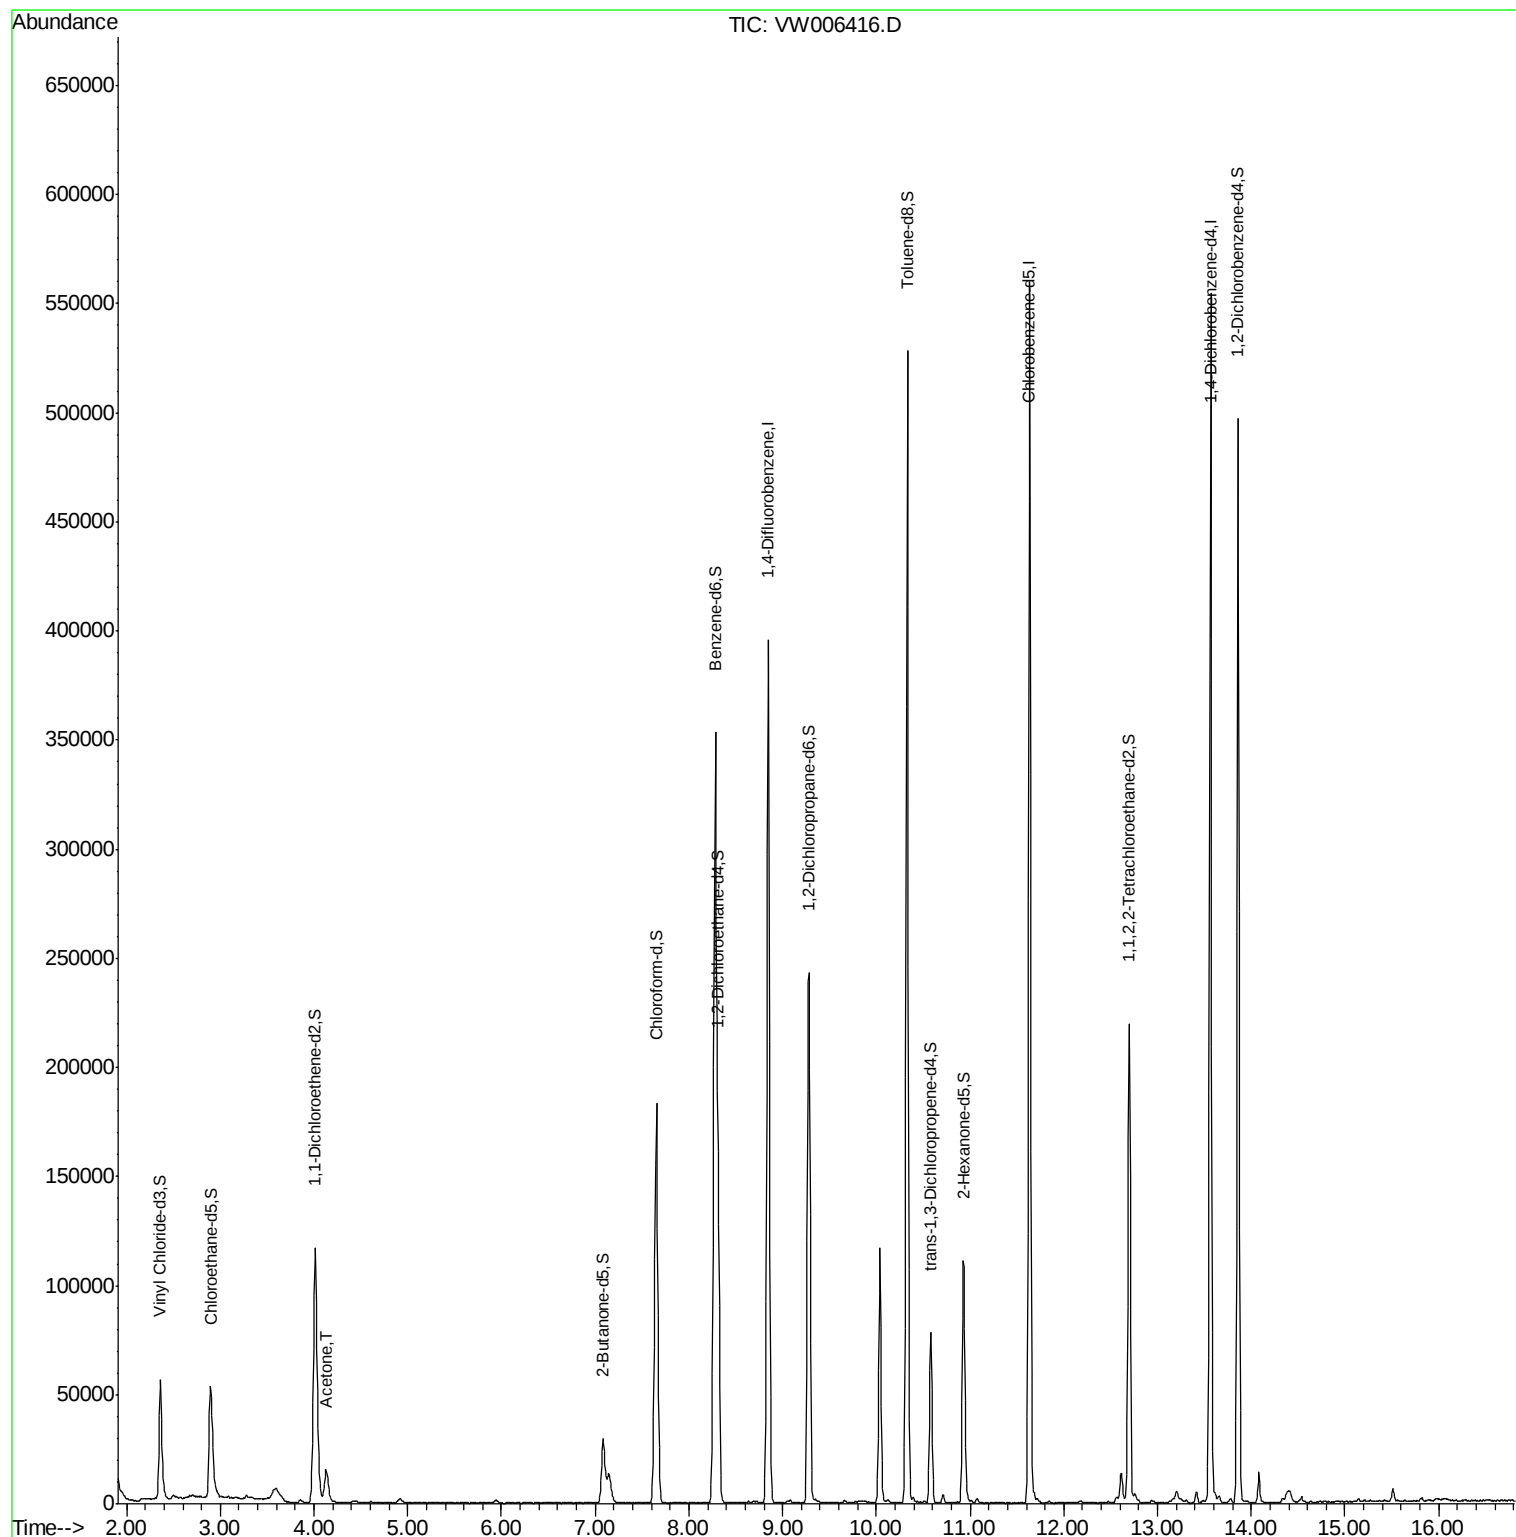

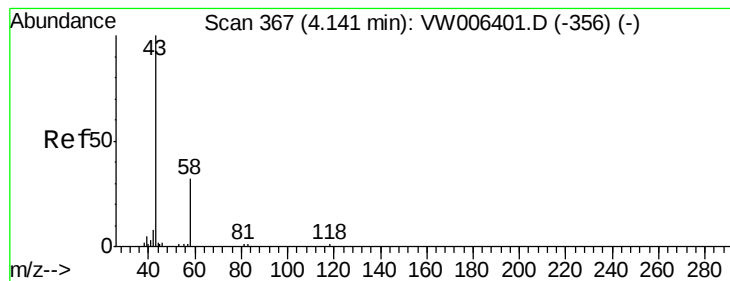

#13
 Acetone
 Concen: 19.527 ug/L
 RT: 4.13 min Scan# 365
 Delta R.T. -0.01 min
 Lab File: VW006416.D
 Acq: 26 Oct 2018 19:47

Instrument :
 MSVOA_W
 ClientSampleId :
 A40H7

Tot Ion: 43 Resp: 26075
 Ion Ratio Lower Upper
 43 100
 58 30.8 0.0 61.2

