


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102818\
Data File : VW006400.D
Acq On : 26 Oct 2018 11:00
Operator : SY/AP
Sample : BFB94
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB94

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Title : VOC Analysis
Last Update : Fri Oct 26 23:43:44 2018

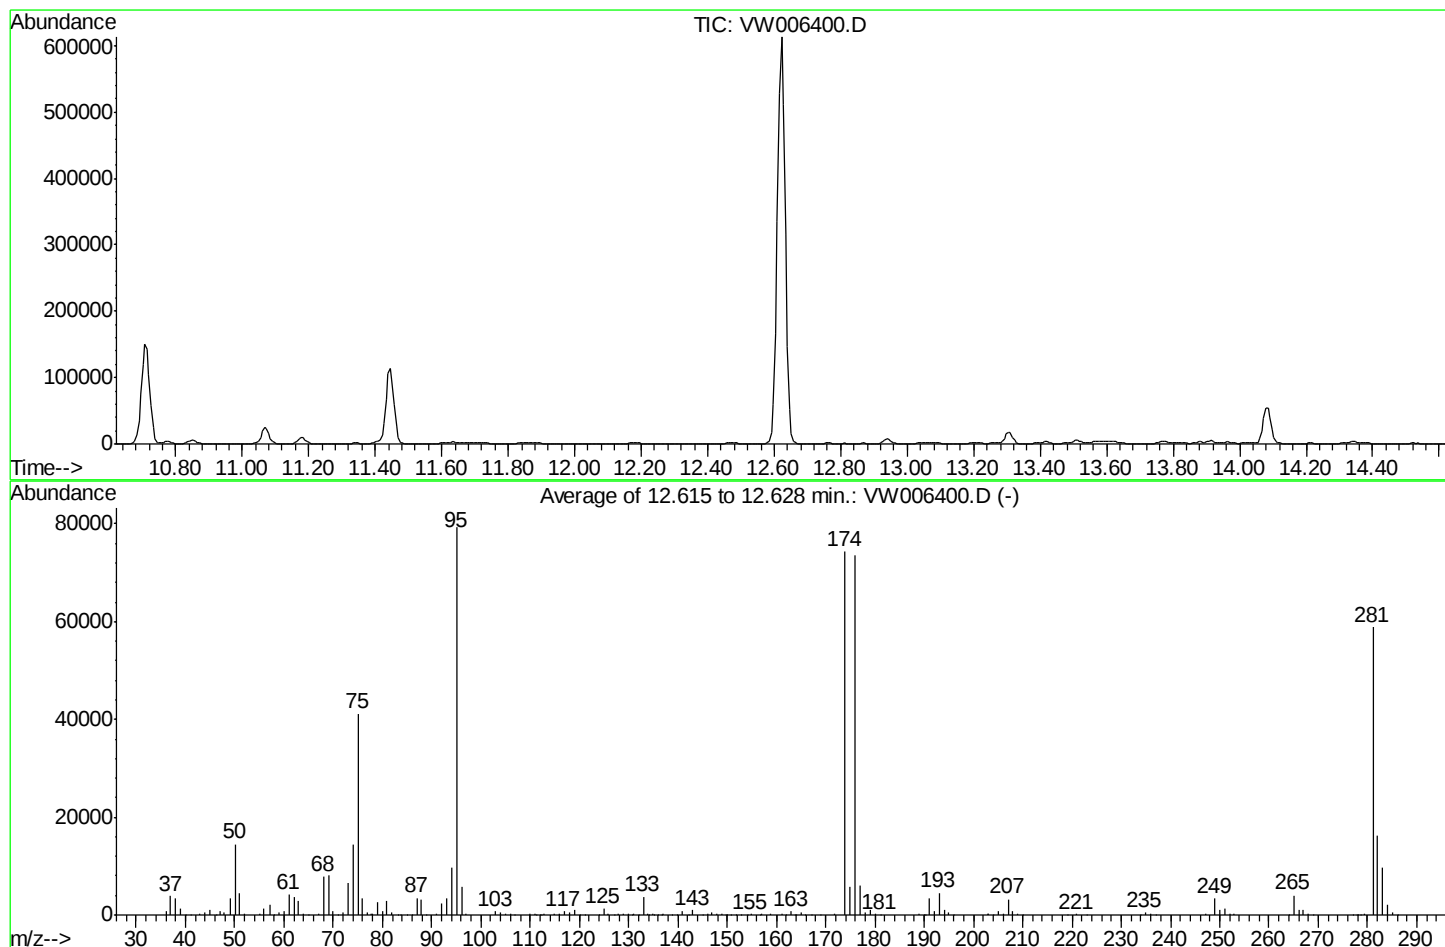

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	14499	PASS
75	95	30	80	51.8	41104	PASS
95	95	100	100	100.0	79282	PASS
96	95	5	9	7.3	5767	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	93.7	74272	PASS
175	174	5	9	7.7	5736	PASS
176	174	95	101	99.2	73696	PASS
177	176	5	9	8.1	5953	PASS

Scan 1750 (12.573 min): VW006400.D
BFB94

m/z	Abundance
39.00	101.0
39.80	74.0
44.00	212.0
55.20	56.0
169.10	72.0
207.10	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

m/z	Abundance
36.00	824.0
37.00	3829.0
38.00	3426.0
39.00	1104.0
40.00	137.0
41.00	102.0
43.00	236.0
44.00	650.0
45.00	1319.0
46.10	100.0
47.00	927.0
48.00	358.0
49.00	3067.0
50.10	13771.0
51.00	4427.0
52.00	178.0
55.00	240.0
56.00	1223.0
57.00	2101.0
58.10	174.0
59.10	789.0
60.00	792.0
61.00	3930.0
62.00	3582.0
63.00	2577.0
63.90	222.0
65.00	106.0
67.00	288.0
68.00	6983.0
69.00	7488.0
70.00	692.0
71.00	120.0
72.00	400.0
73.00	7339.0
74.00	13706.0
75.00	37952.0
76.00	3377.0
77.00	462.0
77.70	323.0
78.00	230.0
78.90	2421.0
79.90	585.0
81.00	2921.0
81.90	594.0
83.20	120.0
83.80	137.0
85.00	108.0
86.00	118.0
87.00	3135.0
87.90	2934.0
91.00	255.0
92.00	2047.0
93.00	3311.0
94.10	8820.0
95.00	71008.0
96.10	5285.0
97.00	339.0
102.90	722.0
103.90	579.0
105.00	371.0
106.00	397.0
106.80	150.0
109.90	305.0
110.80	270.0
112.00	163.0
112.90	143.0
115.00	418.0
116.00	340.0
117.00	728.0
118.00	842.0
119.00	1034.0
120.00	165.0
121.00	157.0
123.80	55.0
125.00	1809.0
127.10	100.0
127.80	220.0
128.90	212.0
129.80	172.0
130.80	188.0
132.10	183.0
133.00	5072.0
134.90	571.0
136.80	167.0
138.80	83.0
140.90	642.0
142.10	84.0
143.00	819.0
144.90	170.0
146.00	195.0
146.90	593.0
147.90	244.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

148.90	329.0
149.80	129.0
154.90	182.0
156.80	123.0
158.80	147.0
160.90	485.0
161.90	133.0
163.00	1061.0
164.10	168.0
164.90	618.0
165.80	142.0
167.00	121.0
171.90	300.0
173.90	58808.0
175.00	4753.0
175.90	57936.0
177.00	5443.0
178.00	415.0
179.00	1207.0
180.00	334.0
181.00	134.0
189.00	364.0
190.20	156.0
191.00	4510.0
192.00	938.0
193.00	5790.0
194.00	1118.0
194.90	695.0
196.10	73.0
202.90	470.0
204.00	74.0
205.00	1116.0
206.00	301.0
207.00	3992.0
208.00	723.0
209.00	468.0
210.10	67.0
219.00	115.0
221.00	202.0
223.00	78.0
234.00	73.0
234.90	558.0
235.90	195.0
237.00	99.0
247.00	184.0
249.00	4197.0
250.00	1178.0
251.00	1875.0
252.00	504.0
253.00	216.0
264.00	70.0
265.00	4592.0
266.00	1181.0
267.00	1262.0
268.10	286.0
268.90	106.0
277.00	82.0
277.90	81.0
279.20	353.0
281.10	70048.0
282.10	19544.0
283.00	11541.0
284.00	2545.0
285.10	723.0
286.10	99.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

m/z	Abundance
36.00	649.0
37.00	4106.0
38.00	3785.0
39.10	1630.0
40.00	125.0
43.00	197.0
44.00	733.0
45.00	1306.0
46.20	70.0
47.00	899.0
47.90	529.0
49.00	3772.0
50.00	16432.0
51.00	4987.0
52.00	264.0
55.10	306.0
56.00	1474.0
57.10	2759.0
57.90	126.0
59.00	702.0
60.00	1001.0
61.00	4333.0
62.00	3961.0
63.00	3320.0
63.90	274.0
65.00	128.0
66.90	278.0
68.00	9181.0
69.00	8964.0
70.00	729.0
71.00	80.0
72.00	594.0
73.00	7269.0
74.00	15863.0
75.00	45720.0
76.00	3740.0
77.00	436.0
78.00	370.0
78.90	3183.0
80.00	866.0
80.90	3159.0
81.90	717.0
83.00	115.0
85.00	88.0
85.80	77.0
86.90	3686.0
87.90	3673.0
88.90	265.0
90.90	408.0
92.00	2700.0
93.00	3621.0
94.00	10862.0
95.00	89280.0
96.00	6639.0
97.10	181.0
103.00	772.0
104.00	740.0
104.90	452.0
105.90	468.0
106.80	126.0
110.00	245.0
110.90	271.0
112.20	243.0
113.00	134.0
114.90	457.0
115.90	341.0
116.90	850.0
117.90	539.0
119.00	1185.0
119.90	183.0
121.10	135.0
123.90	122.0
125.00	1310.0
125.70	472.0
127.00	107.0
127.90	339.0
129.00	230.0
129.90	406.0
131.10	272.0
131.90	72.0
132.00	70.0
133.00	4085.0
133.80	858.0
134.90	552.0
135.80	62.0
137.00	229.0
138.80	81.0
139.90	86.0
140.90	862.0
143.00	1081.0
145.00	124.0
146.00	197.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

147.00	485.0
147.80	237.0
148.90	263.0
150.00	144.0
151.80	60.0
152.80	65.0
154.90	260.0
157.00	206.0
158.90	200.0
161.00	379.0
162.00	176.0
162.90	690.0
163.90	158.0
164.90	484.0
165.90	72.0
167.10	54.0
169.00	148.0
172.00	400.0
173.90	83528.0
175.00	6104.0
175.90	82416.0
176.90	6544.0
178.00	467.0
179.00	1002.0
180.00	181.0
181.10	151.0
189.00	356.0
191.00	3420.0
192.00	812.0
193.00	4746.0
194.00	982.0
195.00	510.0
195.90	63.0
203.10	431.0
204.00	120.0
205.00	954.0
206.10	277.0
207.10	3672.0
208.00	809.0
209.00	404.0
218.90	87.0
220.90	218.0
234.90	536.0
236.00	160.0
236.90	109.0
247.10	133.0
249.00	3592.0
250.00	1107.0
251.00	1409.0
252.00	381.0
252.90	191.0
265.00	4521.0
265.90	1377.0
267.00	903.0
268.00	278.0
269.00	138.0
276.90	83.0
278.10	99.0
279.30	259.0
281.10	64568.0
282.00	17688.0
283.10	10642.0
284.10	2193.0
285.00	740.0
285.90	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

m/z	Abundance
36.00	735.0
37.00	3586.0
38.00	3167.0
39.00	1228.0
40.00	141.0
43.00	141.0
44.00	495.0
45.00	888.0
47.00	935.0
48.00	487.0
49.10	3113.0
50.00	13294.0
51.00	4228.0
52.00	186.0
55.00	239.0
56.00	1348.0
57.00	1805.0
58.00	115.0
59.00	283.0
60.10	794.0
61.00	4017.0
62.00	3509.0
63.00	2447.0
64.00	300.0
65.00	104.0
67.10	226.0
68.00	7300.0
69.00	8130.0
70.00	694.0
70.90	55.0
72.00	527.0
73.10	5180.0
74.00	13416.0
75.00	39640.0
76.00	2922.0
77.00	503.0
77.80	322.0
78.90	2533.0
79.90	628.0
80.90	2696.0
81.90	606.0
83.00	93.0
85.90	99.0
87.00	3493.0
88.00	2995.0
91.00	343.0
92.00	2507.0
93.00	2998.0
94.00	9519.0
95.00	77560.0
96.00	5377.0
96.90	264.0
103.00	518.0
103.90	405.0
104.90	278.0
105.90	331.0
106.80	89.0
110.10	152.0
111.10	272.0
112.00	84.0
112.80	156.0
115.00	183.0
115.90	346.0
116.90	629.0
117.90	571.0
119.00	853.0
119.90	61.0
120.90	71.0
123.90	89.0
124.80	531.0
125.80	241.0
127.80	273.0
128.90	143.0
129.80	288.0
131.00	217.0
132.10	91.0
133.00	1872.0
134.00	342.0
135.10	258.0
136.90	206.0
139.90	90.0
140.90	902.0
142.00	96.0
143.00	970.0
144.80	85.0
146.00	144.0
146.90	408.0
147.90	283.0
149.00	246.0
149.90	101.0
150.80	62.0
152.80	77.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94

154.00	89.0
154.80	257.0
157.00	233.0
158.80	147.0
161.10	283.0
162.00	67.0
163.00	468.0
163.70	76.0
164.90	242.0
169.00	116.0
171.80	253.0
173.90	80480.0
174.90	6352.0
175.90	80736.0
176.90	5874.0
178.00	395.0
179.00	792.0
180.00	104.0
181.20	64.0
189.00	204.0
189.90	80.0
191.00	2254.0
192.10	601.0
193.00	2952.0
194.00	743.0
194.90	199.0
195.90	81.0
203.00	320.0
205.00	577.0
206.00	189.0
207.10	2118.0
208.00	597.0
208.90	272.0
209.90	71.0
219.00	56.0
220.90	124.0
234.90	388.0
236.10	75.0
237.00	143.0
247.00	106.0
249.00	2299.0
250.00	738.0
251.00	1034.0
252.00	307.0
252.90	105.0
265.00	2920.0
266.10	718.0
267.00	686.0
268.00	155.0
268.80	68.0
278.20	77.0
278.70	81.0
281.10	41784.0
282.10	11473.0
283.00	6916.0
284.10	1308.0
285.10	514.0
285.90	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB94