


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102819\
 Data File : VW013758.D
 Acq On : 28 Oct 2019 09:50
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
 Title : SW846 8260
 Last Update : Wed Oct 23 14:11:46 2019

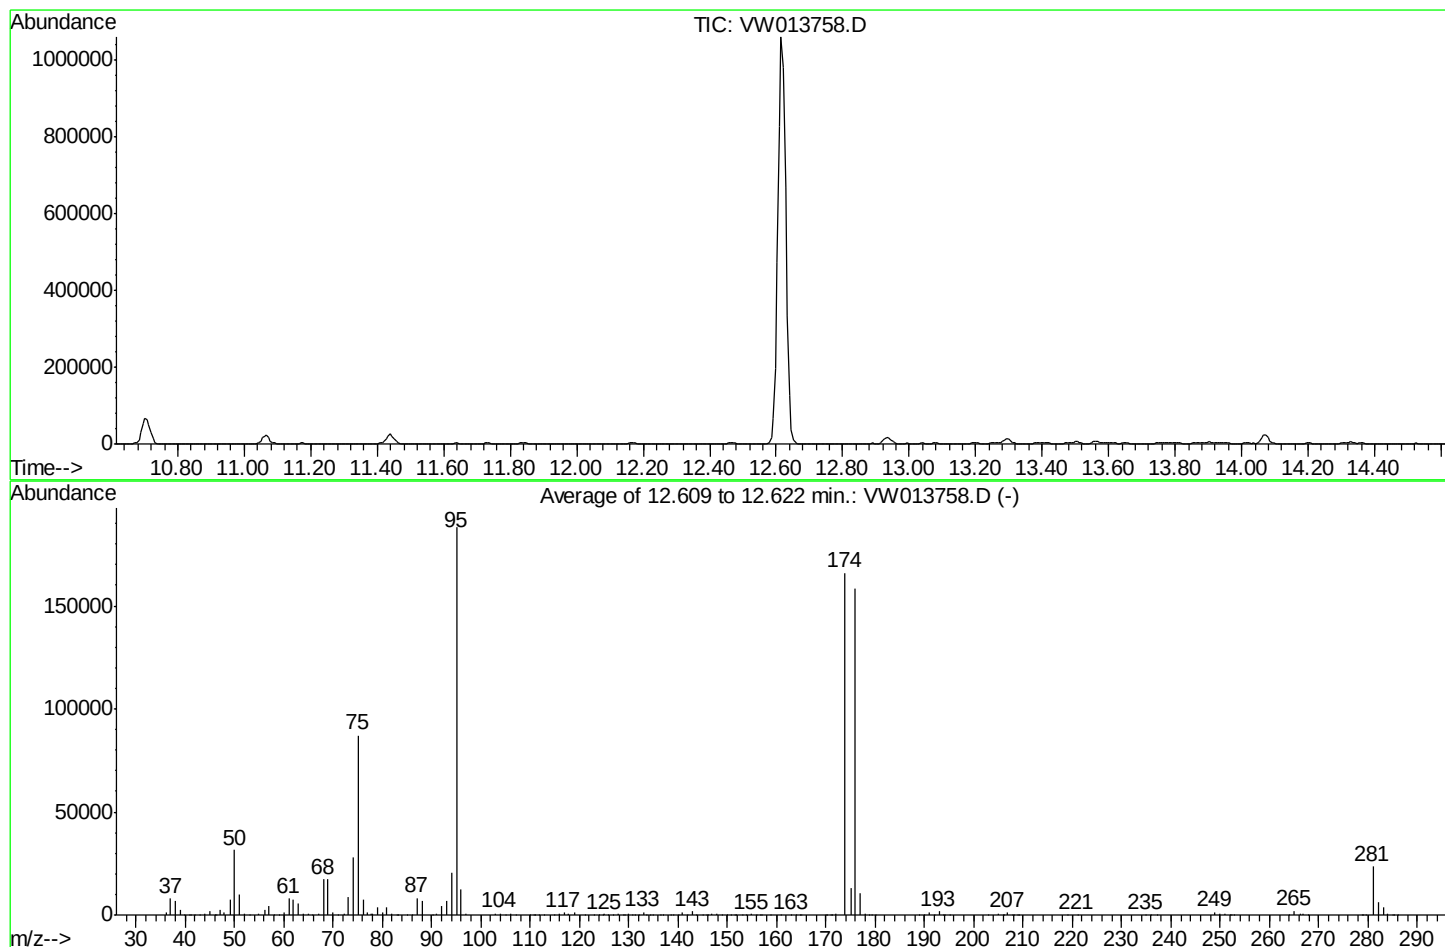

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	31437	PASS
75	95	30	60	46.3	87069	PASS
95	95	100	100	100.0	188138	PASS
96	95	5	9	6.8	12722	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.3	166101	PASS
175	174	5	9	7.9	13183	PASS
176	174	95	101	95.3	158344	PASS
177	176	5	9	6.7	10657	PASS