
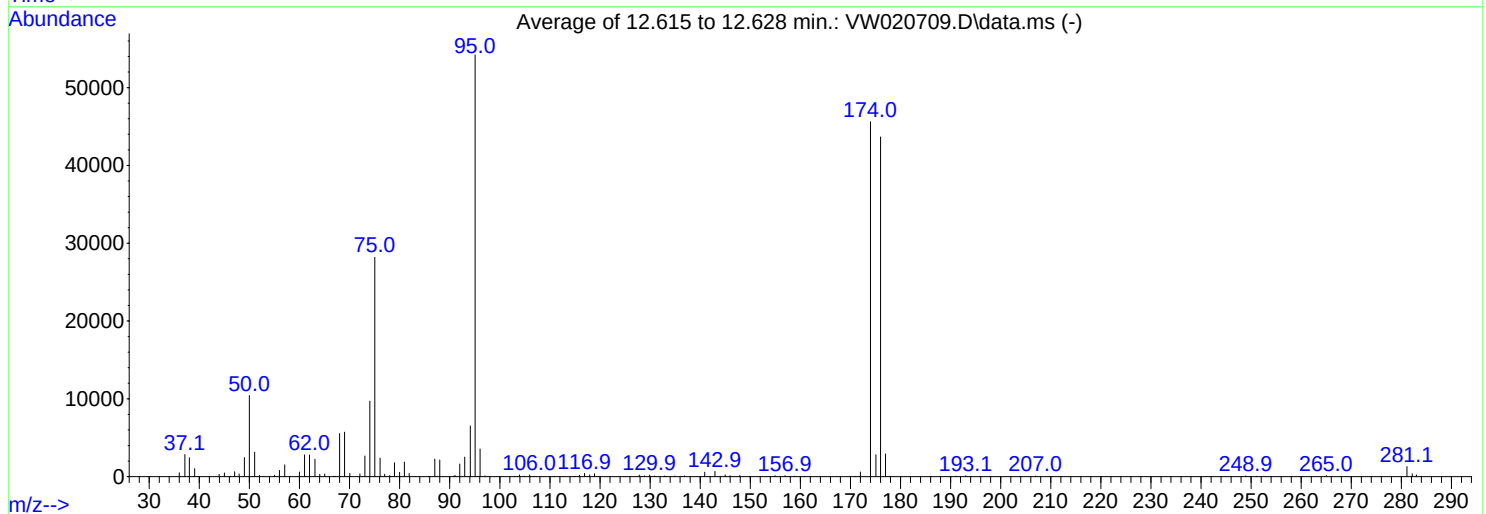


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102821\
 Data File : VW020709.D
 Acq On : 28 Oct 2021 08:10
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W102821S.M
 Title : SW846 8260
 Last Update : Fri Oct 29 05:37:46 2021

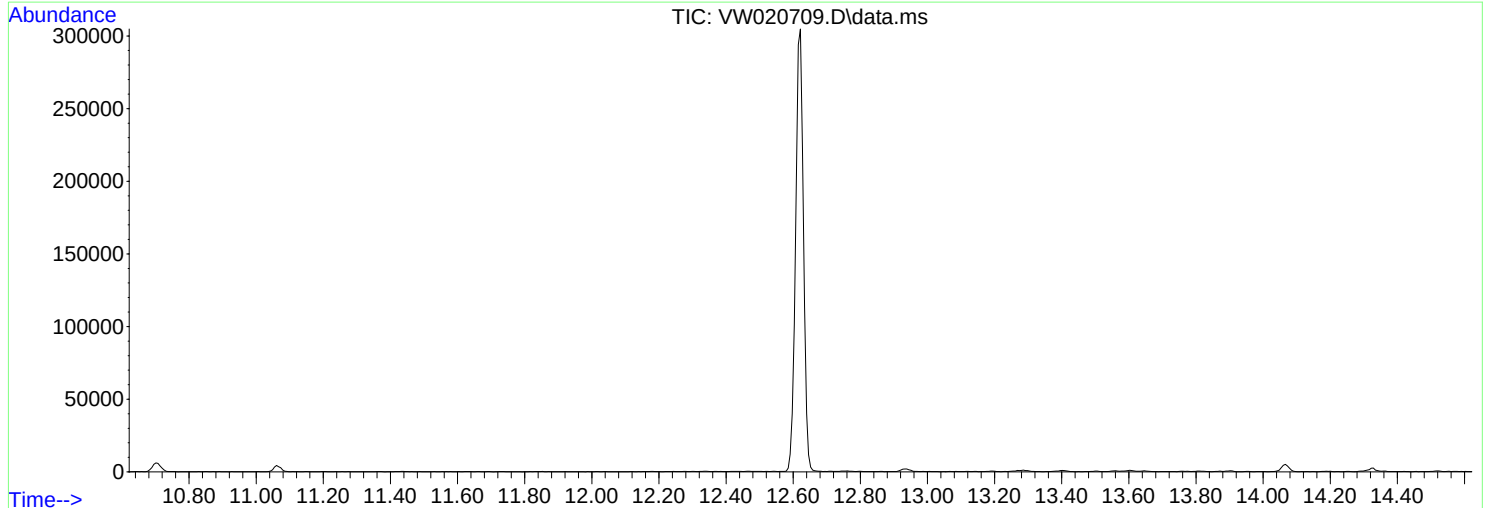

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	10434	PASS
75	95	30	60	52.0	28192	PASS
95	95	100	100	100.0	54211	PASS
96	95	5	9	6.6	3559	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.1	45613	PASS
175	174	5	9	6.2	2820	PASS
176	174	95	101	95.7	43664	PASS
177	176	5	9	6.7	2915	PASS