

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW102919\
Quantitation Report (QT Reviewed)


Data File : VW013799.D
Acq On : 29 Oct 2019 17:46
Operator : SY/VA
Sample : K5535-11
Misc : 6.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 08:04:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 30 06:58:53 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
BEK33

Manual Integrations
APPROVED

MMDadoda
10/30/2019 11:11:58 AM

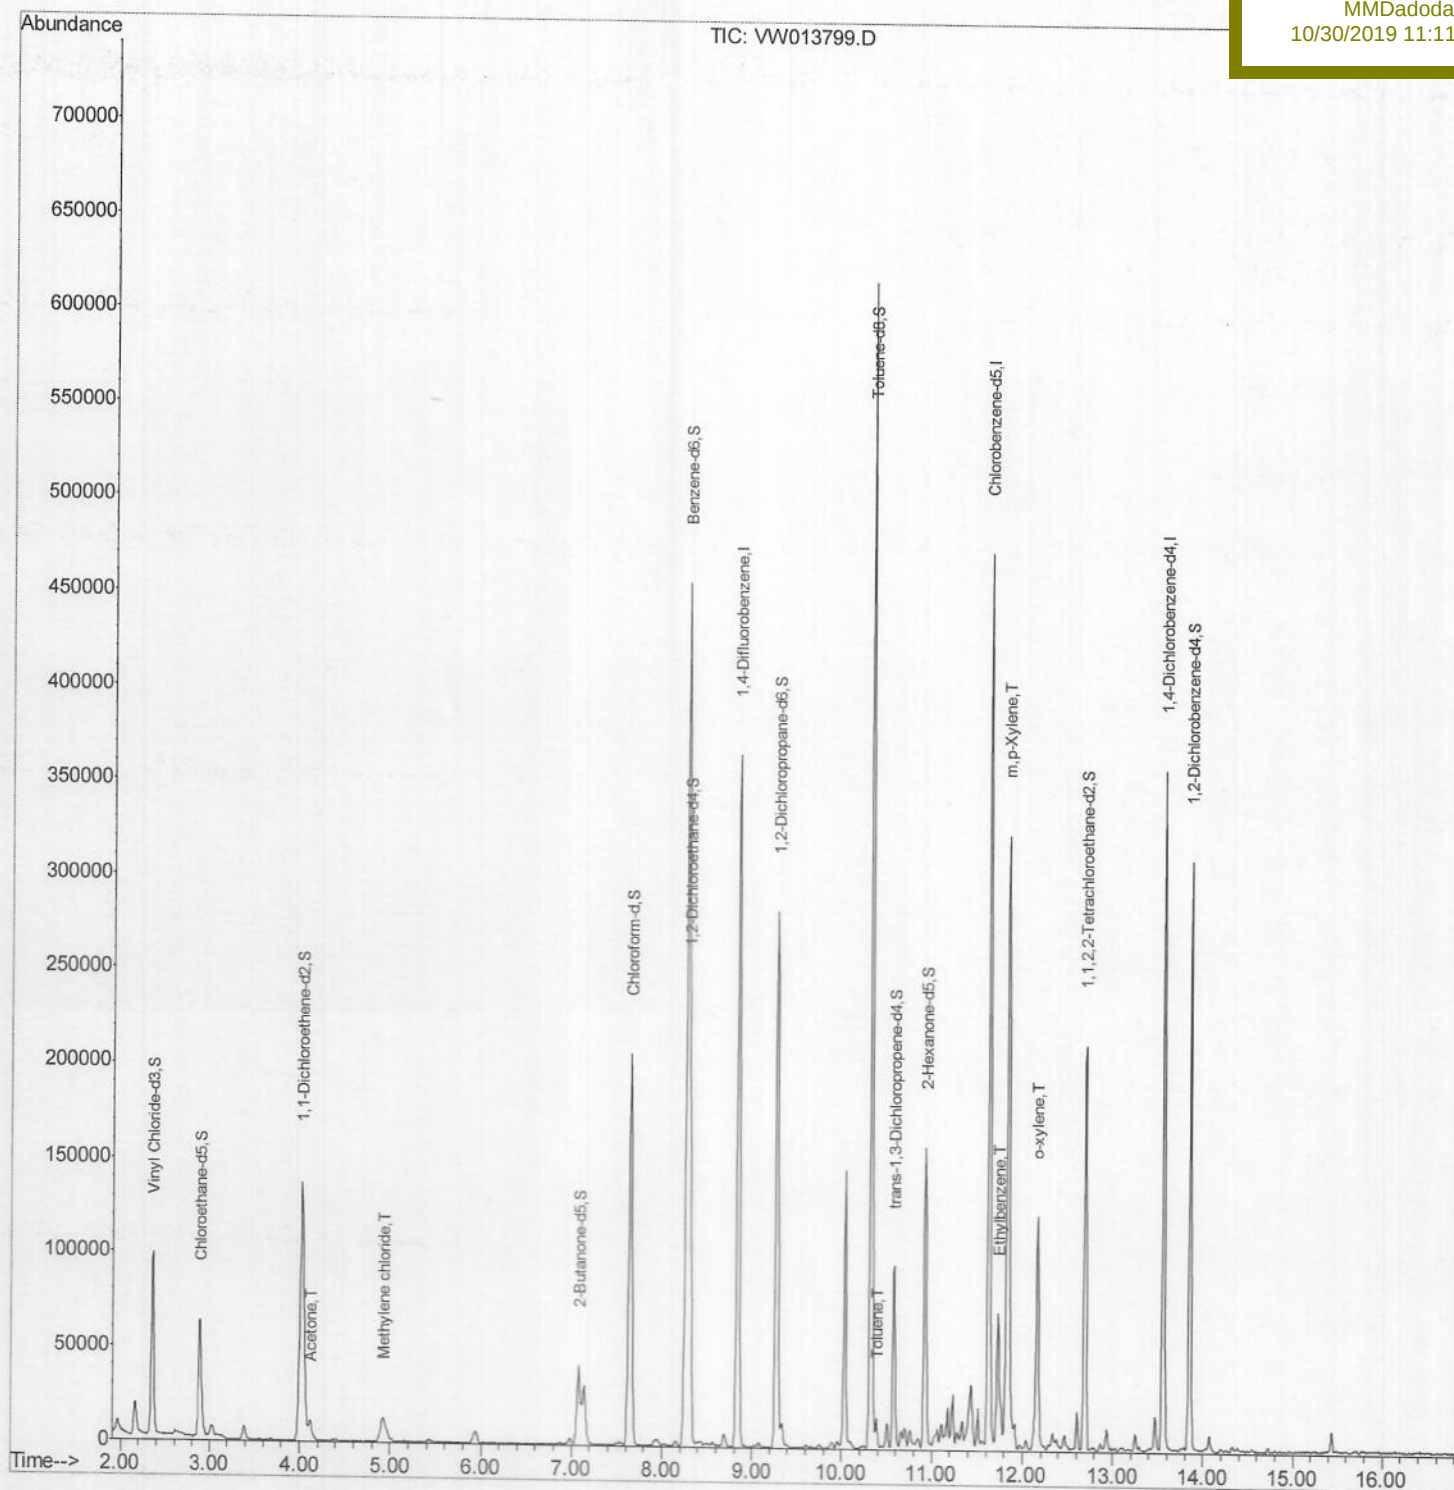




Data File : VW013799.D
Acq On : 29 Oct 2019 17:46
Operator : SY/VA
Sample : K5535-11
Misc : 6.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 07:03:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 30 06:58:53 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
BEK33

Manual Integrations
APPROVED

MMDadoda
10/30/2019 11:11:58 AM

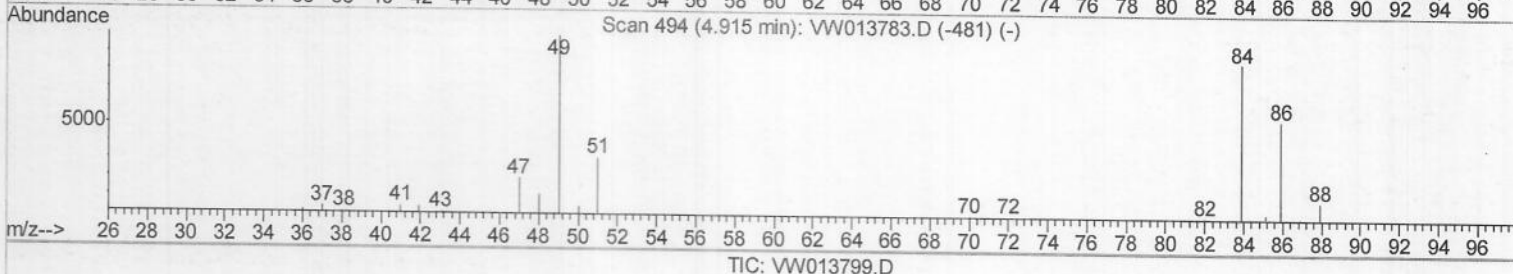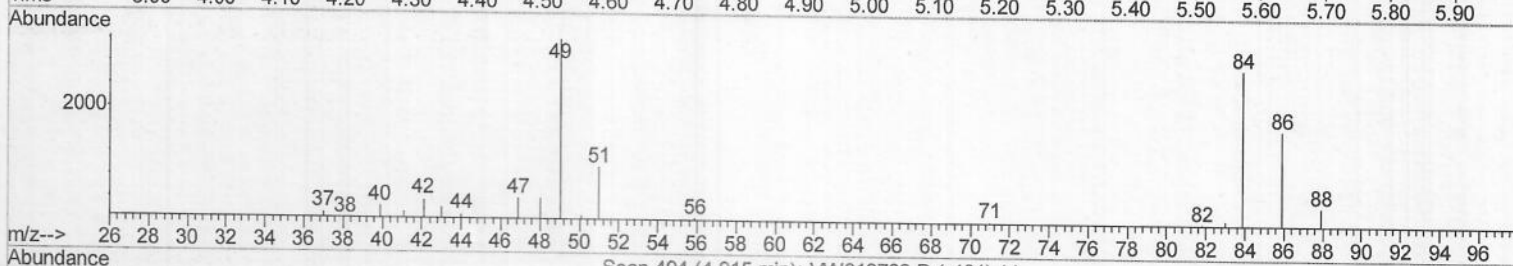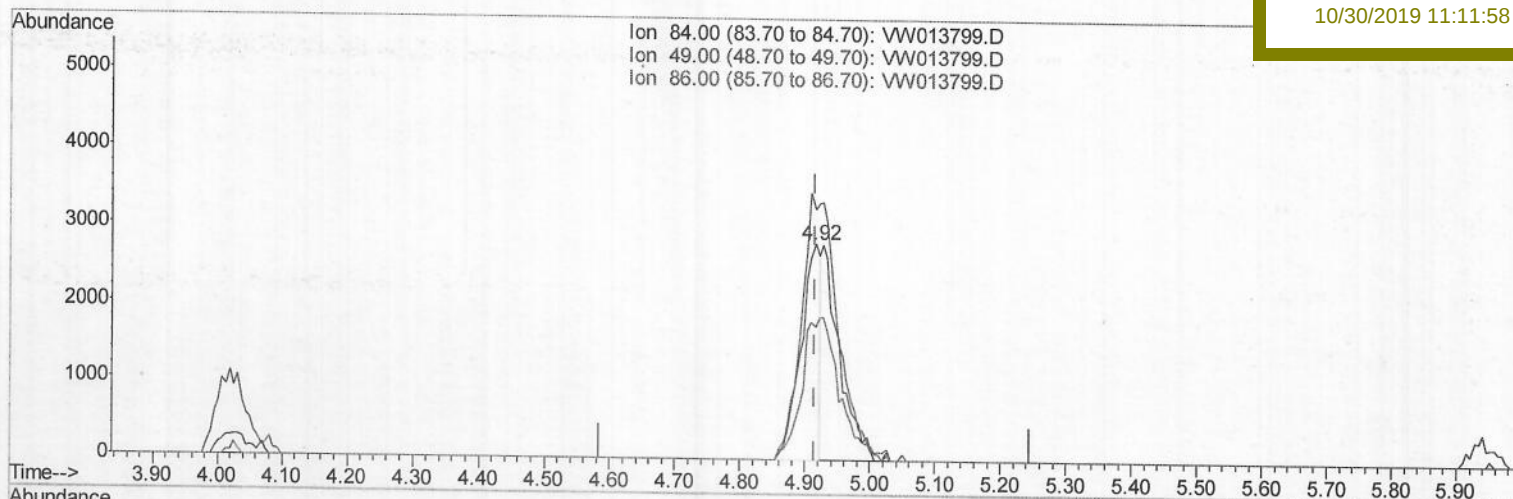

(16) Methylene chloride (T)

4.915min (+0.000) 0.91ug/L

response 5701

Ion	Exp%	Act%
84.00	100	100
49.00	114.50	115.70
86.00	61.00	61.62
0.00	0.00	0.00

Data File : VW013799.D

Acq On : 29 Oct 2019 17:46

Operator : SY/VA

Sample : K5535-11

Misc : 6.36G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 30 07:03:26 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M

Quant Title : VOC Analysis

QLast Update : Wed Oct 30 06:58:53 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :




BEK33

Manual Integrations

APPROVED

MMDadoda

10/30/2019 11:11:58 AM

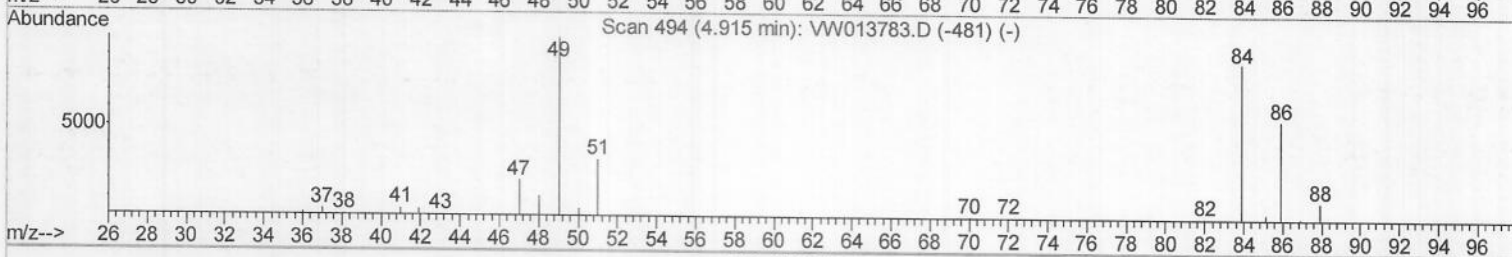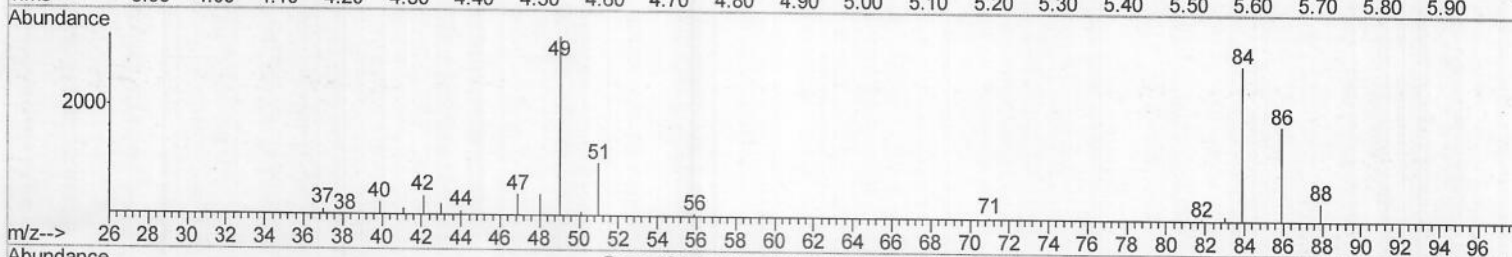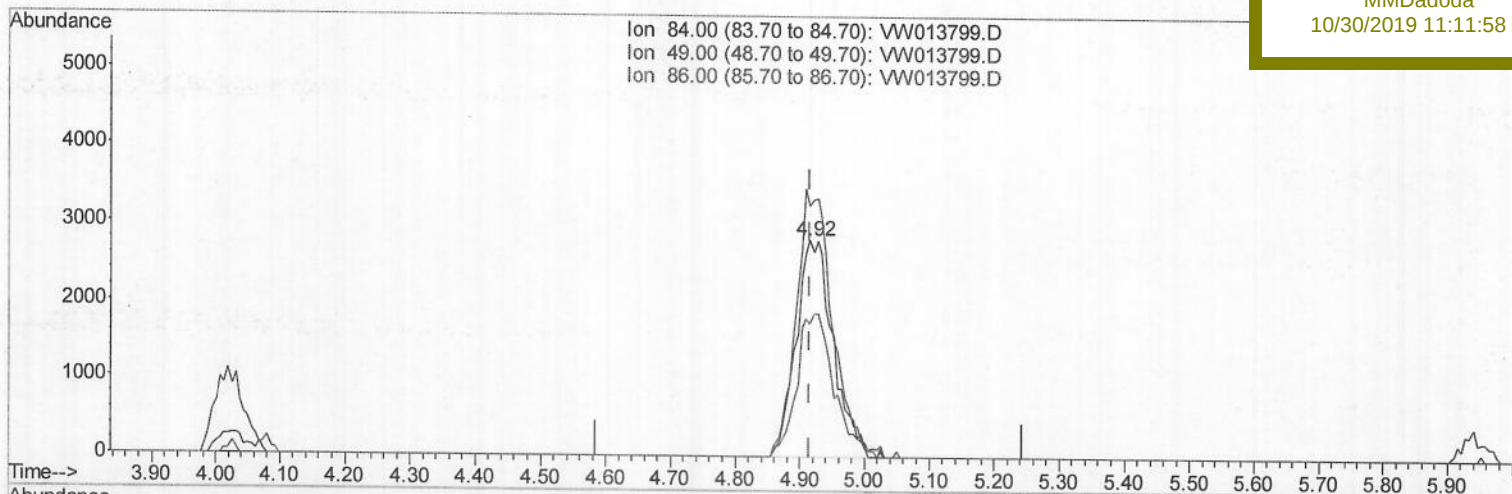

TIC: VW013799.D

(16) Methylene chloride (T)

4.915min (+0.000) 1.77ug/L m

response 11053

Ion	Exp%	Act%
-----	------	------

84.00	100	100
-------	-----	-----

49.00	114.50	115.70
-------	--------	--------

86.00	61.00	61.62
-------	-------	-------

0.00	0.00	0.00
------	------	------

Data File : VW013799.D
Acq On : 29 Oct 2019 17:46
Operator : SY/VA
Sample : K5535-11
Misc : 6.36G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BEK33

Quant Time: Oct 30 08:04:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 30 06:58:53 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
10/30/2019 11:11:58 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	325960	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	281601	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	104007	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	108659	27.17	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	108.68%	
7) Chloroethane-d5	2.89	69	87006	23.31	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	93.24%	
10) 1,1-Dichloroethene-d2	4.02	63	156970	17.77	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	71.08%	
20) 2-Butanone-d5	7.07	46	69363	48.49	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	96.98%	
24) Chloroform-d	7.65	84	219988	24.12	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	96.48%	
26) 1,2-Dichloroethane-d4	8.30	65	120795	25.33	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	101.32%	
29) Benzene-d6	8.27	84	464524	27.46	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	109.84%	
33) 1,2-Dichloropropane-d6	9.27	67	139430	27.59	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	110.36%	
37) Toluene-d8	10.32	98	405733	26.00	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	104.00%	
38) trans-1,3-Dichloropropene-	10.58	79	56010	24.57	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	98.28%	
39) 2-Hexanone-d5	10.93	63	53329	55.21	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	110.42%	
48) 1,1,2,2-Tetrachloroethane-	12.69	84	106008	25.61	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	102.44%	
61) 1,2-Dichlorobenzene-d4	13.85	152	88002	23.94	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	95.76%	

Target Compounds

					Qvalue
13) Acetone	4.12	43	17187	10.826 ug/L	96
16) Methylene chloride	4.92	84	11053m	1.771 ug/L	96
44) Toluene	10.39	91	10522	0.485 ug/L	95
53) Ethylbenzene	11.73	91	46816	1.952 ug/L	95
54) m,p-Xylene	11.83	106	96648	10.427 ug/L	99
55) o-xylene	12.16	106	32597	3.706 ug/L	97

3 MD 11/07/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed