

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102919\
 Data File : VW013800.D
 Acq On : 29 Oct 2019 18:13
 Operator : SY/VA
 Sample : K5565-01
 Misc : 5.35G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JLNA0

Manual Integrations
 APPROVED

MMDadoda
 10/30/2019 11:12:04 AM

Quant Time: Oct 30 07:09:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 30 06:58:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	252041	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	222671	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	99475	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	89043	28.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.16%
7) Chloroethane-d5	2.89	69	73033	25.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.20%
10) 1,1-Dichloroethene-d2	4.02	63	126664	18.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.20%
20) 2-Butanone-d5	7.07	46	50180	45.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.74%
24) Chloroform-d	7.65	84	178255	25.28	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.12%
26) 1,2-Dichloroethane-d4	8.31	65	95035	25.77	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.08%
29) Benzene-d6	8.27	84	369203	27.60	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.40%
33) 1,2-Dichloropropane-d6	9.27	67	113839	28.49	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.96%
37) Toluene-d8	10.32	98	315698	25.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.36%
38) trans-1,3-Dichloropropene-	10.58	79	41717	23.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.60%
39) 2-Hexanone-d5	10.93	63	38938	50.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	80546	24.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	86002	24.46	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.84%

Target Compounds					Ovalue
13) Acetone	4.12	43	4252	3.464 ug/L	95
16) Methylene chloride	4.92	84	7781m	1.612 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102919\
Data File : VW013800.D
Acq On : 29 Oct 2019 18:13
Operator : SY/VA
Sample : K5565-01
Misc : 5.35G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
JLNA0

Manual Integrations
APPROVED

MMDadoda
10/30/2019 11:12:04 AM

Quant Time: Oct 30 07:09:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 30 06:58:53 2019
Response via : Initial Calibration

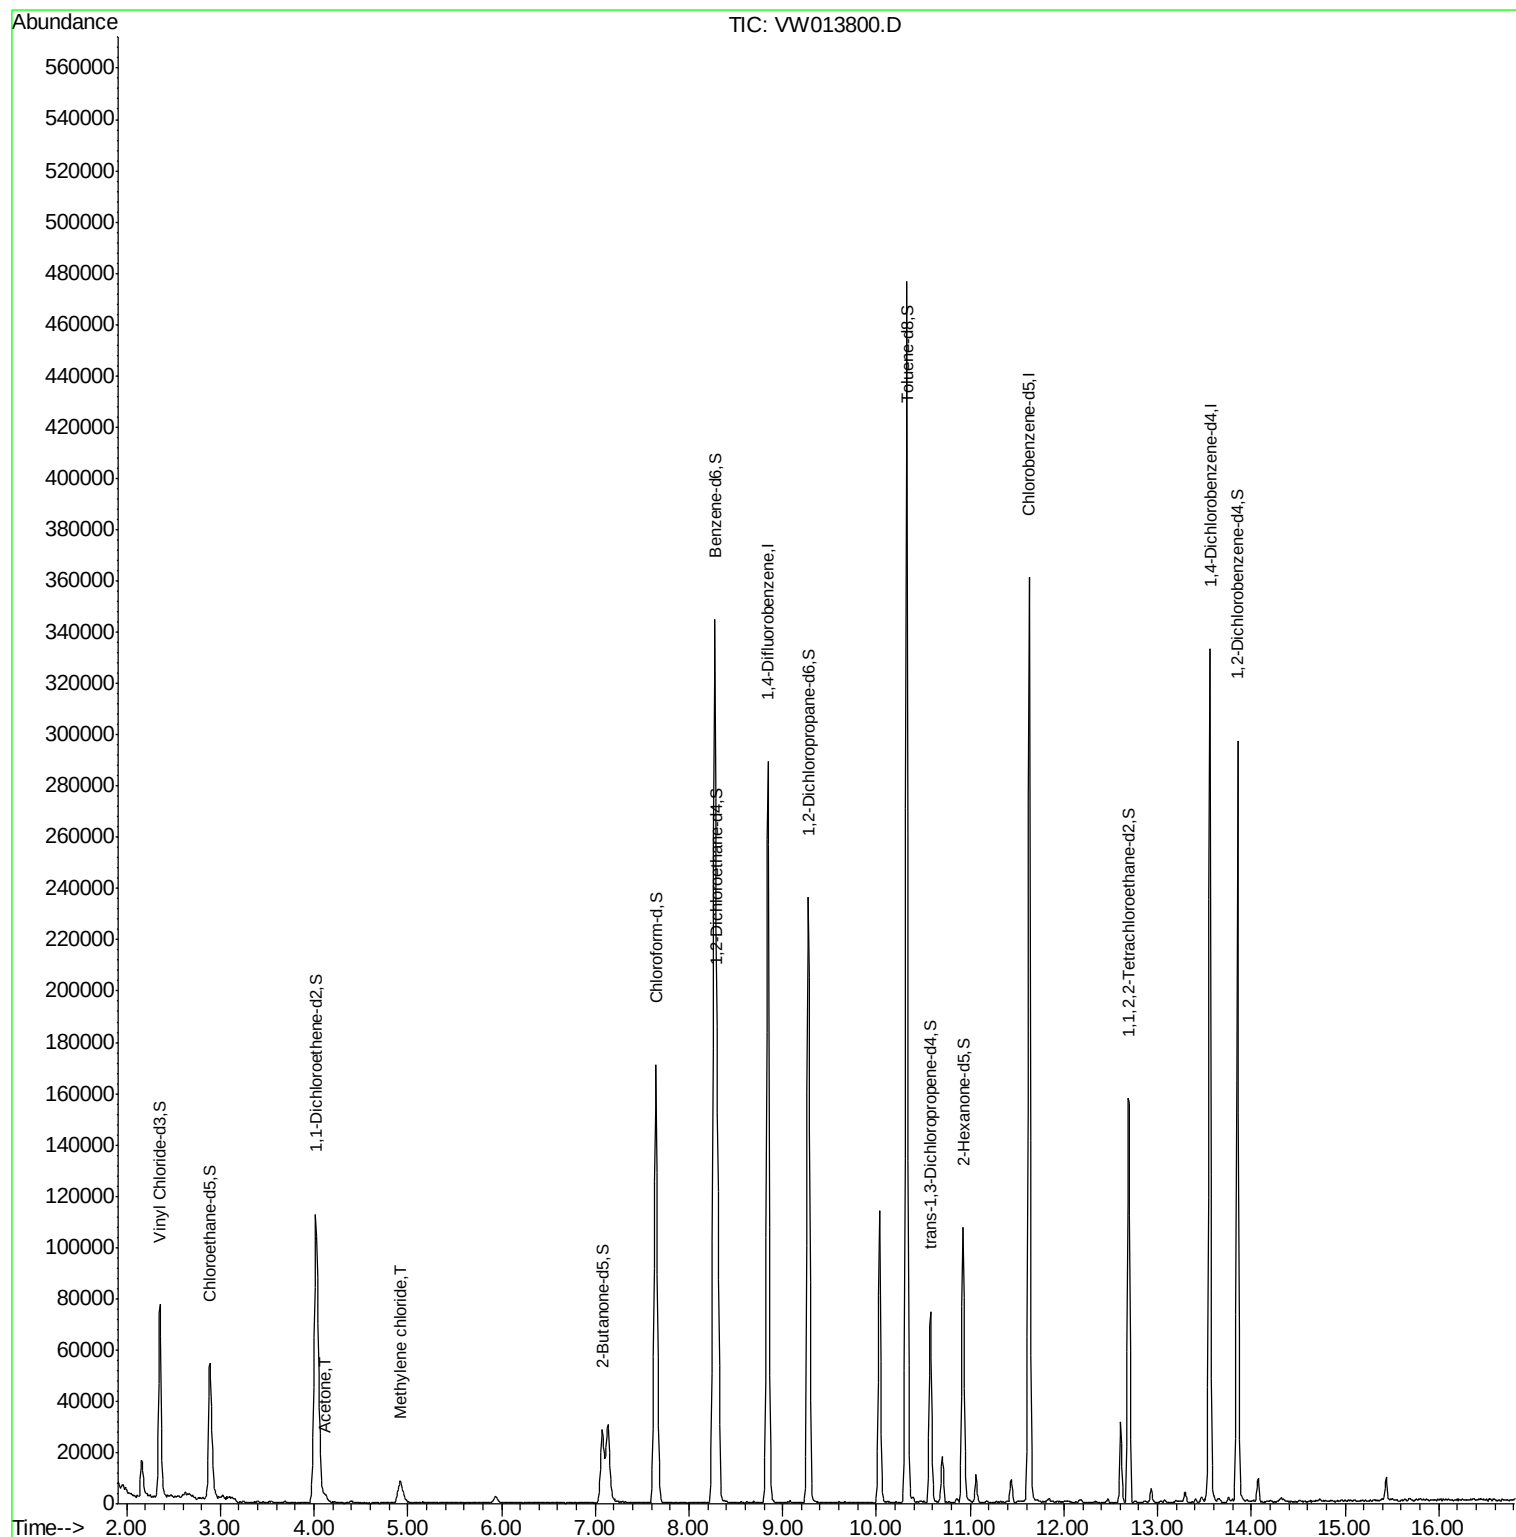

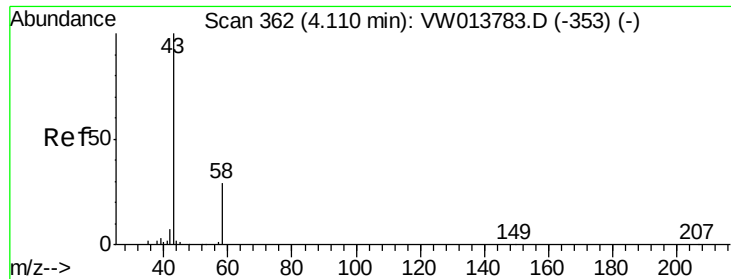

#13

Acetone

Concen: 3.464 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW013800.D

Acq: 29 Oct 2019 18:13

Instrument :

MSVOA_W

ClientSampleId :

JLNA0

Tot Ion: 43 Resp: 4252

Ion Ratio Lower Upper

43 100


58 38.3 0.0 70.4

Manual Integrations

APPROVED




MMDadoda

10/30/2019 11:12:04 AM

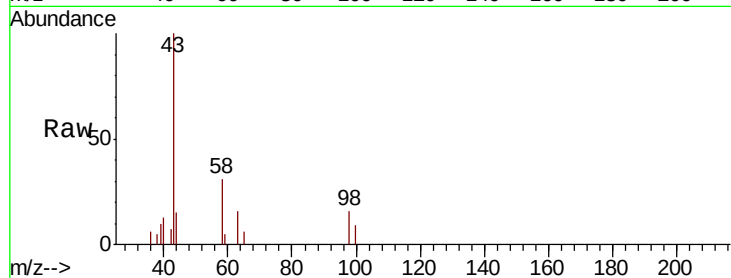

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

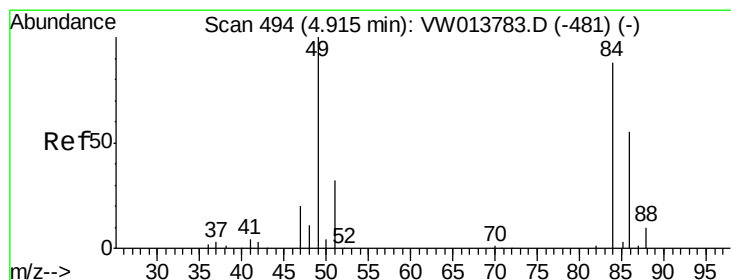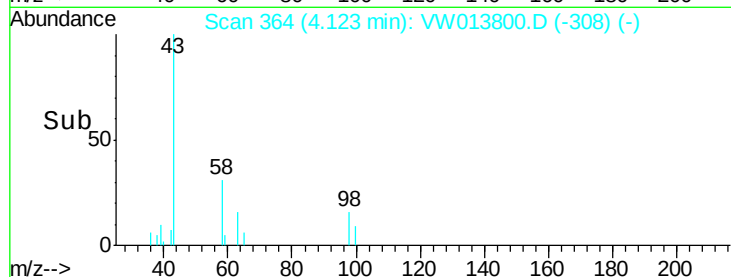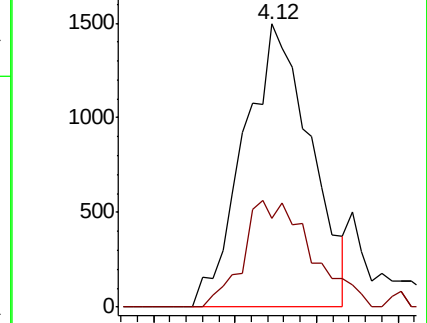

#16

Methylene chloride

Concen: 1.612 ug/L m

RT: 4.92 min Scan# 494

Delta R.T. 0.00 min

Lab File: VW013800.D

Acq: 29 Oct 2019 18:13


Tgt Ion: 84 Resp: 7781

Ion Ratio Lower Upper

84 100

49 119.5 80.2 148.9

86 65.2 42.7 79.3

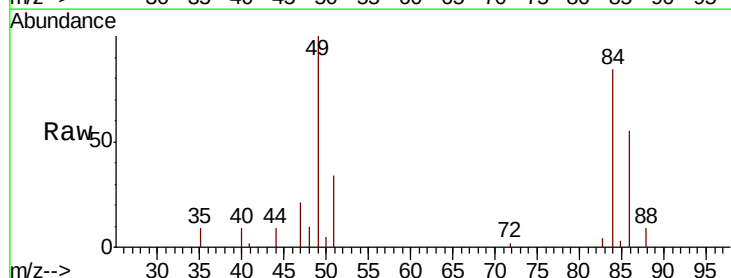

Abundance Ion 84.00 (83.70 to 84.70): VW

Ion 49.00 (48.70 to 49.70): VW

Ion 86.00 (85.70 to 86.70): VW

