

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102919\
 Data File : VW013818.D
 Acq On : 30 Oct 2019 02:57
 Operator : SY/VA
 Sample : K5549-14
 Misc : 5.12G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAQ67

Quant Time: Oct 30 08:04:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 30 08:16:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	284748	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	284826	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	150446	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	91165	26.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.36%
7) Chloroethane-d5	2.89	69	72794	22.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.28%
10) 1,1-Dichloroethene-d2	4.02	63	137755	17.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.40%
20) 2-Butanone-d5	7.07	46	84238	67.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.84%
24) Chloroform-d	7.65	84	198302	24.89	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.56%
26) 1,2-Dichloroethane-d4	8.31	65	118165	28.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	113.44%
29) Benzene-d6	8.27	84	414059	24.20	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.80%
33) 1,2-Dichloropropane-d6	9.27	67	131729	25.77	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.08%
37) Toluene-d8	10.32	98	380280	24.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.40%
38) trans-1,3-Dichloropropene-	10.58	79	56491	24.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.00%
39) 2-Hexanone-d5	10.92	63	73049	74.77	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	149.54%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	134012	32.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	128.04%#
61) 1,2-Dichlorobenzene-d4	13.85	152	144815	27.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.96%


Target Compounds					Ovalue
13) Acetone	4.12	43	20473	14.762 ug/L	95
44) Toluene	10.39	91	11434	0.521 ug/L	96
47) Tetrachloroethene	10.86	164	5773	1.203 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102919\
Data File : VW013818.D
Acq On : 30 Oct 2019 02:57
Operator : SY/VA
Sample : K5549-14
Misc : 5.12G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAQ67

Quant Time: Oct 30 08:04:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 30 08:16:17 2019
Response via : Initial Calibration

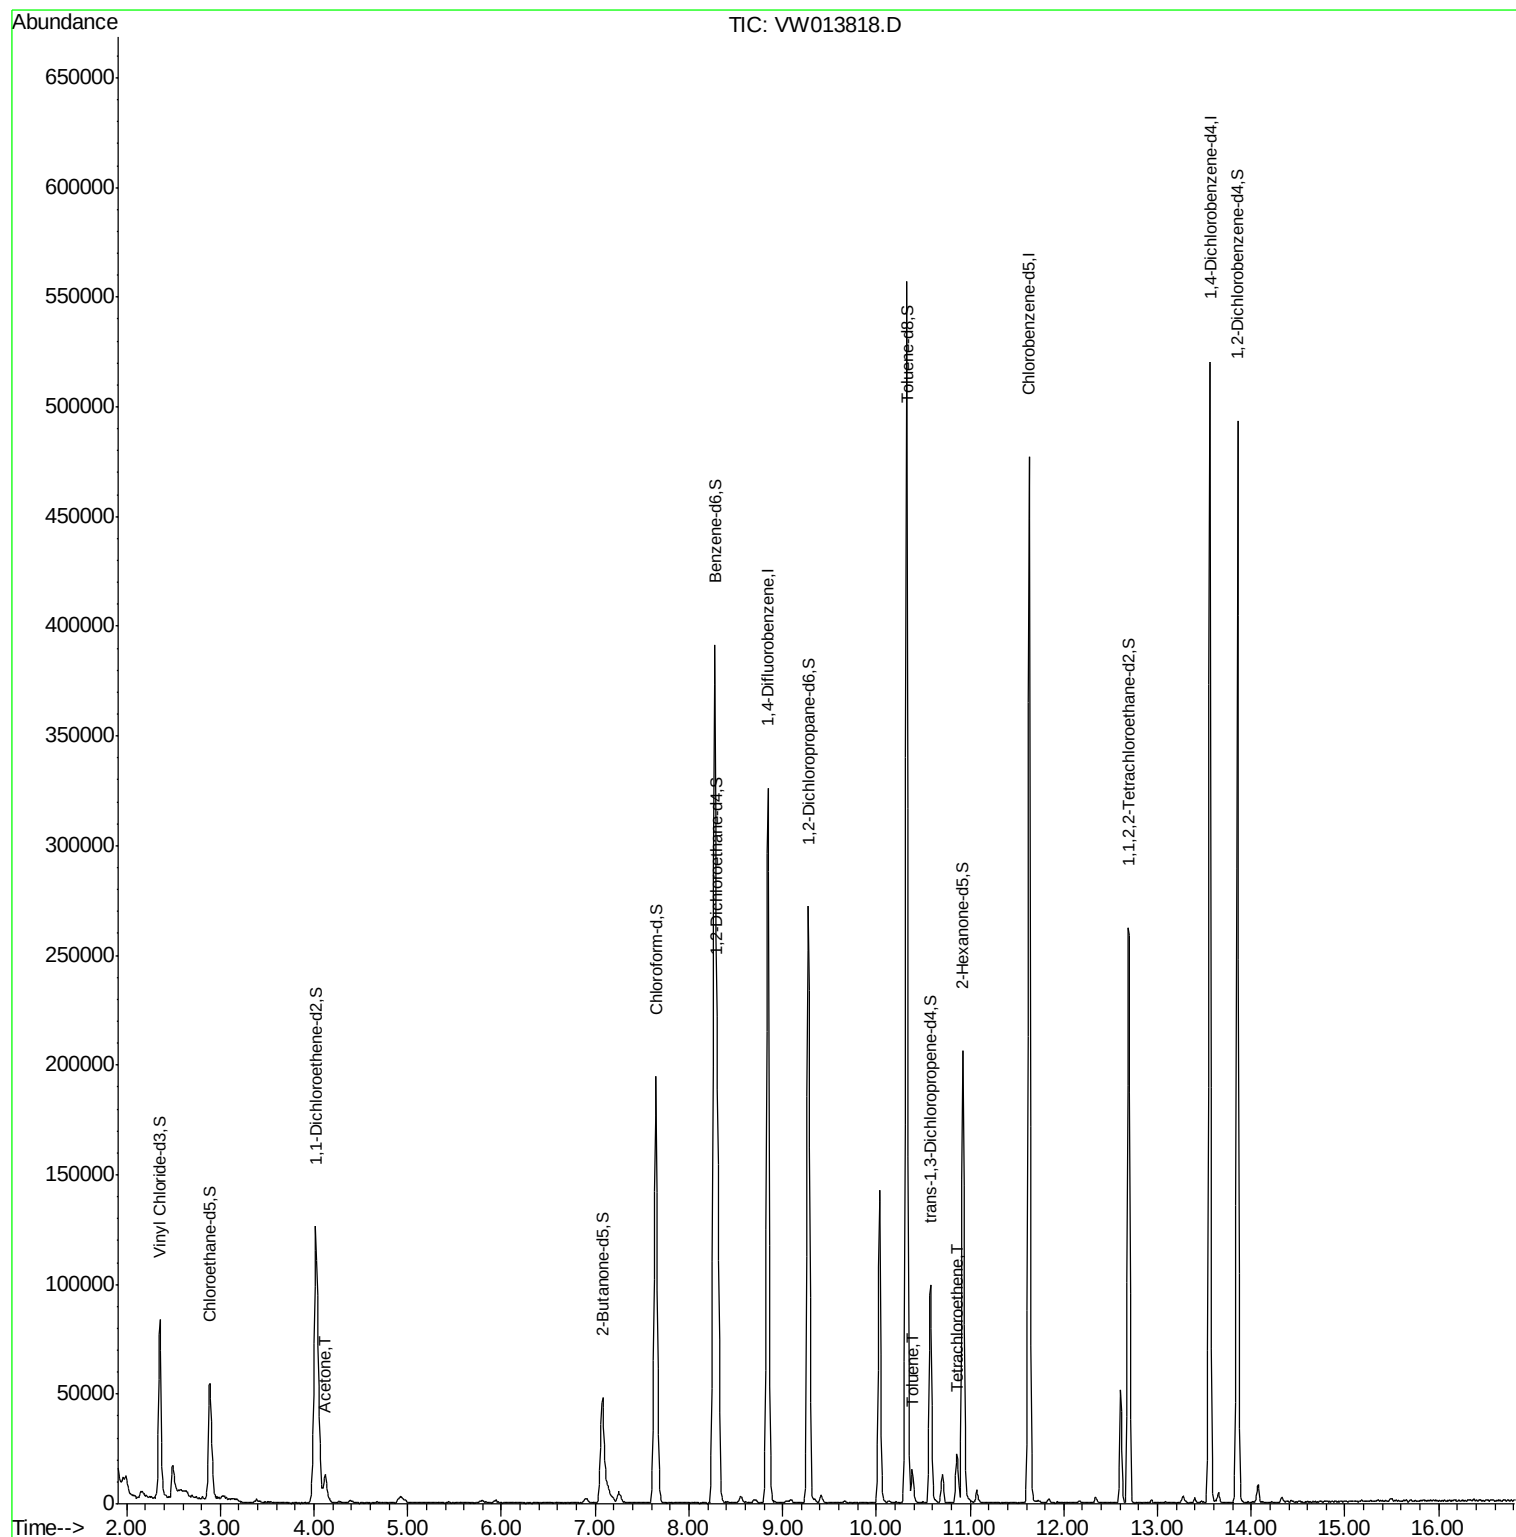

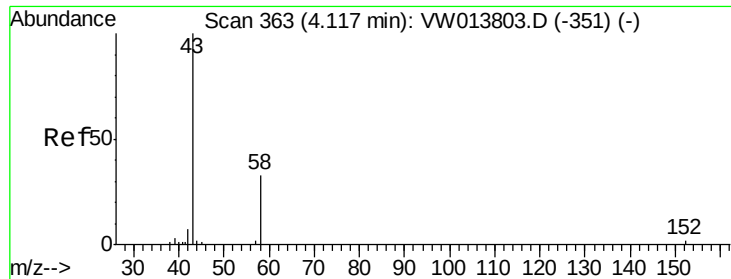

#13

Acetone

Concen: 14.762 ug/L

RT: 4.12 min Scan# 363

Delta R.T. 0.00 min

Lab File: VW013818.D

Acq: 30 Oct 2019 02:57

Instrument :

MSVOA_W

ClientSampleId :





GAQ67

Tot Ion: 43 Resp: 20473

Ion Ratio Lower Upper

43 100

58 32.1 0.0 70.4

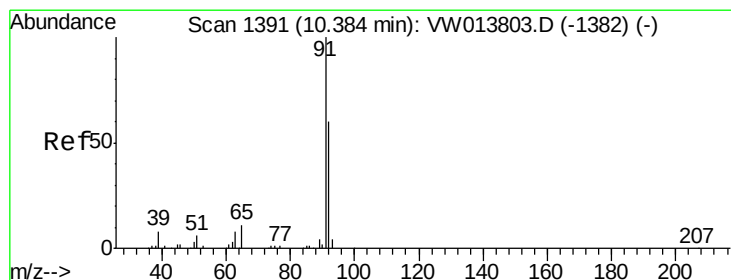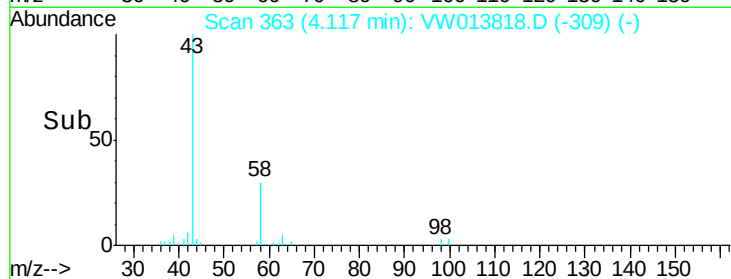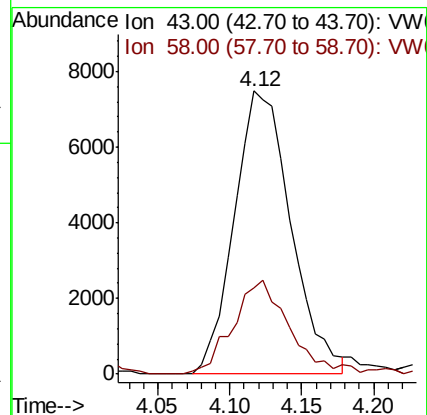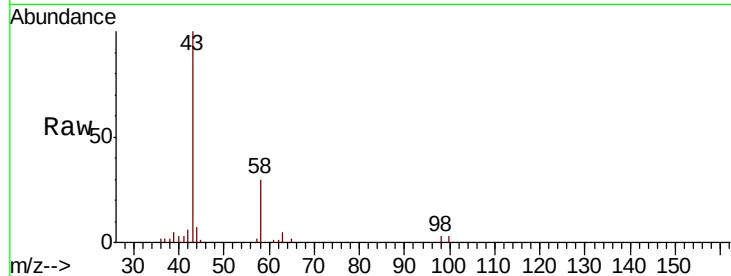

#44

Toluene

Concen: 0.521 ug/L

RT: 10.39 min Scan# 1392

Delta R.T. 0.01 min

Lab File: VW013818.D




Acq: 30 Oct 2019 02:57


Tgt Ion: 91 Resp: 11434

Ion Ratio Lower Upper

91 100

92 56.9 42.0 78.0

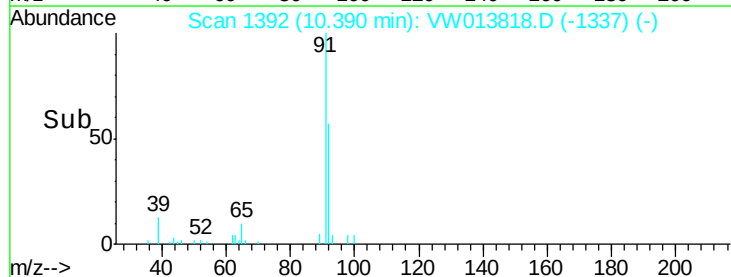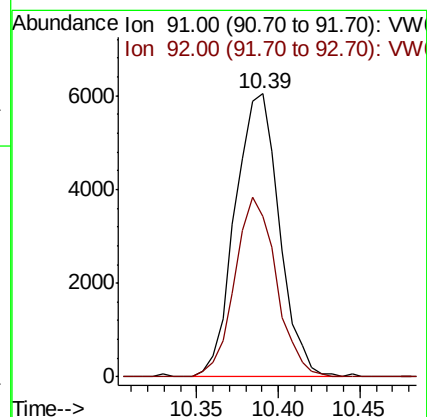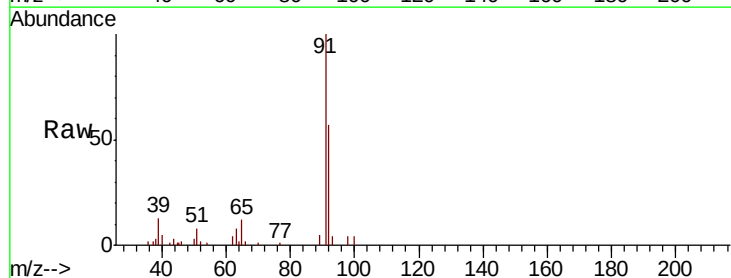

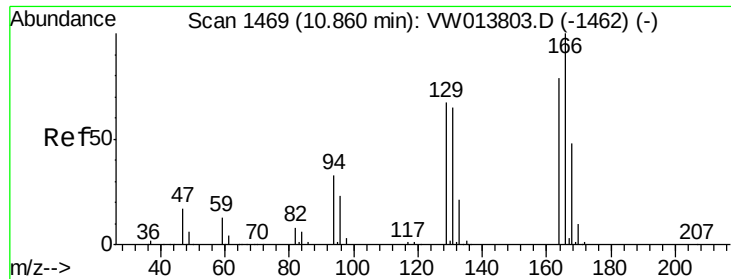

#47

Tetrachloroethene

Concen: 1.203 ug/L

RT: 10.86 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VW013818.D


Acq: 30 Oct 2019 02:57

Instrument :

MSVOA_W

ClientSampleId :

GAQ67

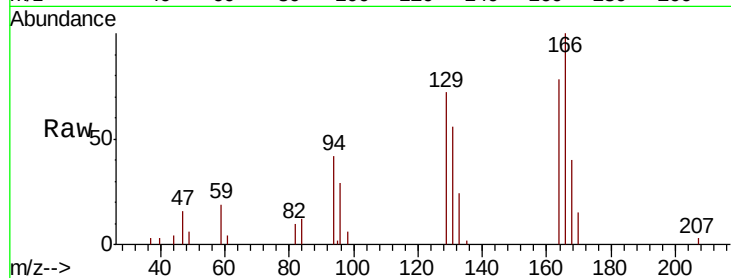

Tot Ion:164 Resp: 5773

Ion Ratio Lower Upper

164 100

129 92.9 61.8 114.8

131 72.2 59.2 110.0

166 128.8 89.2 165.8

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

