
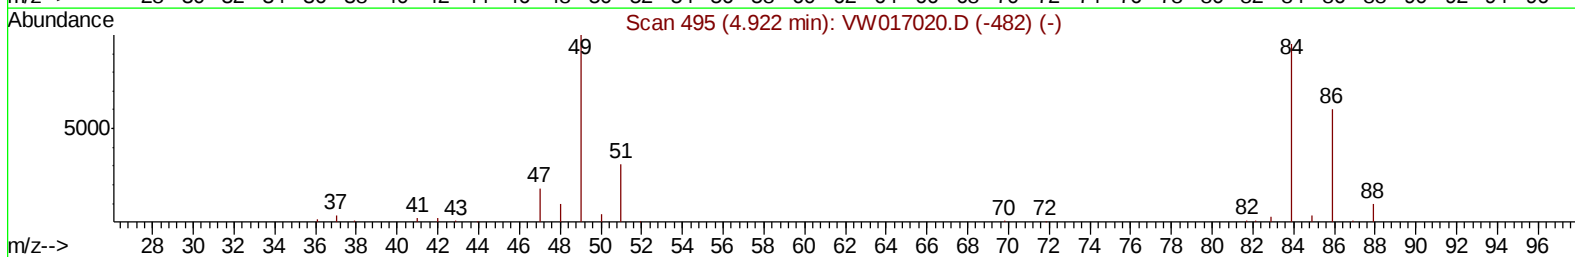
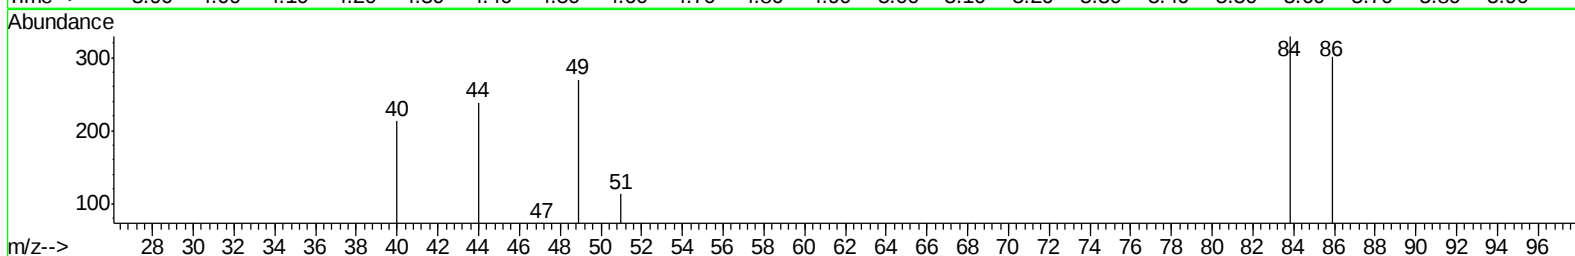


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
Data File : VW017026.D
Acq On : 29 Oct 2020 15:27
Operator : SY/VA
Sample : L4543-05
Misc : 5.71G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 30 02:40:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 30 01:03:22 2020
Response via : Initial Calibration

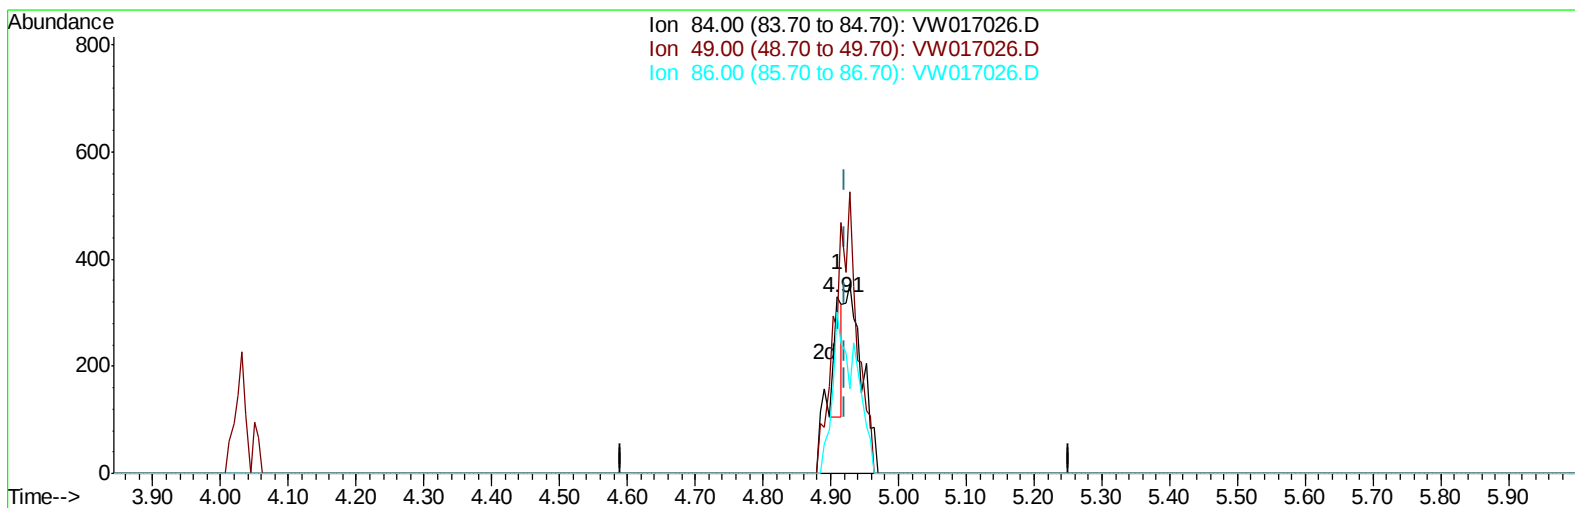

TIC: VW017026.D

(16) Methylene chloride (T)

4.909min (-0.012) 0.43ug/L

response 197

Ion	Exp%	Act%
84.00	100	100
49.00	105.40	82.07
86.00	67.70	91.49#
0.00	0.00	0.00