
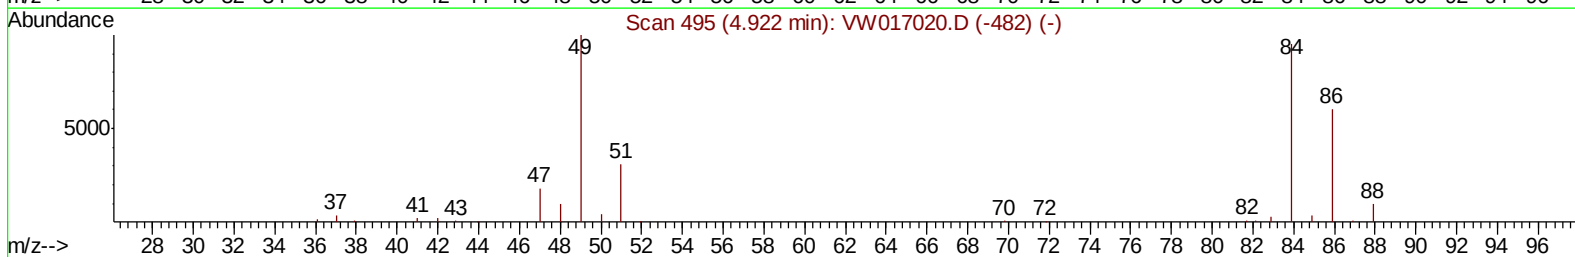
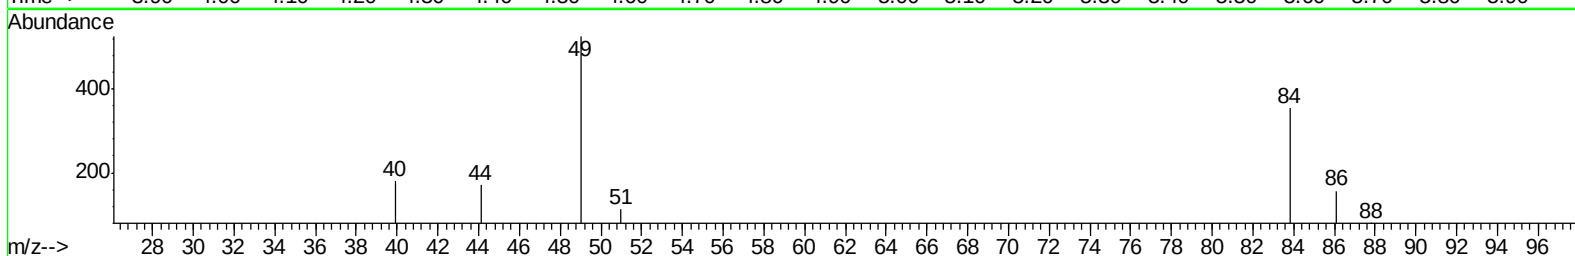


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102920\
Data File : VW017026.D
Acq On : 29 Oct 2020 15:27
Operator : SY/VA
Sample : L4543-05
Misc : 5.71G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Oct 30 02:40:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 30 01:03:22 2020
Response via : Initial Calibration

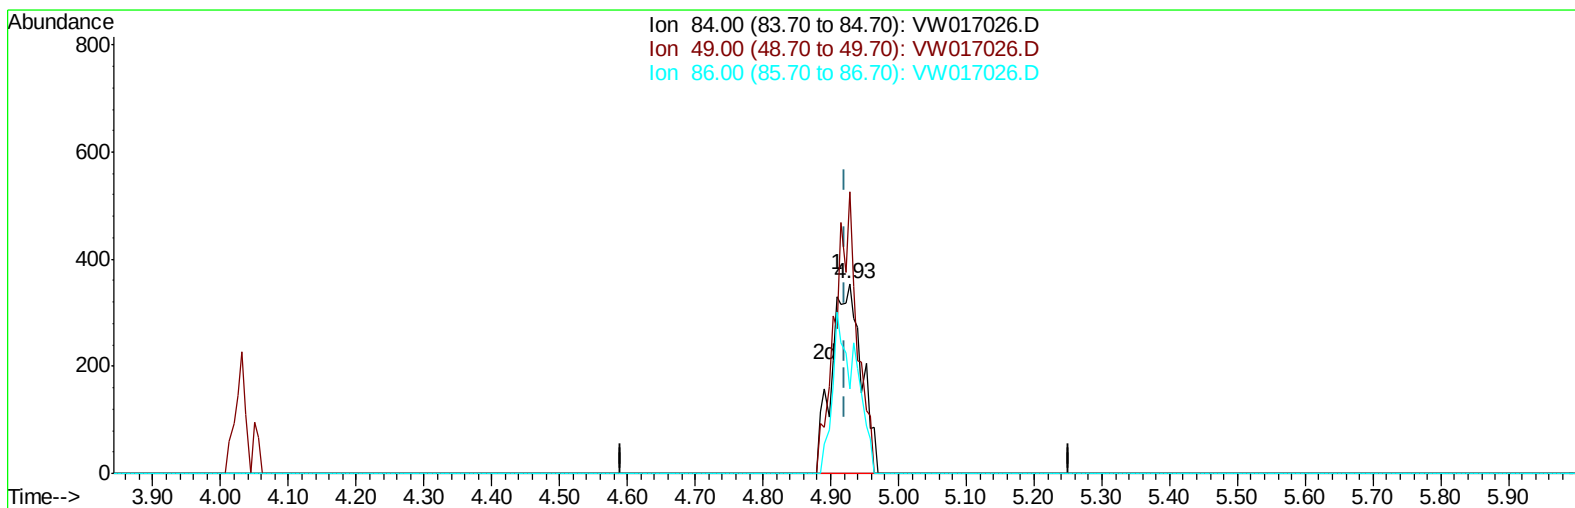

TIC: VW017026.D

(16) Methylene chloride (T)

4.928min (+0.006) 2.41ug/L m

response 1096

Ion	Exp%	Act%
84.00	100	100
49.00	105.40	148.59#
86.00	67.70	44.35#
0.00	0.00	0.00