

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
 Data File : VW017026.D
 Acq On : 29 Oct 2020 15:27
 Operator : SY/VA
 Sample : L4543-05
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG446

Manual Integrations
 APPROVED

MMDadoda
 11/4/2020 11:31:09 AM

Quant Time: Oct 30 02:40:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 30 01:03:22 2020
 Response via : Initial Calibration

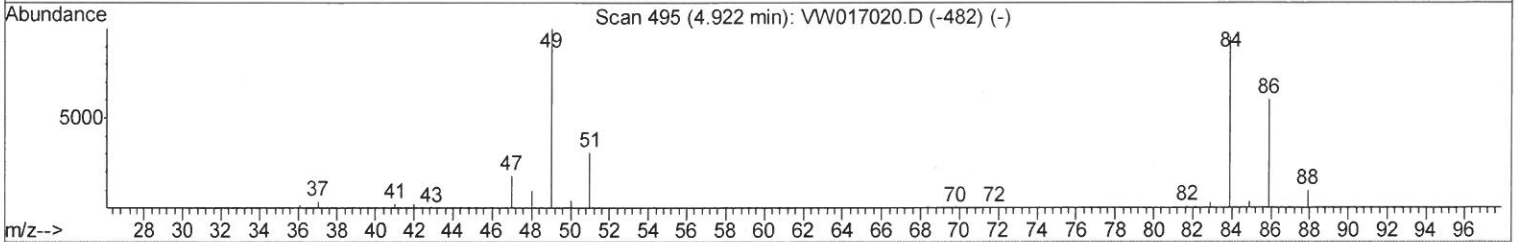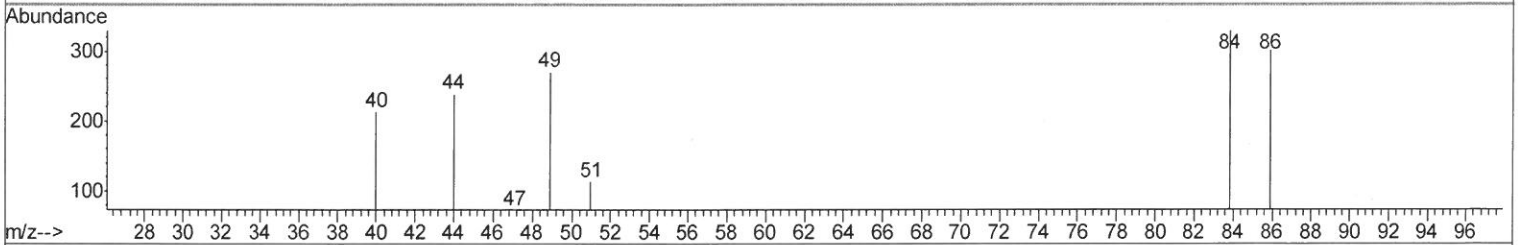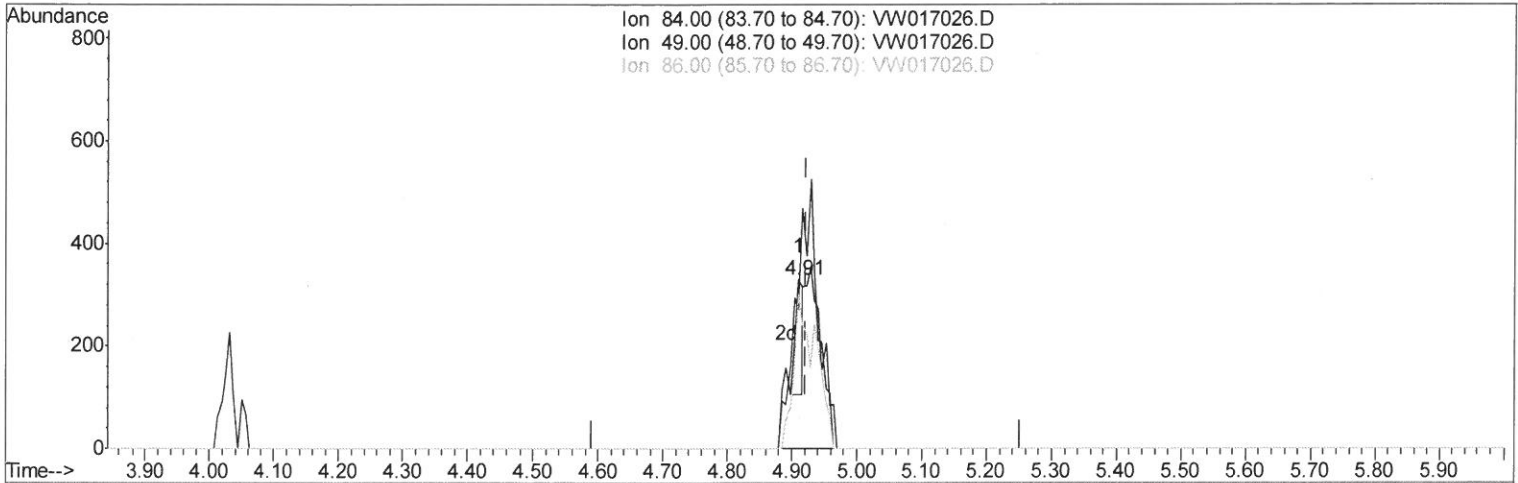

TIC: VW017026.D

(16) Methylene chloride (T)

4.909min (-0.012) 0.43ug/L

response 197

Ion	Exp%	Act%
84.00	100	100
49.00	105.40	82.07
86.00	67.70	91.49#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
Data File : VW017026.D
Acq On : 29 Oct 2020 15:27
Operator : SY/VA
Sample : L4543-05
Misc : 5.71G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG446

Manual Integrations
APPROVED

MMDadoda
11/4/2020 11:31:09 AM

Quant Time: Oct 30 02:40:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 30 01:03:22 2020
Response via : Initial Calibration

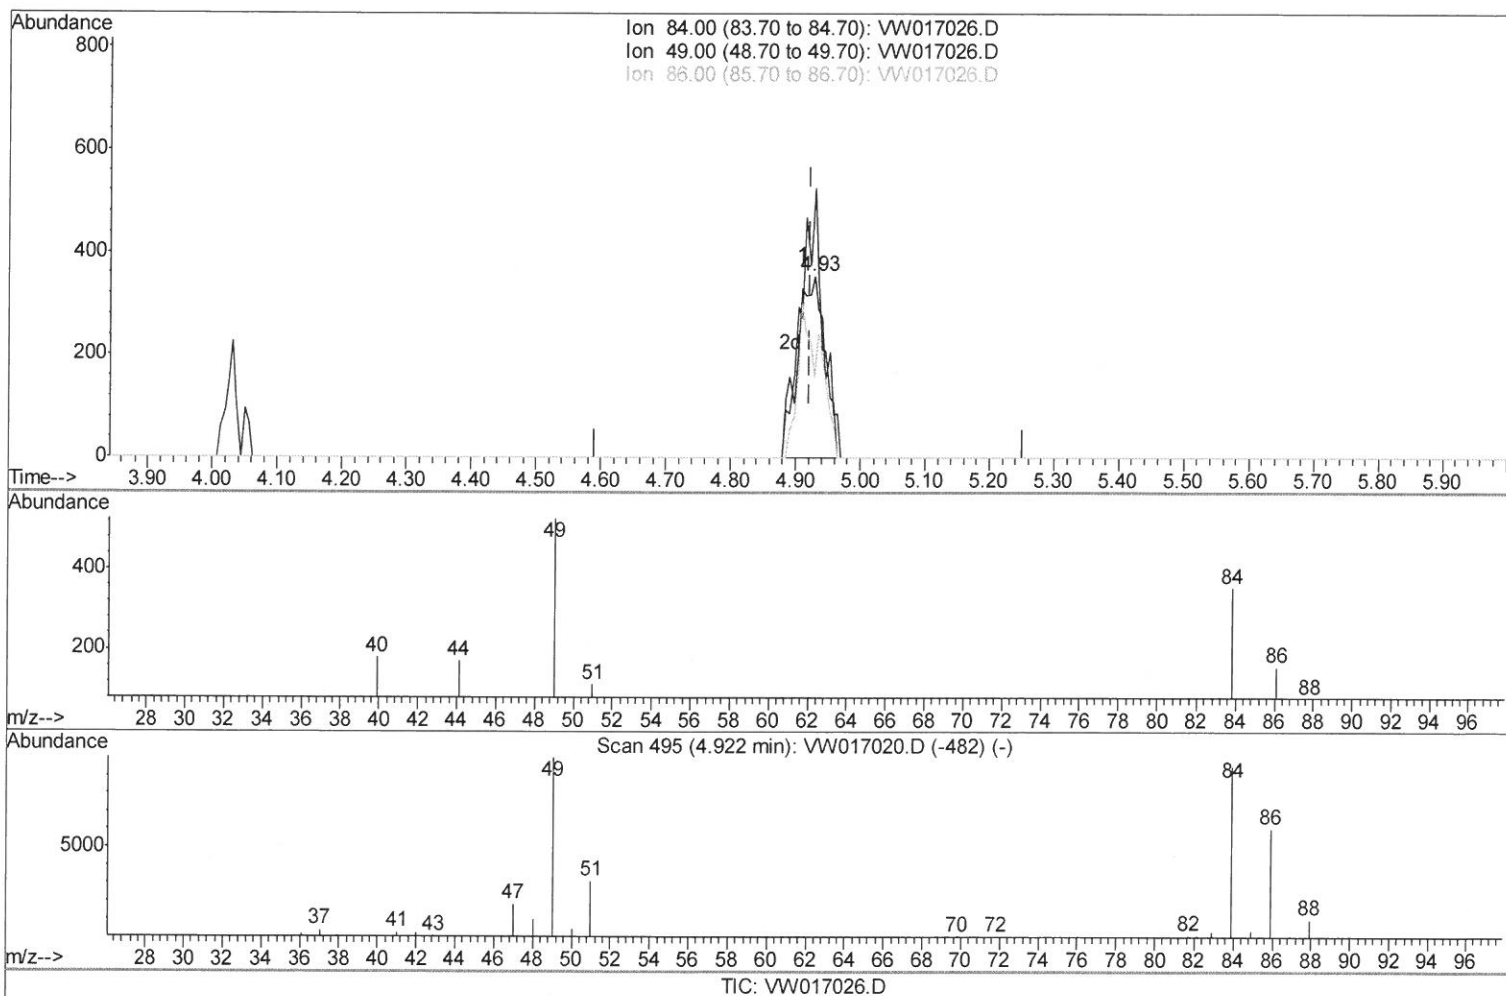

(16) Methylene chloride (T)

4.928min (+0.006) 2.41ug/L m

response 1096

Ion	Exp%	Act%
84.00	100	100
49.00	105.40	148.59#
86.00	67.70	44.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
 Data File : VW017026.D
 Acq On : 29 Oct 2020 15:27
 Operator : SY/VA
 Sample : L4543-05
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG446

Manual Integrations
 APPROVED

MMDadoda
 11/4/2020 11:31:09 AM

Quant Time: Oct 30 02:40:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 30 01:03:22 2020
 Response via : Initial Calibration

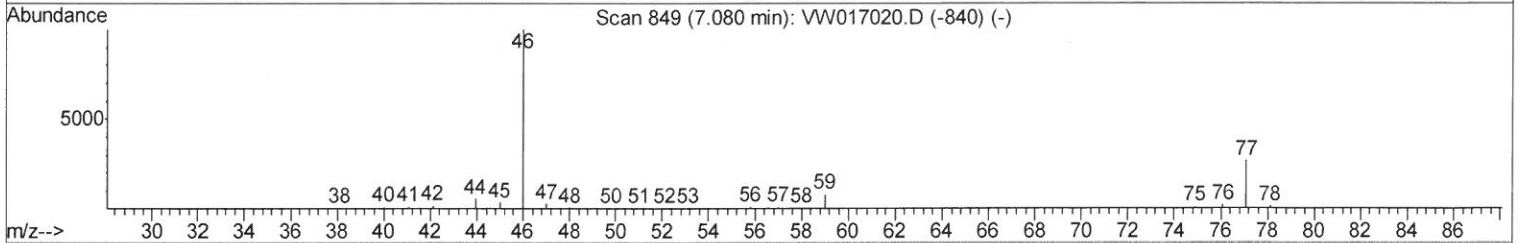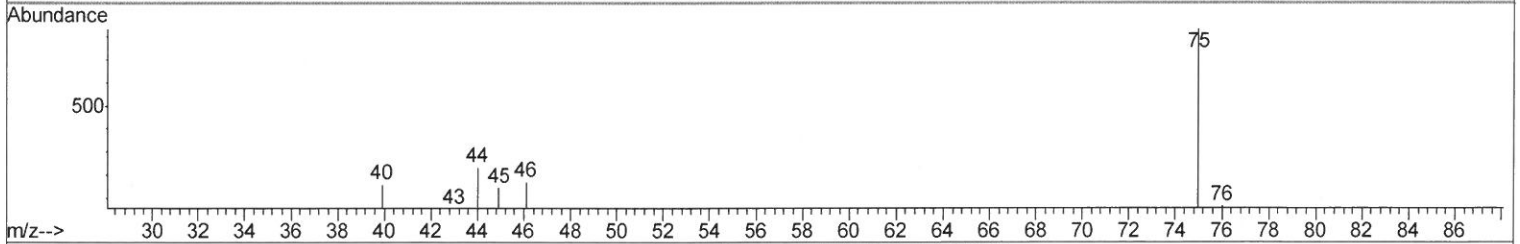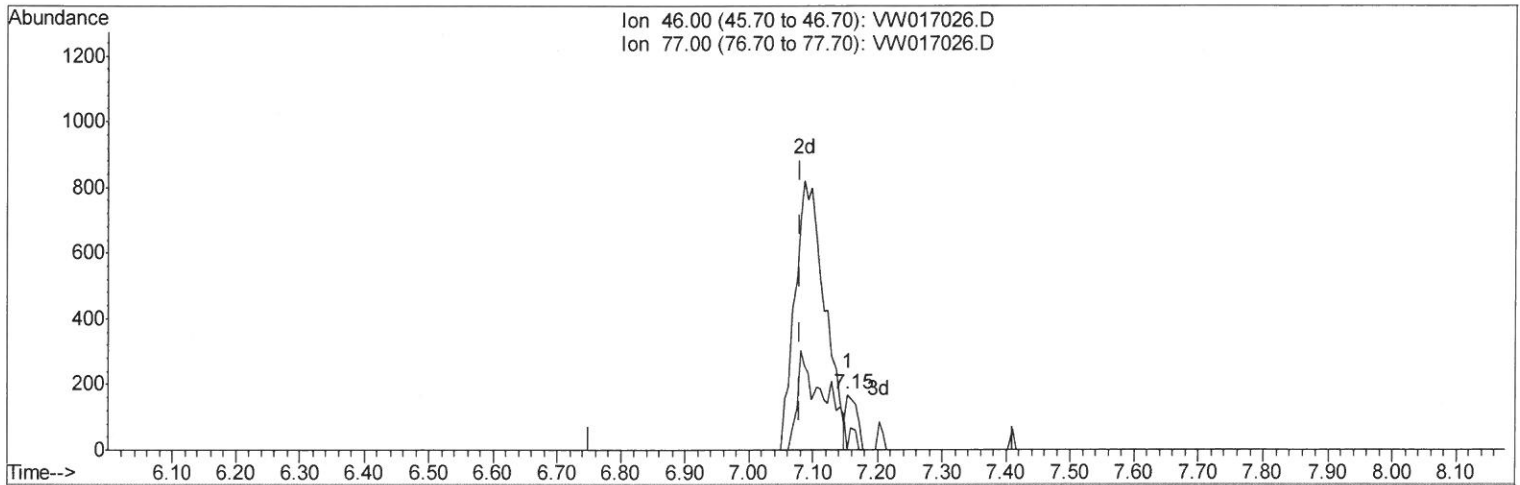

TIC: VW017026.D

(20) 2-Butanone-d5 (S)
 7.153min (+0.073) 2.69ug/L
 response 201

Ion	Exp%	Act%
46.00	100	100
77.00	29.00	23.38
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
 Data File : VW017026.D
 Acq On : 29 Oct 2020 15:27
 Operator : SY/VA
 Sample : L4543-05
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG446

Manual Integrations
 APPROVED

MMDadoda
 11/4/2020 11:31:09 AM

Quant Time: Oct 30 02:40:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 30 01:03:22 2020
 Response via : Initial Calibration

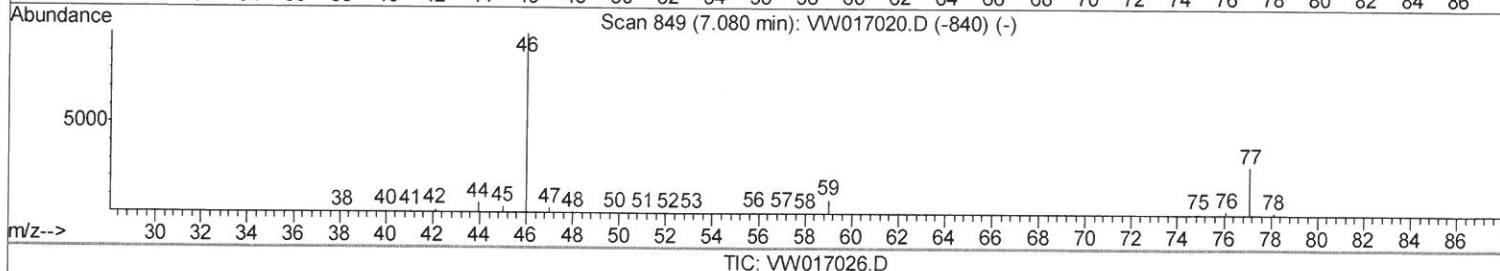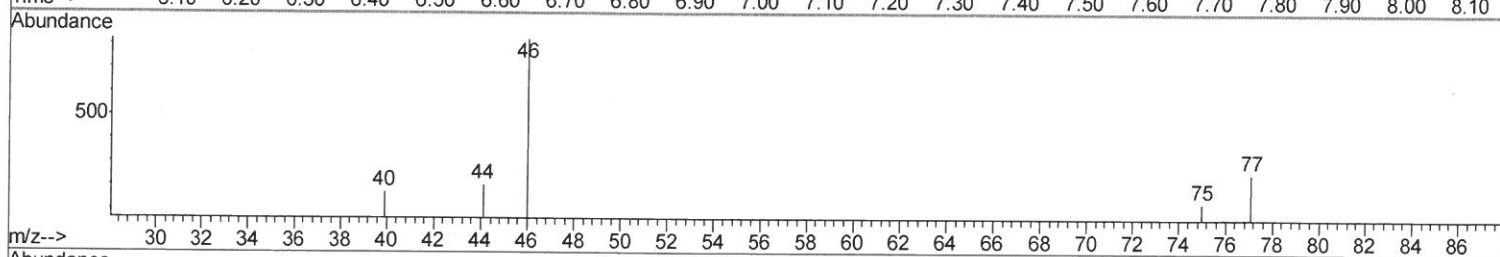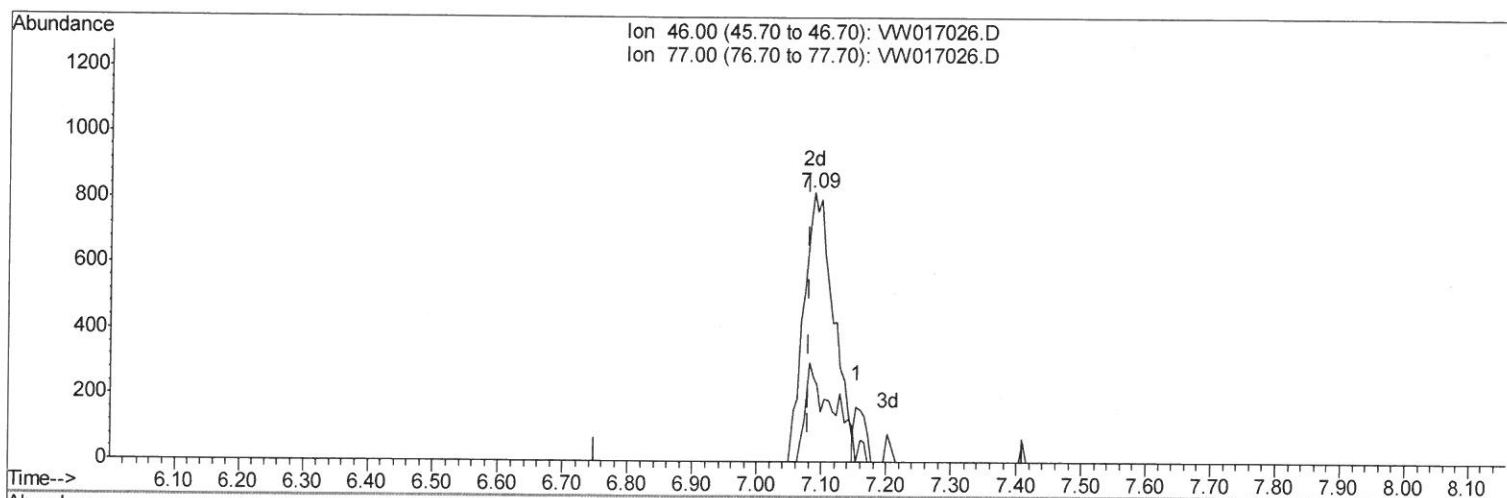

(20) 2-Butanone-d5 (S)

7.086min (+0.006) 35.06ug/L m

response 2622

Ion	Exp%	Act%
46.00	100	100
77.00	29.00	1.79#
0.00	0.00	0.00
0.00	0.00	0.00

11/06/2020 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
 Data File : VW017026.D
 Acq On : 29 Oct 2020 15:27
 Operator : SY/VA
 Sample : L4543-05
 Misc : 5.71G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG446

Manual Integrations
 APPROVED

MMDadoda
 11/4/2020 11:31:09 AM

Quant Time: Oct 30 02:42:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 30 01:03:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	34398	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	27012	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	5955	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	12104	30.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	121.96%
7) Chloroethane-d5	2.90	69	10182	33.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	132.40%
10) 1,1-Dichloroethene-d2	4.03	63	15830	20.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	82.00%
20) 2-Butanone-d5	7.09	46	2622m	35.06	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.12%
24) Chloroform-d	7.65	84	20806	26.22	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.88%
26) 1,2-Dichloroethane-d4	8.31	65	9487	25.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.64%
29) Benzene-d6	8.28	84	40685	29.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	117.28%
33) 1,2-Dichloropropane-d6	9.28	67	11178	29.85	ug/L	

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102920\
Data File : VW017026.D
Acq On : 29 Oct 2020 15:27
Operator : SY/VA
Sample : L4543-05
Misc : 5.71G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG446

Manual Integrations
APPROVED

MMDadoda
11/4/2020 11:31:09 AM

Quant Time: Oct 30 02:42:43 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 30 01:03:22 2020
Response via : Initial Calibration

