
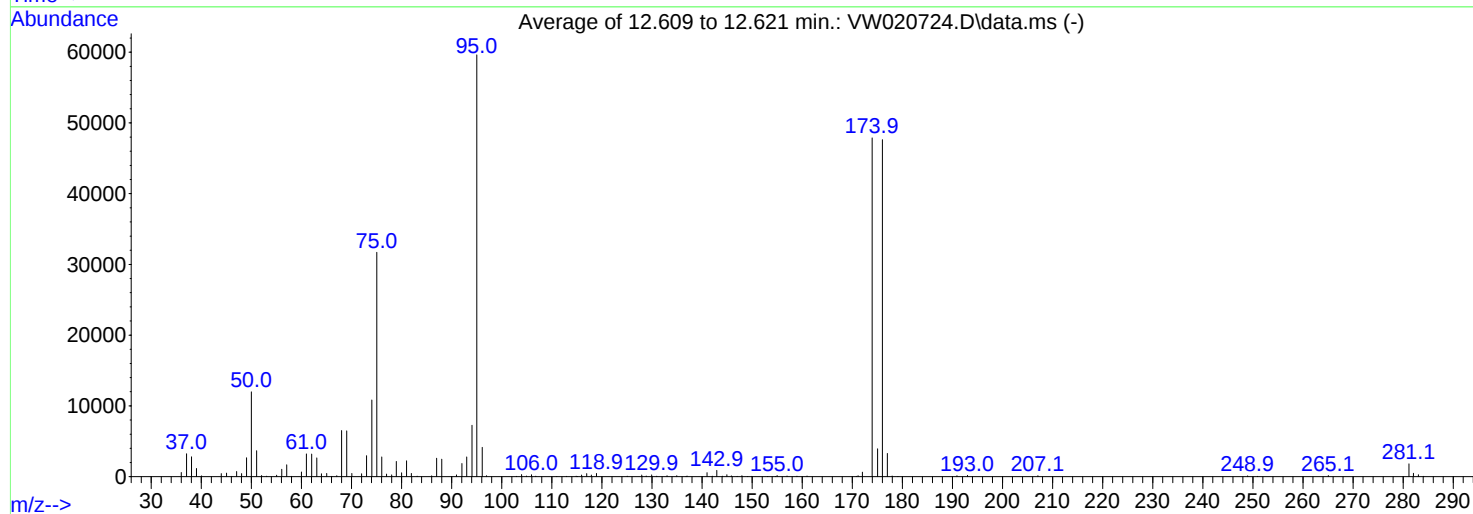


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102921\
 Data File : VW020724.D
 Acq On : 29 Oct 2021 09:48
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W102821S.M
 Title : SW846 8260
 Last Update : Fri Oct 29 05:37:46 2021

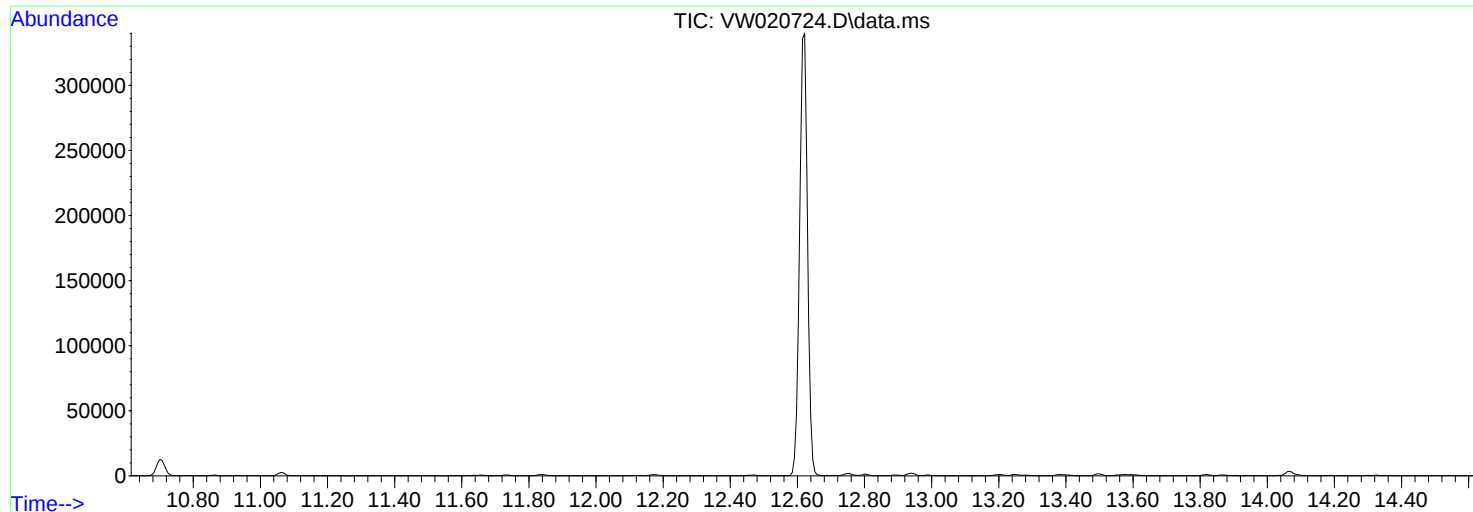

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	11979	PASS
75	95	30	60	53.2	31707	PASS
95	95	100	100	100.0	59624	PASS
96	95	5	9	6.9	4136	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.3	47880	PASS
175	174	5	9	8.2	3933	PASS
176	174	95	101	99.5	47632	PASS
177	176	5	9	6.9	3281	PASS