

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
 Data File : VW030809.D
 Acq On : 29 Oct 2024 17:17
 Operator : SY/MD
 Sample : P4492-16
 Misc : 5.39g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 30 01:17:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 30 01:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	256445	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	256458	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	116600	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	81943	20.329	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.320%
7) Chloroethane-d5	2.899	69	75683	24.804	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	4.021	65	32840	19.588	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.360%
21) 2-Butanone-d5	7.075	46	38576	53.178	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.360%
24) Chloroform-d	7.648	84	175203	23.890	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.560%
26) 1,2-Dichloroethane-d4	8.307	65	103686	27.189	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.760%
32) Benzene-d6	8.276	84	330641	22.213	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.840%
36) 1,2-Dichloropropane-d6	9.276	67	115037	26.331	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.320%
41) Toluene-d8	10.325	98	318438	23.435	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.760%
43) trans-1,3-Dichloroprop...	10.575	79	45457	24.848	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.400%
47) 2-Hexanone-d5	10.922	63	34570	61.436	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.880%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	94043	29.311	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.240%
66) 1,2-Dichlorobenzene-d4	13.855	152	116120	29.433	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	117.720%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3982	0.633	ug/L	Qvalue # 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
Data File : VW030809.D
Acq On : 29 Oct 2024 17:17
Operator : SY/MD
Sample : P4492-16
Misc : 5.39g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 30 01:17:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 30 01:14:06 2024
Response via : Initial Calibration

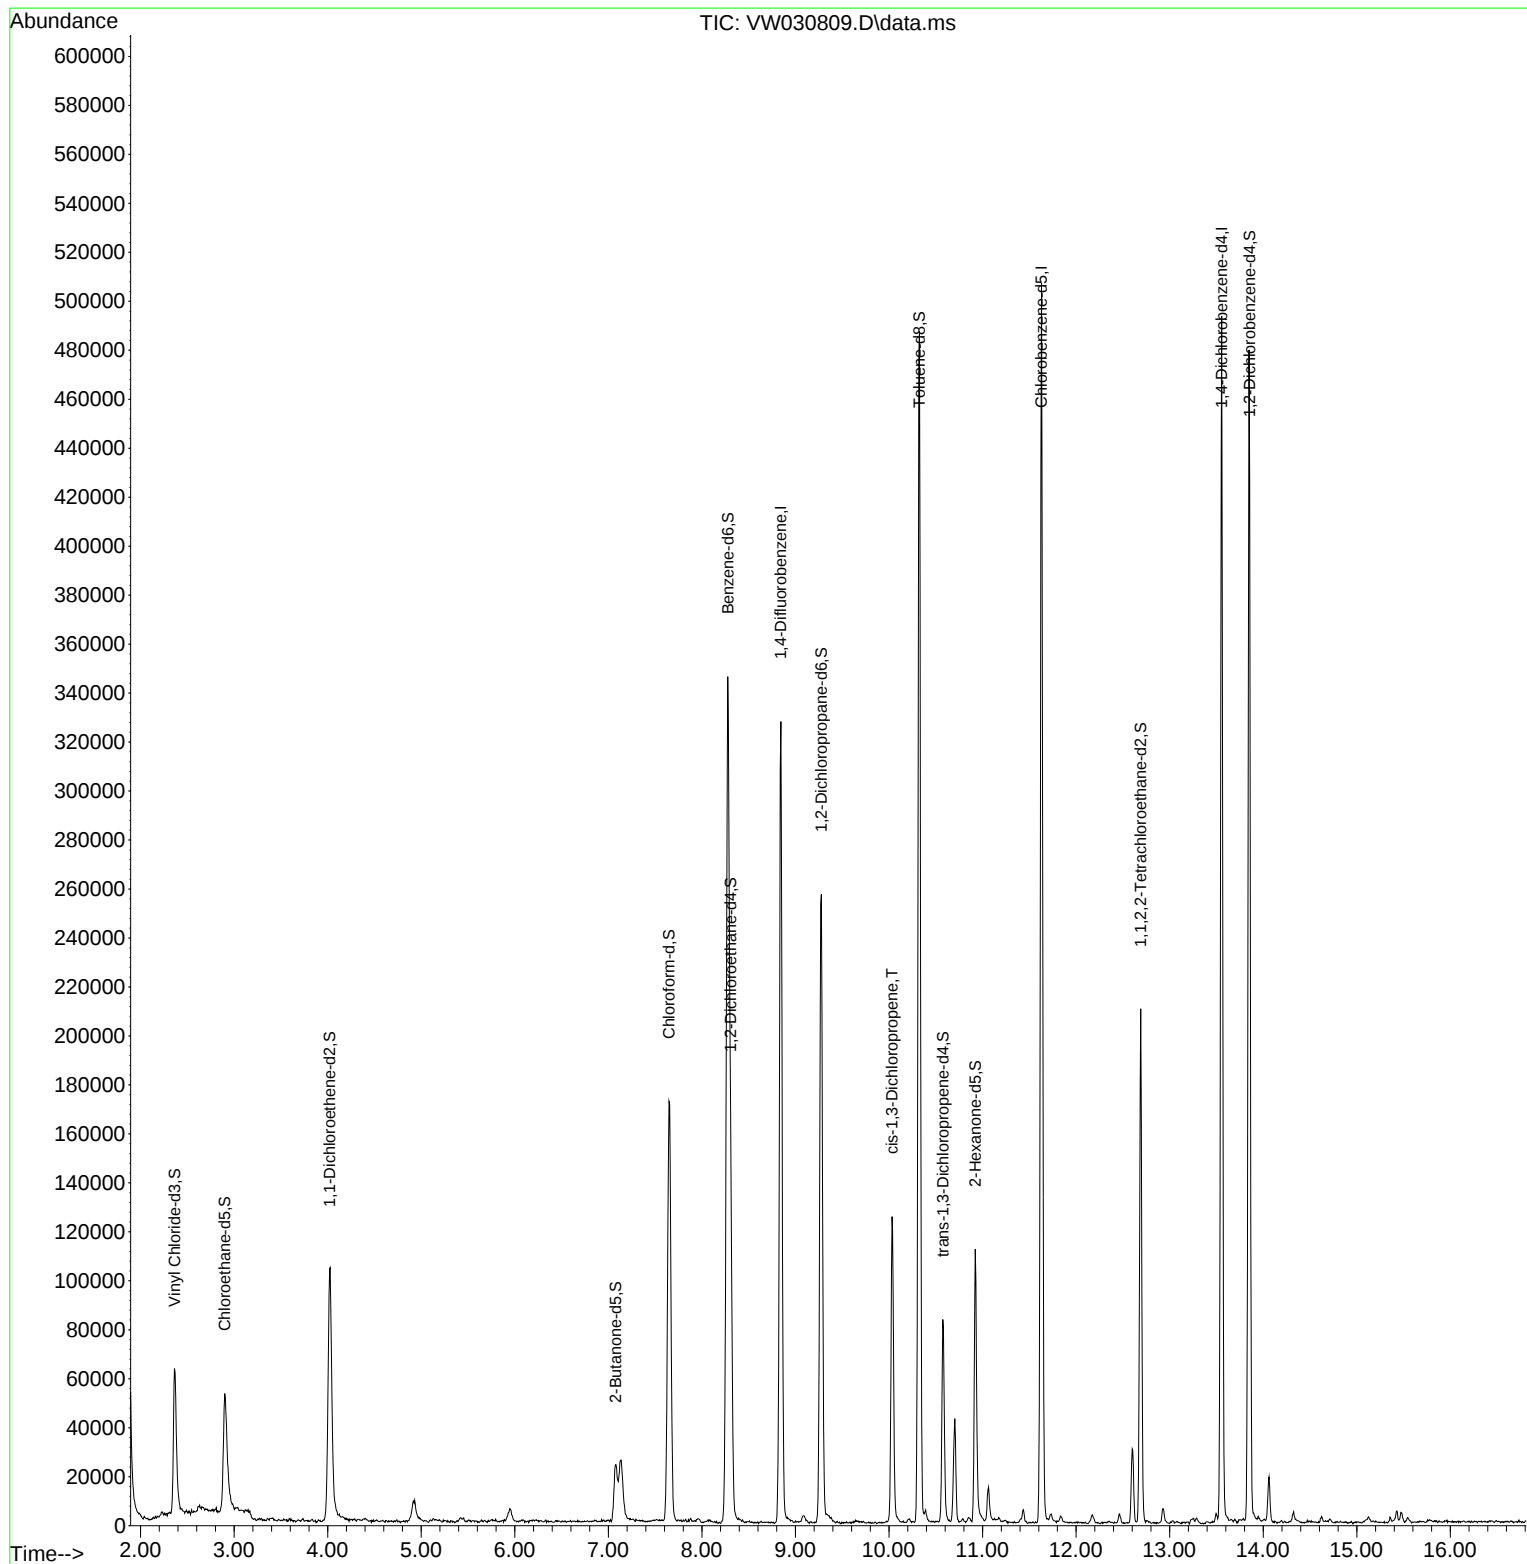

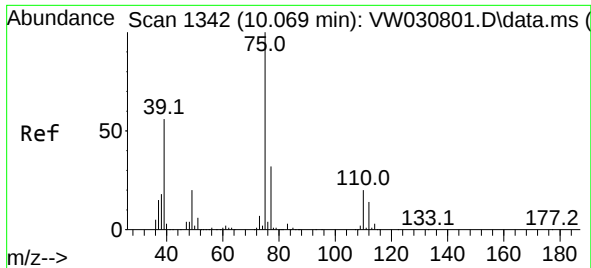

#39
 cis-1,3-Dichloropropene
 Concen: 0.633 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW030809.D
 Acq: 29 Oct 2024 17:17

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3982
 Ion Ratio Lower Upper
 75 100
 77 45.0 21.1 39.1#

