

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
 Data File : VW030810.D
 Acq On : 29 Oct 2024 17:41
 Operator : SY/MD
 Sample : P4492-15
 Misc : 5.52g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 30 01:18:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 30 01:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	285288	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	277666	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120653	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	92169	20.554	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.200%
7) Chloroethane-d5	2.899	69	81399	23.980	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.920%
11) 1,1-Dichloroethene-d2	4.021	65	39839	21.360	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.440%
21) 2-Butanone-d5	7.075	46	43012	53.298	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.600%
24) Chloroform-d	7.648	84	207412	25.422	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.680%
26) 1,2-Dichloroethane-d4	8.307	65	114485	26.985	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.960%
32) Benzene-d6	8.276	84	372148	23.092	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.360%
36) 1,2-Dichloropropane-d6	9.276	67	115405	24.398	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.600%
41) Toluene-d8	10.325	98	326207	22.173	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.680%
43) trans-1,3-Dichloroprop...	10.581	79	43156	21.789	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.160%
47) 2-Hexanone-d5	10.922	63	33182	54.465	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.940%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	90823	26.145	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	112214	27.487	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3887	0.571	ug/L	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
Data File : VW030810.D
Acq On : 29 Oct 2024 17:41
Operator : SY/MD
Sample : P4492-15
Misc : 5.52g/10mL/MSVOA_W/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 30 01:18:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 30 01:14:06 2024
Response via : Initial Calibration

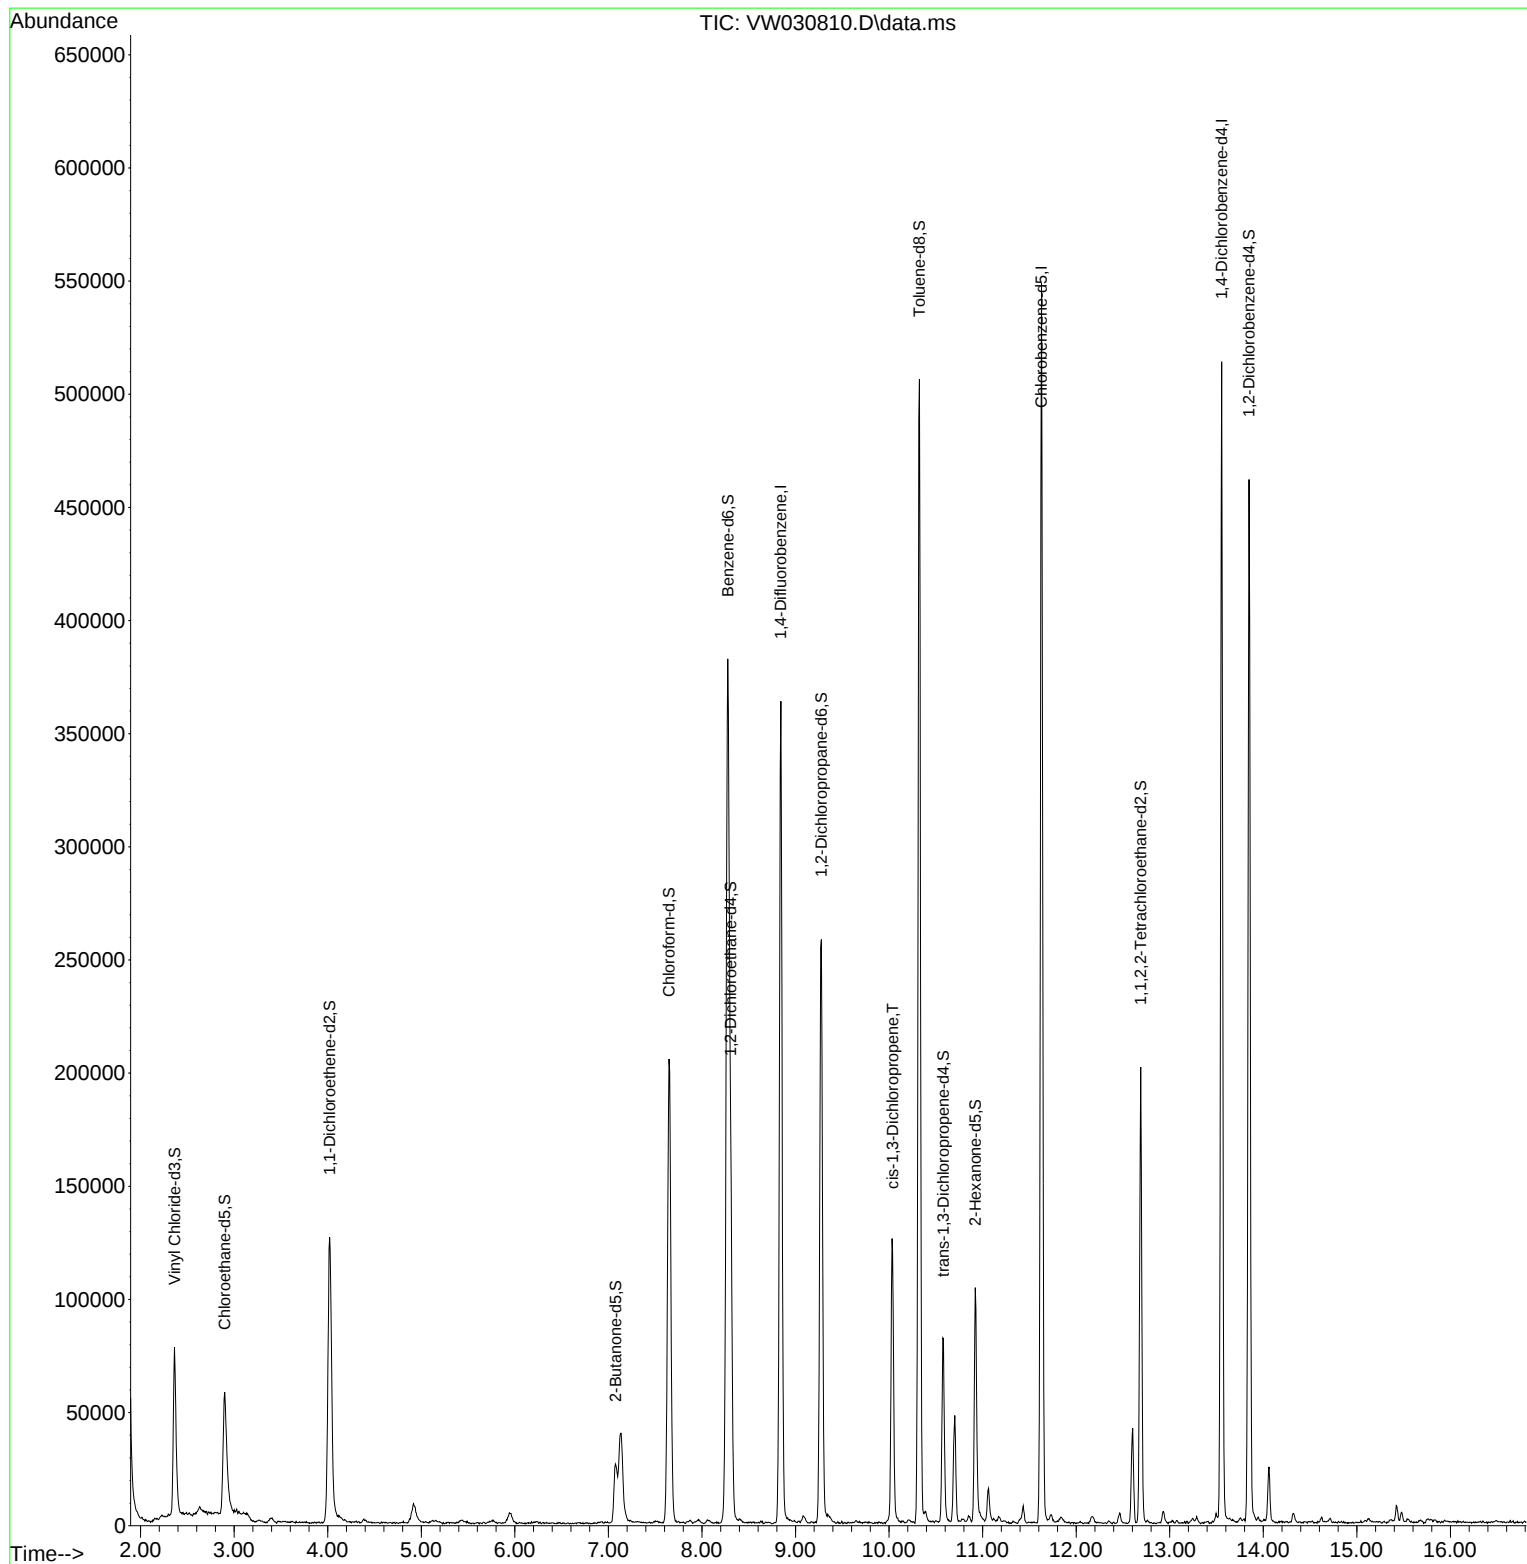

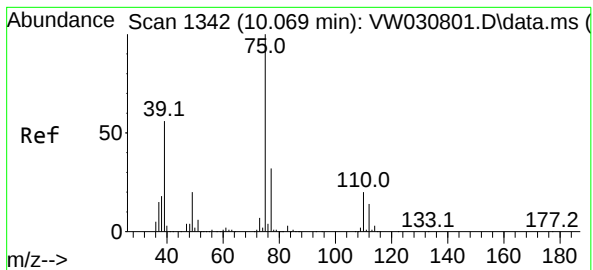

#39
 cis-1,3-Dichloropropene
 Concen: 0.571 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW030810.D
 Acq: 29 Oct 2024 17:41

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3887
 Ion Ratio Lower Upper
 75 100
 77 53.0 21.1 39.1#

