

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
 Data File : VW030812.D
 Acq On : 29 Oct 2024 18:29
 Operator : SY/MD
 Sample : P4493-12
 Misc : 5.86g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 30 01:18:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 30 01:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	259477	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	233192	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	104271	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	90072	22.084	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.320%
7) Chloroethane-d5	2.899	69	83888	27.172	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.680%
11) 1,1-Dichloroethene-d2	4.021	65	37224	21.943	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.760%
21) 2-Butanone-d5	7.075	46	41569	56.634	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.260%
24) Chloroform-d	7.648	84	191966	25.870	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.480%
26) 1,2-Dichloroethane-d4	8.307	65	113508	29.416	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	117.680%
32) Benzene-d6	8.276	84	369283	27.285	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.120%
36) 1,2-Dichloropropane-d6	9.270	67	107945	27.173	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.680%
41) Toluene-d8	10.319	98	304206	24.621	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.480%
43) trans-1,3-Dichloroprop...	10.581	79	41508	24.953	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.800%
47) 2-Hexanone-d5	10.922	63	32831	64.166	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	128.340%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	90132	30.895	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	123.560%#
66) 1,2-Dichlorobenzene-d4	13.849	152	109759	31.110	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	124.440%#
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3563	0.623	ug/L	# 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
Data File : VW030812.D
Acq On : 29 Oct 2024 18:29
Operator : SY/MD
Sample : P4493-12
Misc : 5.86g/10mL/MSVOA_W/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 30 01:18:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 30 01:14:06 2024
Response via : Initial Calibration

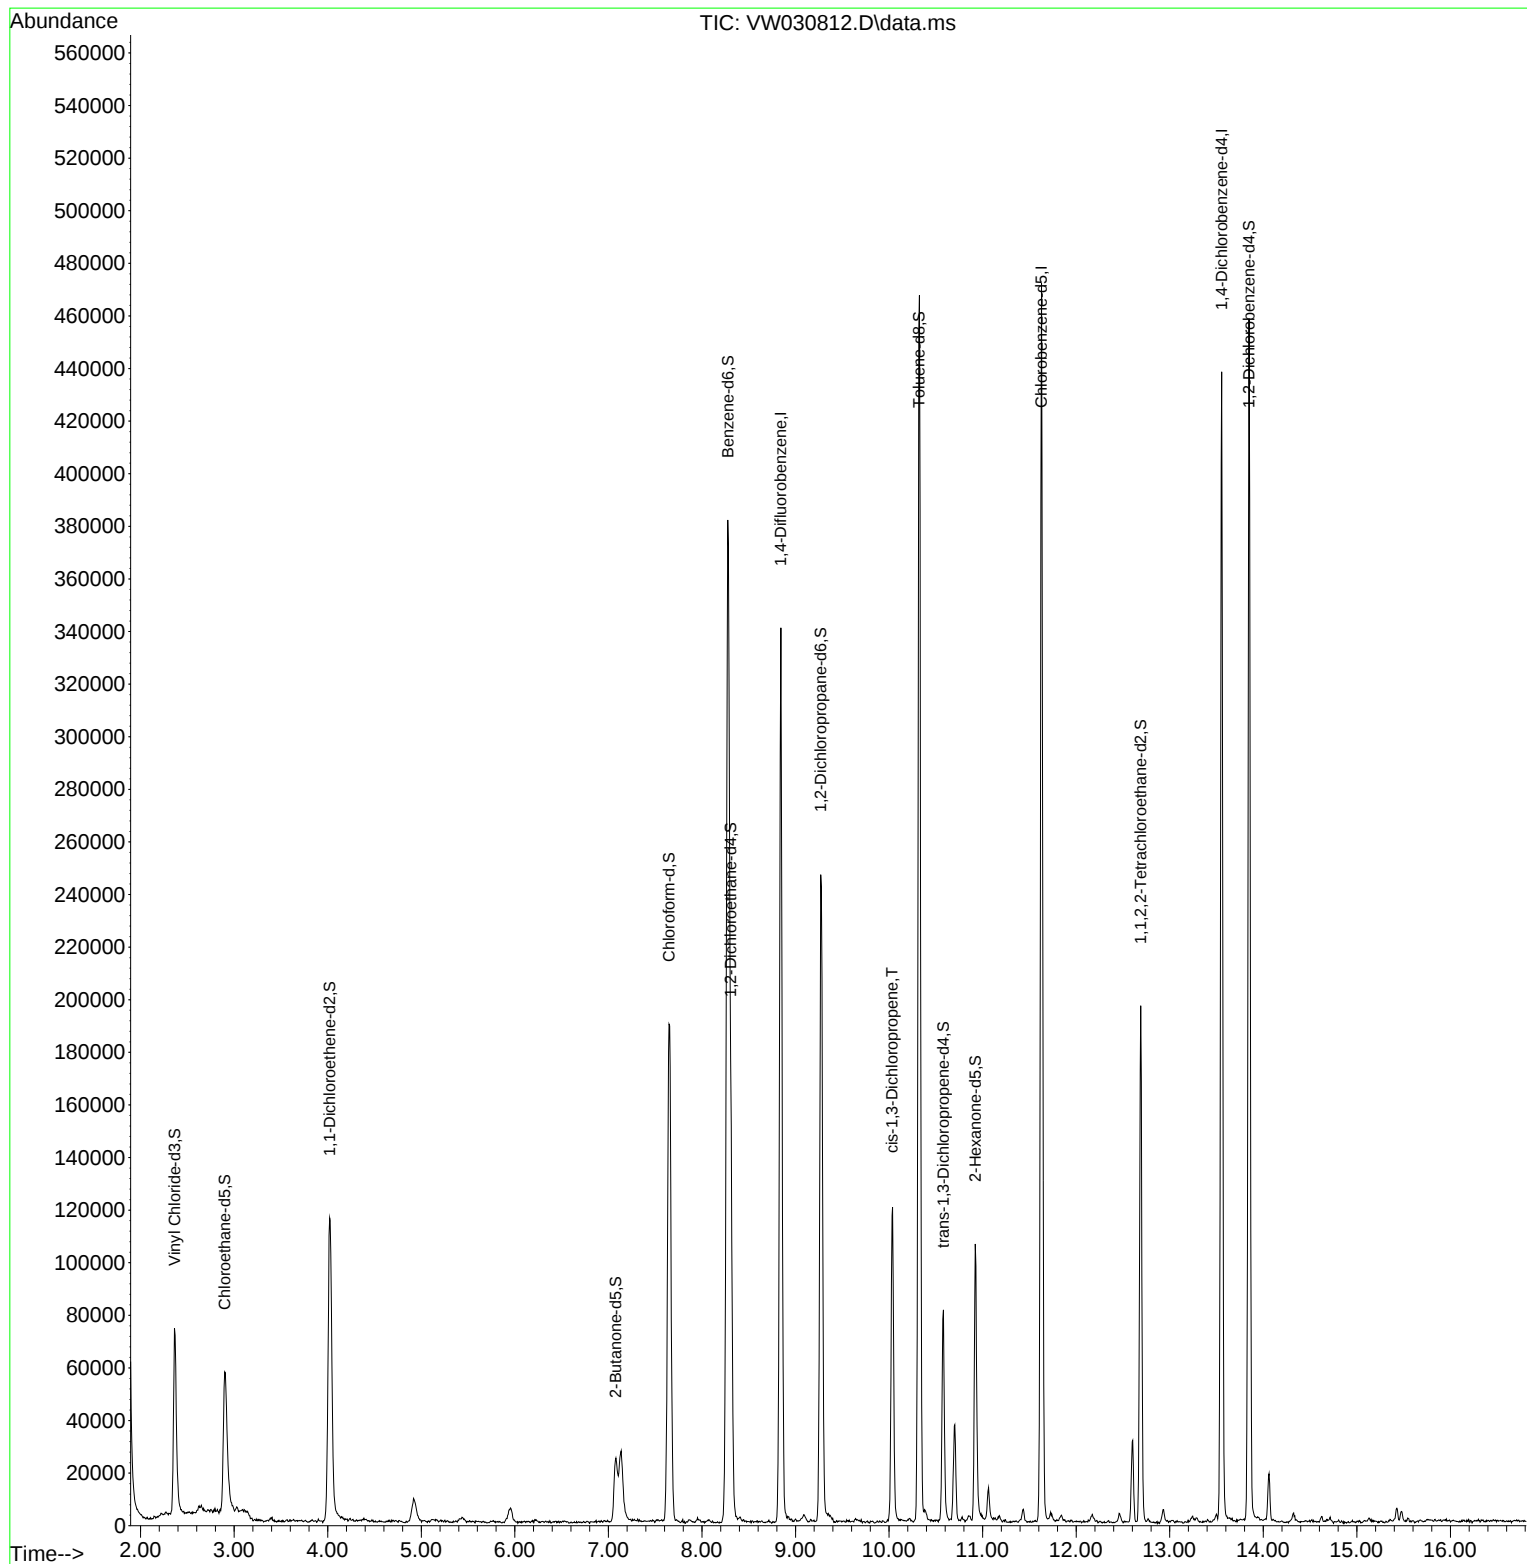

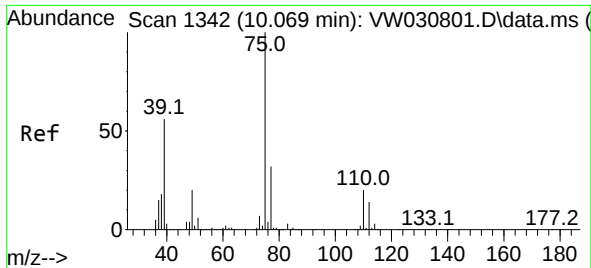

#39

cis-1,3-Dichloropropene

Concen: 0.623 ug/L

RT: 10.032 min Scan# 11

Delta R.T. -0.036 min


Lab File: VW030812.D

Acq: 29 Oct 2024 18:29

Instrument :

MSVOA_W

ClientSampleId :

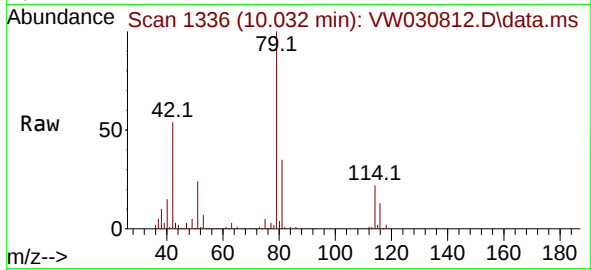

Tgt Ion: 75 Resp: 3563

Ion Ratio Lower Upper

75 100

77 53.8 21.1 39.1#

