

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
 Data File : VW030813.D
 Acq On : 29 Oct 2024 18:53
 Operator : SY/MD
 Sample : P4568-18
 Misc : 5.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 30 01:18:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 30 01:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	261523	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	246779	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	95198	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	34253	8.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	33.320%
7) Chloroethane-d5	2.899	69	43975	14.132	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.520%
11) 1,1-Dichloroethene-d2	4.027	65	14495	8.478	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	33.920%#
21) 2-Butanone-d5	7.081	46	39553	53.466	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.940%
24) Chloroform-d	7.654	84	159624	21.343	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.360%
26) 1,2-Dichloroethane-d4	8.307	65	88387	22.727	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.920%
32) Benzene-d6	8.276	84	207148	14.463	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	57.840%
36) 1,2-Dichloropropane-d6	9.276	67	89486	21.286	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.160%
41) Toluene-d8	10.325	98	152739	11.681	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	46.720%
43) trans-1,3-Dichloroprop...	10.575	79	30570	17.366	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.480%
47) 2-Hexanone-d5	10.922	63	29417	54.329	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	87019	28.186	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	69447	21.560	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.240%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2614	0.432	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
Data File : VW030813.D
Acq On : 29 Oct 2024 18:53
Operator : SY/MD
Sample : P4568-18
Misc : 5.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 30 01:18:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 30 01:14:06 2024
Response via : Initial Calibration

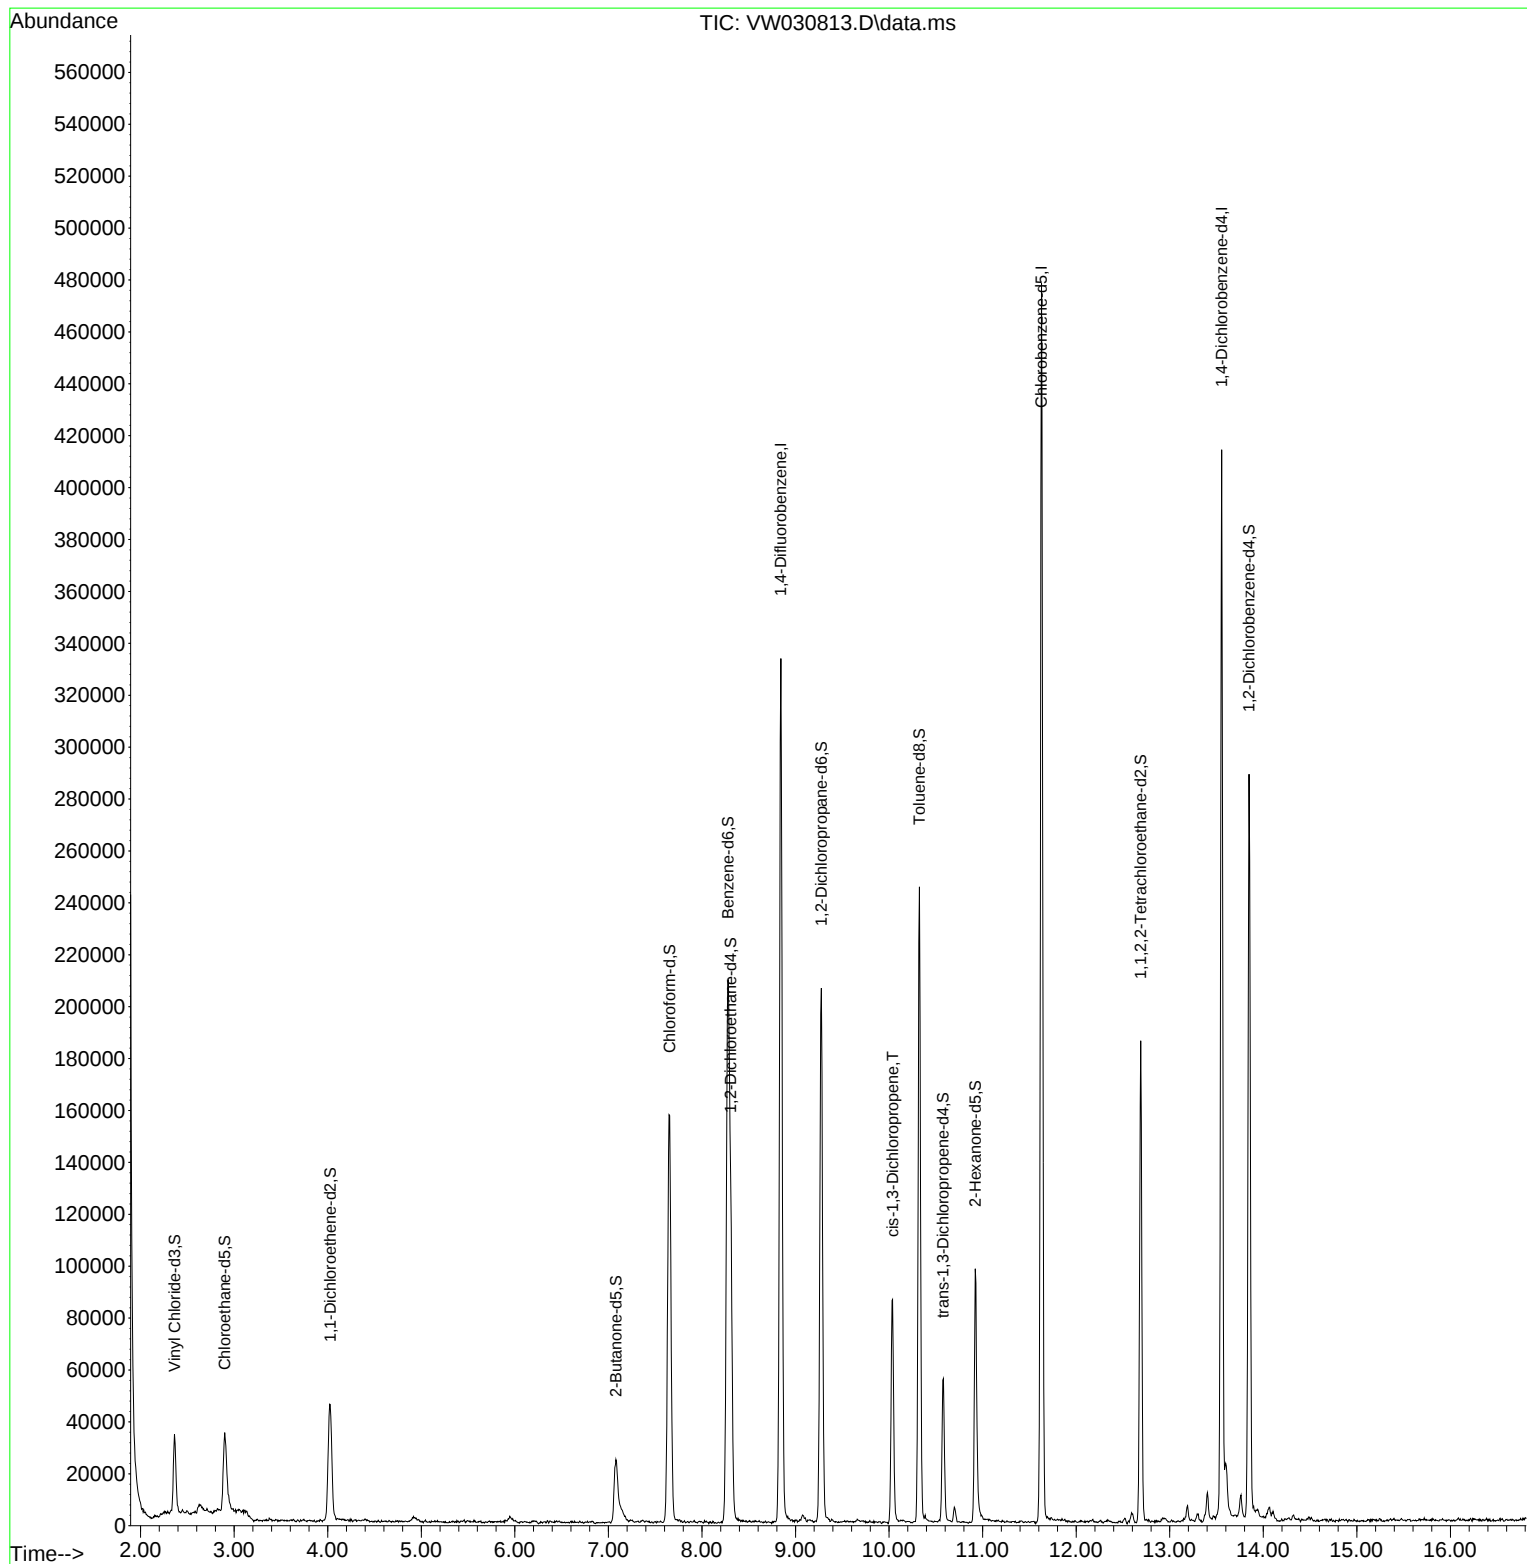

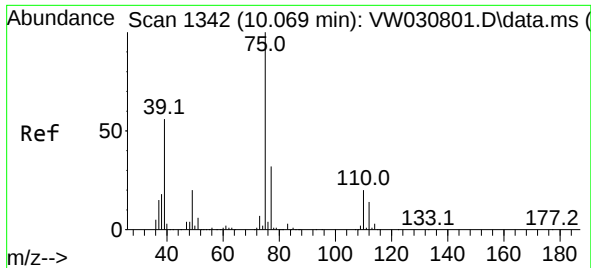

#39
cis-1,3-Dichloropropene
Concen: 0.432 ug/L
RT: 10.038 min Scan# 11
Delta R.T. -0.030 min
Lab File: VW030813.D
Acq: 29 Oct 2024 18:53

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 2614
Ion Ratio Lower Upper
75 100
77 42.4 21.1 39.1#

