

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
 Data File : VW030814.D
 Acq On : 29 Oct 2024 19:17
 Operator : SY/MD
 Sample : P4568-17
 Misc : 4.99g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EF1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/30/2024
 Supervised By :Mahesh Dadoda 10/30/2024

Quant Time: Oct 30 01:18:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 30 01:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	33930	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	30992	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	10314	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	5578	10.459	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	41.840%		
7) Chloroethane-d5	2.887	69	6457	15.994	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.960%		
11) 1,1-Dichloroethene-d2	4.033	65	2421m	10.914	ug/L	0.02
Spiked Amount 25.000	Range 45 - 110		Recovery =	43.640%#		
21) 2-Butanone-d5	7.087	46	4755m	49.542	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	99.080%		
24) Chloroform-d	7.654	84	21885	22.554	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.200%		
26) 1,2-Dichloroethane-d4	8.307	65	11554	22.899	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.600%		
32) Benzene-d6	8.276	84	26657	14.820	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	59.280%		
36) 1,2-Dichloropropane-d6	9.276	67	12412	23.510	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.040%		
41) Toluene-d8	10.325	98	16447	10.016	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	40.080%		
43) trans-1,3-Dichloroprop...	10.581	79	3611	16.334	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	65.320%		
47) 2-Hexanone-d5	10.928	63	2604m	38.294	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.580%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	11807	30.452	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	121.800%#		
66) 1,2-Dichlorobenzene-d4	13.854	152	8617	24.692	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.760%		
Target Compounds					Qvalue	
13) Acetone	4.124	43	2808m	19.984	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
Data File : VW030814.D
Acq On : 29 Oct 2024 19:17
Operator : SY/MD
Sample : P4568-17
Misc : 4.99g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4EF1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/30/2024
Supervised By :Mahesh Dadoda 10/30/2024


Quant Time: Oct 30 01:18:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 30 01:14:06 2024
Response via : Initial Calibration

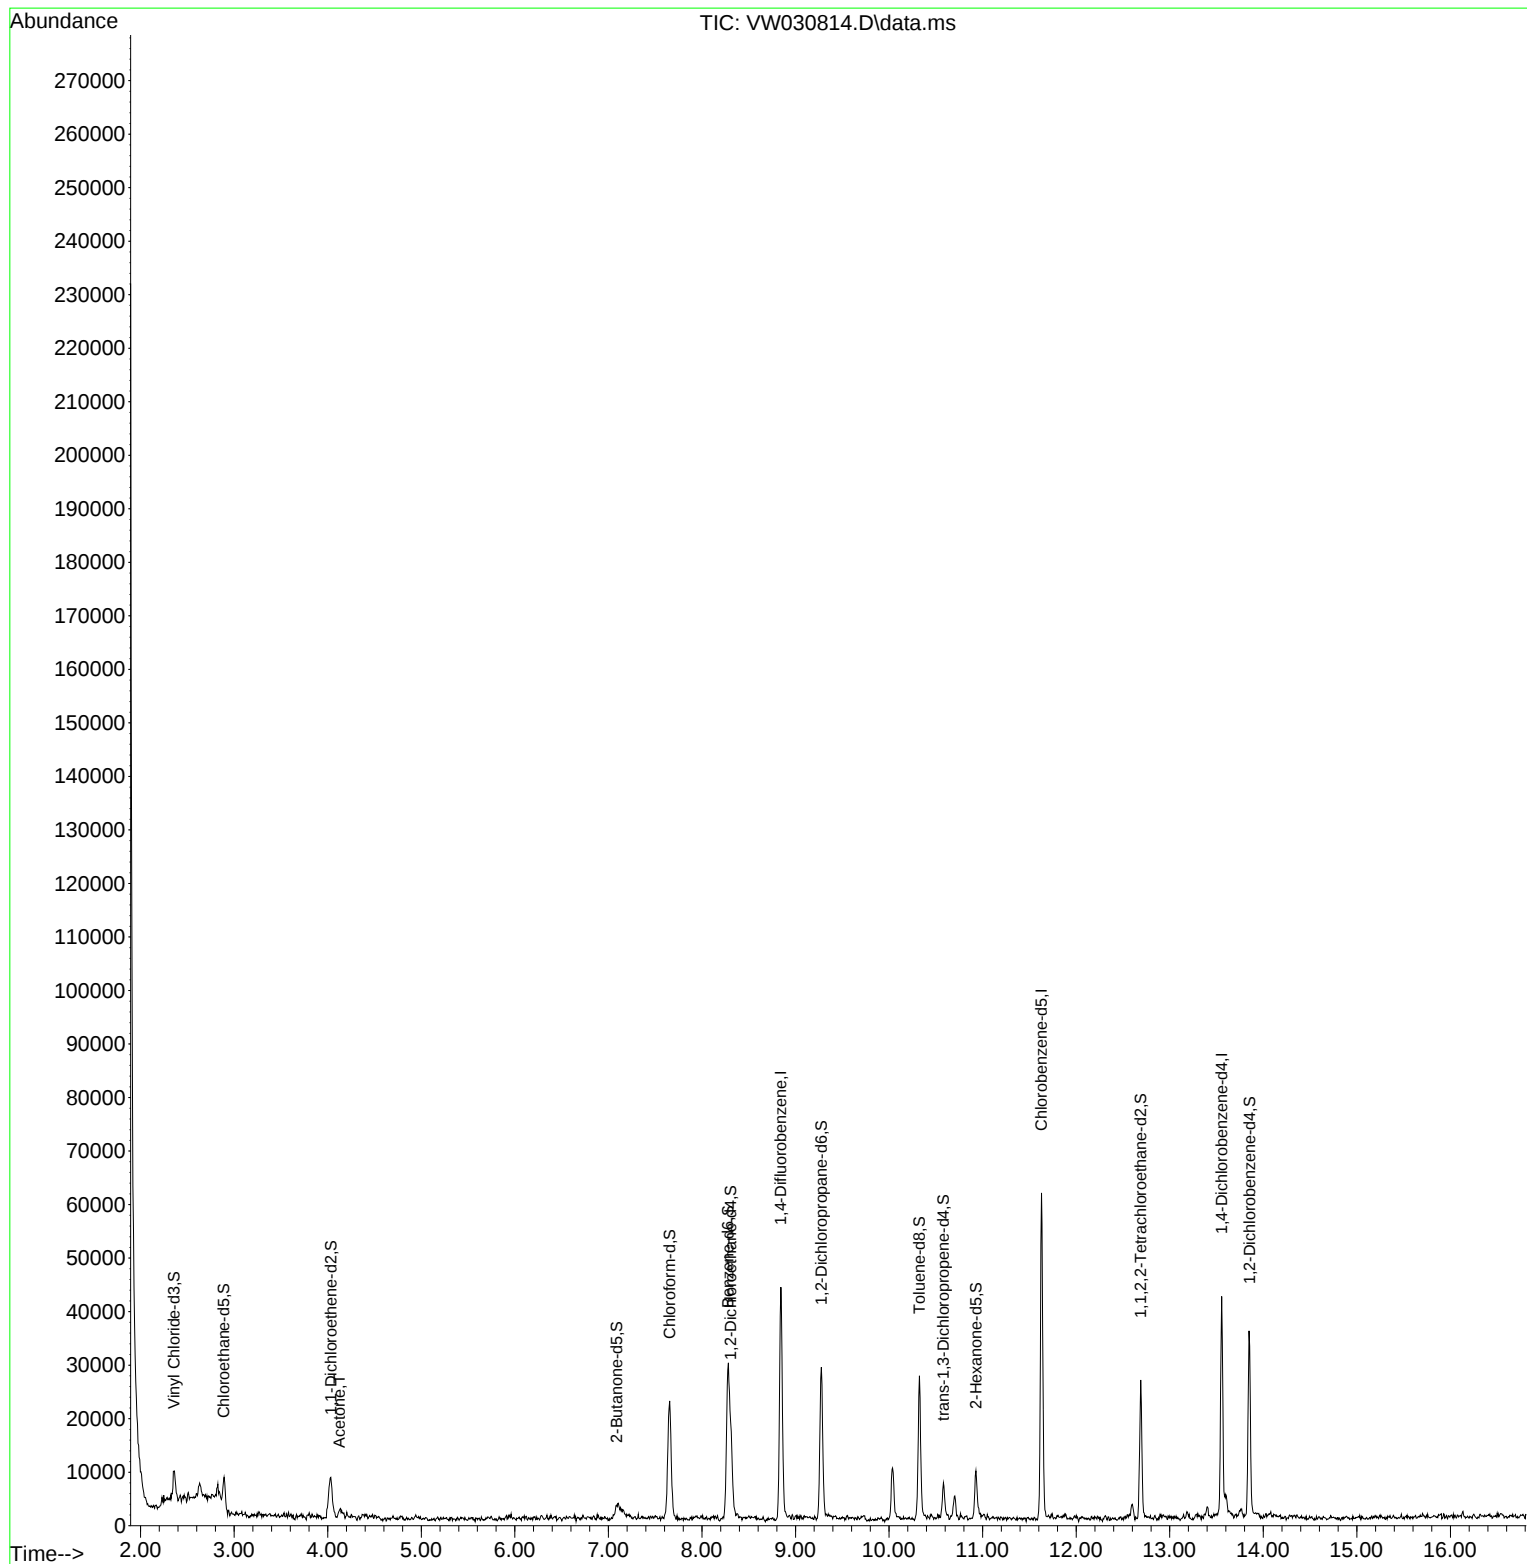

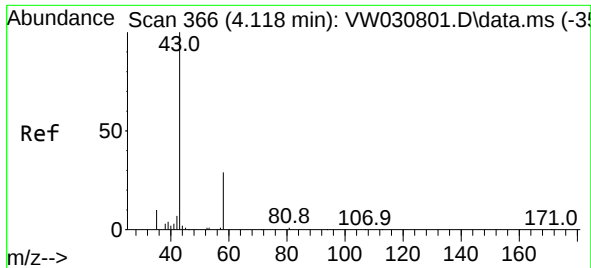

#13
 Acetone
 Concen: 19.984 ug/L m
 RT: 4.124 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW030814.D
 Acq: 29 Oct 2024 19:17

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EF1

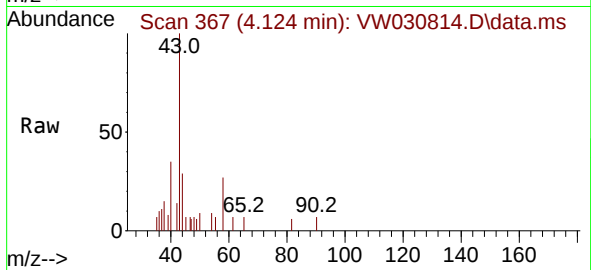

Tgt Ion: 43 Resp: 280
 Ion Ratio Lower Upper
 43 100
 58 17.4 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/30/2024
 Supervised By :Mahesh Dadoda 10/30/2024

