

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
 Data File : VW030818.D
 Acq On : 29 Oct 2024 20:52
 Operator : SY/MD
 Sample : P4568-19
 Misc : 5.20g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EF3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 10/30/2024
 Supervised By :Mahesh Dadoda 10/30/2024

Quant Time: Oct 30 01:20:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 30 01:14:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	28210	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	23367	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	6814	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	5038	11.362	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	45.440%		
7) Chloroethane-d5	2.893	69	5557	16.556	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.240%		
11) 1,1-Dichloroethene-d2	4.027	65	2200	11.929	ug/L	0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	47.720%		
21) 2-Butanone-d5	7.100	46	2924m	36.642	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	73.280%		
24) Chloroform-d	7.661	84	19294	23.916	ug/L	0.01
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.680%		
26) 1,2-Dichloroethane-d4	8.313	65	9738	23.213	ug/L	0.01
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.840%		
32) Benzene-d6	8.276	84	23646	17.435	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	69.760%		
36) 1,2-Dichloropropane-d6	9.276	67	10050	25.247	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.000%		
41) Toluene-d8	10.325	98	13311	10.751	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	43.000%		
43) trans-1,3-Dichloroprop...	10.581	79	2184	13.103	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	52.400%		
47) 2-Hexanone-d5	10.928	63	1623	31.656	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	63.320%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	7775	26.596	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	106.400%		
66) 1,2-Dichlorobenzene-d4	13.849	152	4897	21.240	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.960%		
Target Compounds					Qvalue	
13) Acetone	4.137	43	1952m	16.708	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102924\
Data File : VW030818.D
Acq On : 29 Oct 2024 20:52
Operator : SY/MD
Sample : P4568-19
Misc : 5.20g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
A4EF3

Quant Time: Oct 30 01:20:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 30 01:14:06 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 10/30/2024
Supervised By :Mahesh Dadoda 10/30/2024

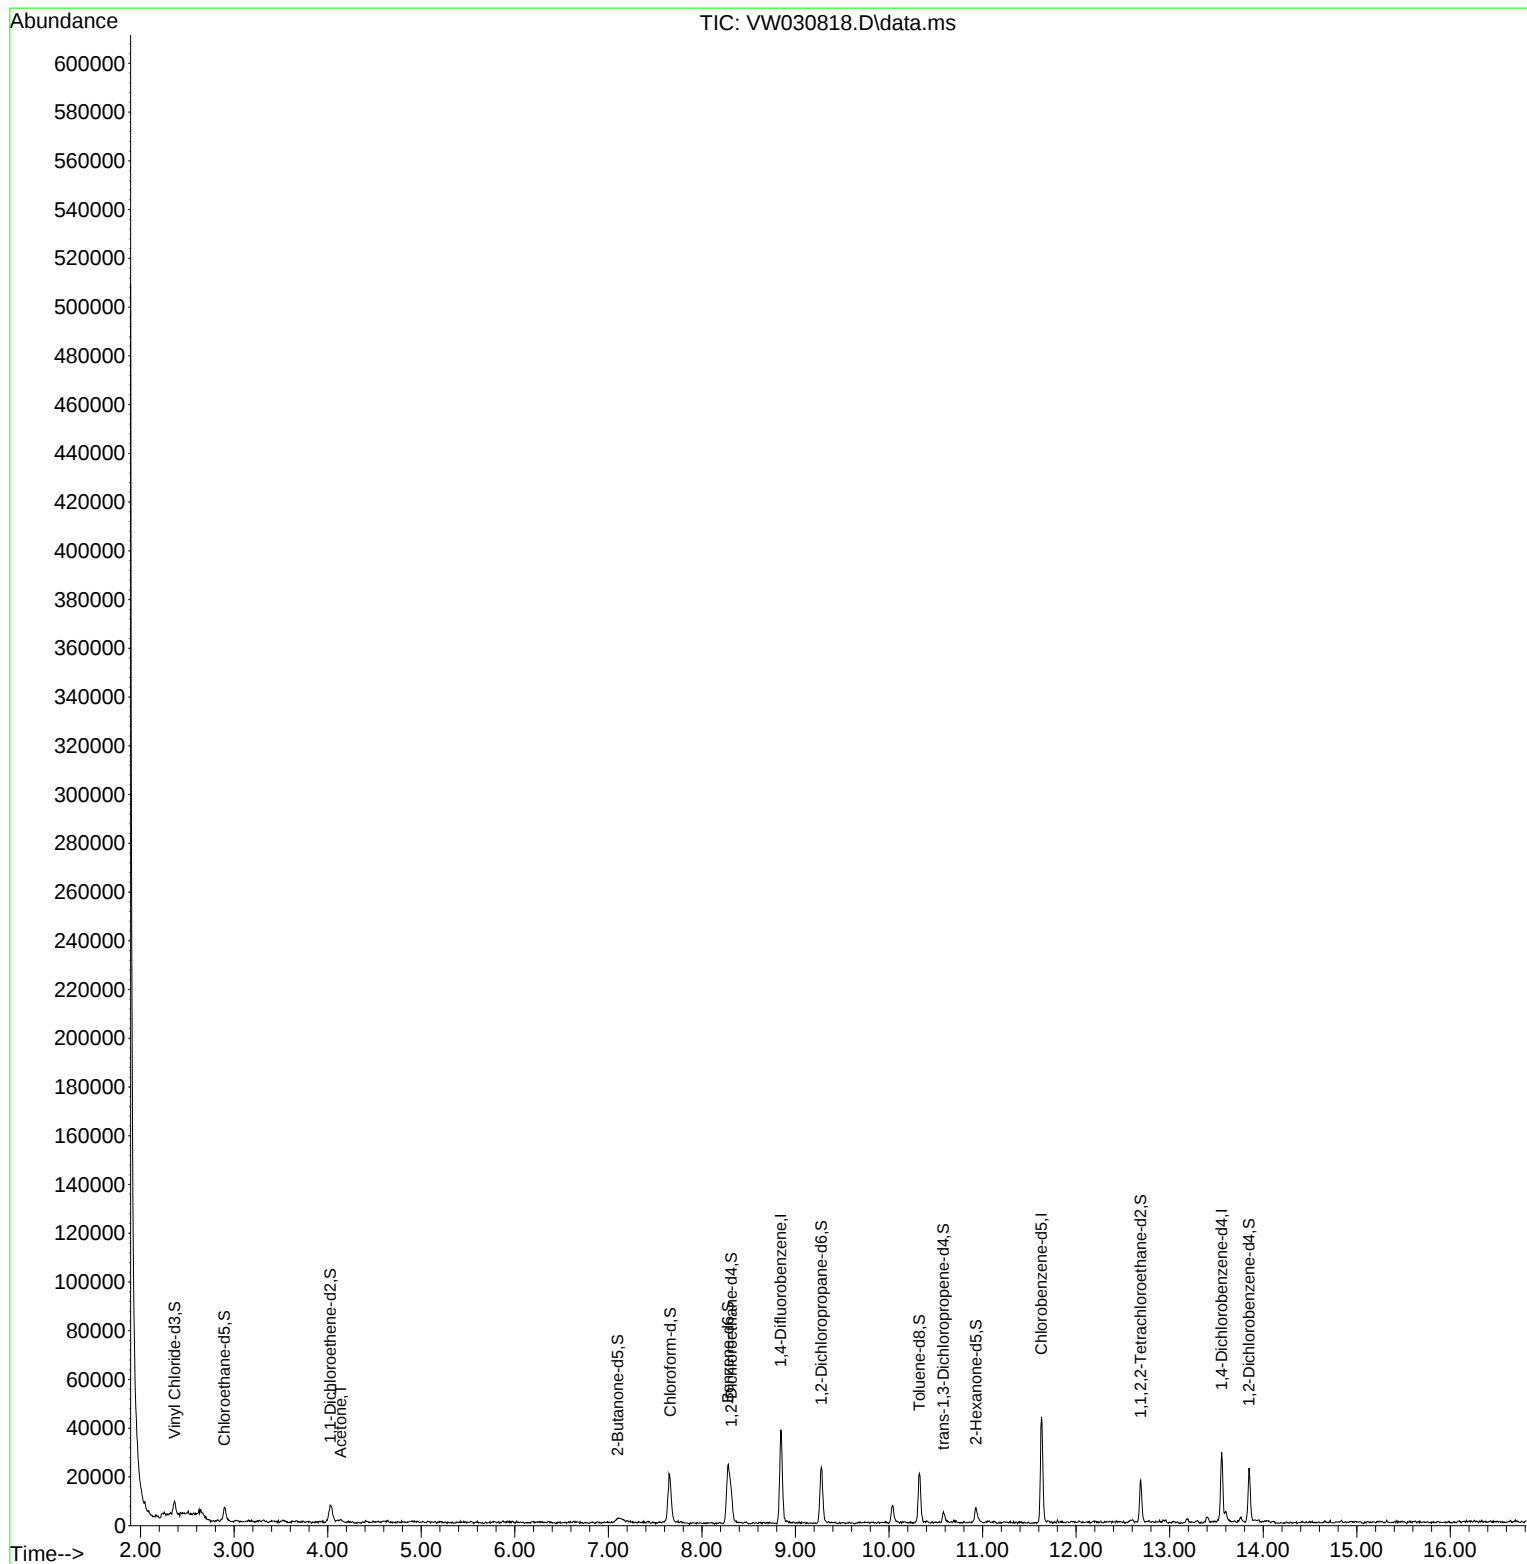

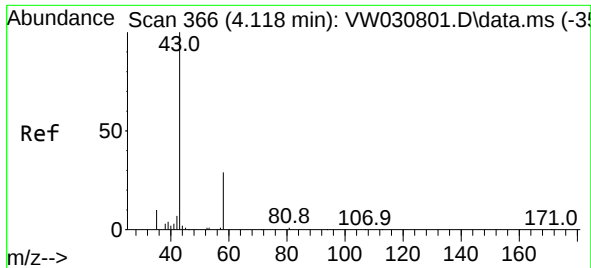

#13
Acetone
Concen: 16.708 ug/L m
RT: 4.137 min Scan# 30
Delta R.T. 0.019 min
Lab File: VW030818.D
Acq: 29 Oct 2024 20:52

Instrument :
MSVOA_W
ClientSampleId :
A4EF3

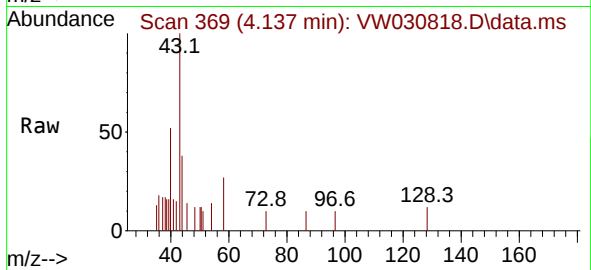

Tgt Ion: 43 Resp: 195
Ion Ratio Lower Upper
43 100
58 5.6 0.0 57.6

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 10/30/2024
Supervised By :Mahesh Dadoda 10/30/2024

