

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW103019\
 Data File : VW013827.D
 Acq On : 30 Oct 2019 10:41
 Operator : SY/VA
 Sample : VW1030SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK15

Quant Time: Oct 31 05:31:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 31 05:29:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	297557	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	300210	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	168606	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	74157	20.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.24%
7) Chloroethane-d5	2.89	69	65146	19.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.48%
10) 1,1-Dichloroethene-d2	4.03	63	115584	14.33	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.32%
20) 2-Butanone-d5	7.08	46	70594	54.06	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.12%
24) Chloroform-d	7.65	84	184496	22.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.64%
26) 1,2-Dichloroethane-d4	8.31	65	102754	23.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.40%
29) Benzene-d6	8.27	84	372930	20.68	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.72%
33) 1,2-Dichloropropane-d6	9.27	67	117844	21.88	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.52%
37) Toluene-d8	10.32	98	337495	20.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.16%
38) trans-1,3-Dichloropropene-	10.58	79	49260	20.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.08%
39) 2-Hexanone-d5	10.92	63	56152	54.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.06%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	109548	24.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	135824	22.80	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.20%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.55	75	17899	5.042 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW103019\
Data File : VW013827.D
Acq On : 30 Oct 2019 10:41
Operator : SY/VA
Sample : VW1030SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK15

Quant Time: Oct 31 05:31:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 31 05:29:18 2019
Response via : Initial Calibration

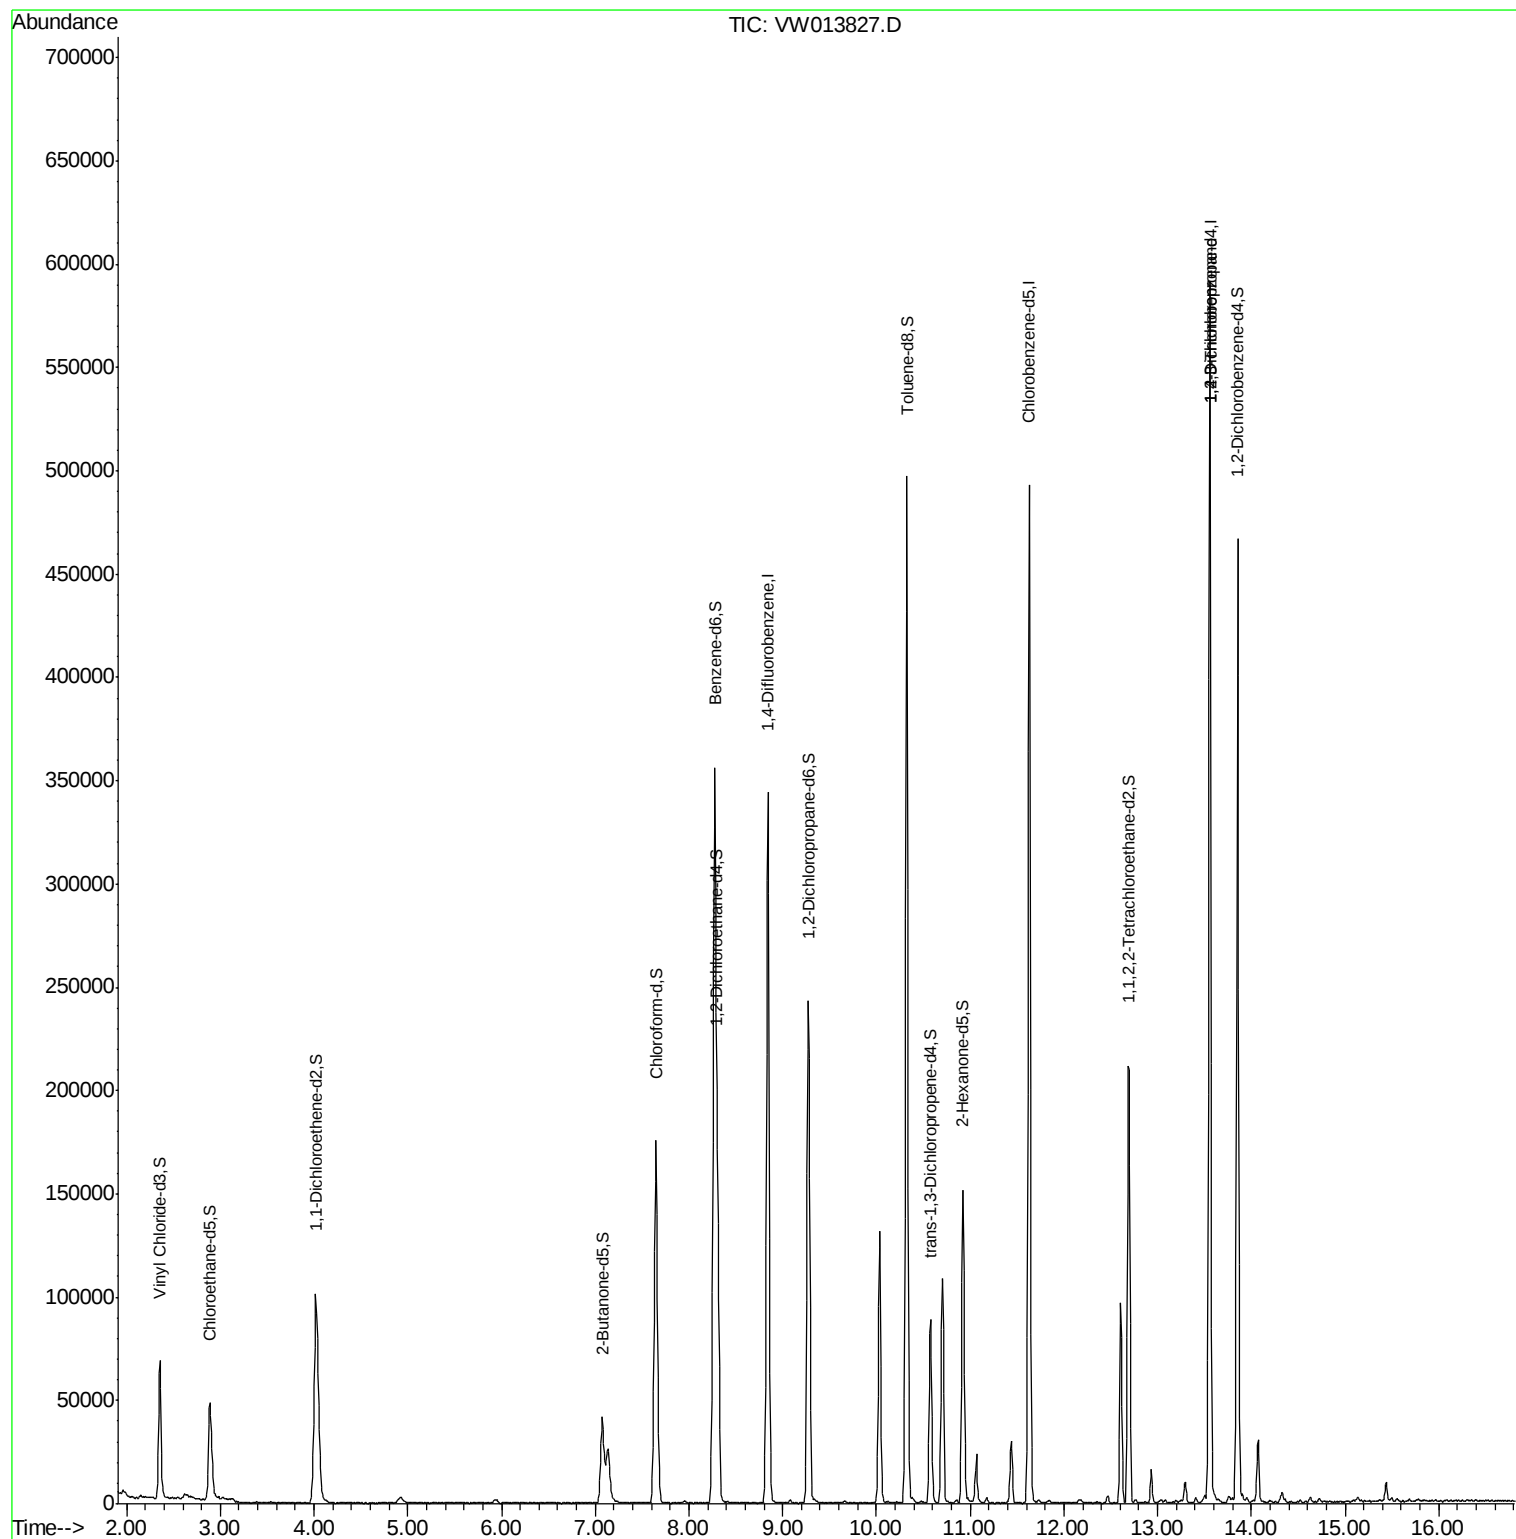

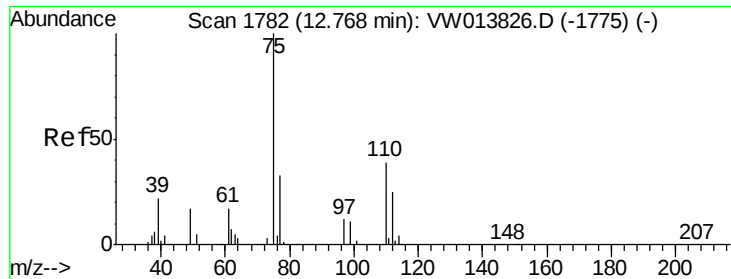

#59

1,2,3-Trichloropropane

Concen: 5.042 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013827.D

Acq: 30 Oct 2019 10:41

Instrument :

MSVOA_W

ClientSampleId :

VBLK15

Tot Ion: 75 Resp: 17899

Ion Ratio Lower Upper

75 100

77 34.1 26.4 39.6

