

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW103019\
 Data File : VW013844.D
 Acq On : 30 Oct 2019 18:11
 Operator : SY/VA
 Sample : K5596-06
 Misc : 4.96G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAQA7

Quant Time: Nov 12 02:51:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 31 05:29:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	304941	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	304772	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	161487	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	90081	24.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.32%
7) Chloroethane-d5	2.89	69	75089	21.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.00%
10) 1,1-Dichloroethene-d2	4.02	63	142448	17.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.96%
20) 2-Butanone-d5	7.07	46	98352	73.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	147.00%#
24) Chloroform-d	7.65	84	210362	24.65	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	8.31	65	124801	27.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.88%
29) Benzene-d6	8.27	84	435545	23.79	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.16%
33) 1,2-Dichloropropane-d6	9.27	67	137513	25.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.60%
37) Toluene-d8	10.32	98	400692	23.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.92%
38) trans-1,3-Dichloropropene-	10.58	79	62289	25.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.00%
39) 2-Hexanone-d5	10.92	63	81877	78.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	156.64%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	147691	32.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	131.88%#
61) 1,2-Dichlorobenzene-d4	13.85	152	150406	26.36	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.44%


Target Compounds					Qvalue
13) Acetone	4.12	43	16657	11.215 ug/L	98
15) Methyl Acetate	4.67	43	2543	1.048 ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW103019\
Data File : VW013844.D
Acq On : 30 Oct 2019 18:11
Operator : SY/VA
Sample : K5596-06
Misc : 4.96G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAQA7

Quant Time: Nov 12 02:51:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 31 05:29:18 2019
Response via : Initial Calibration

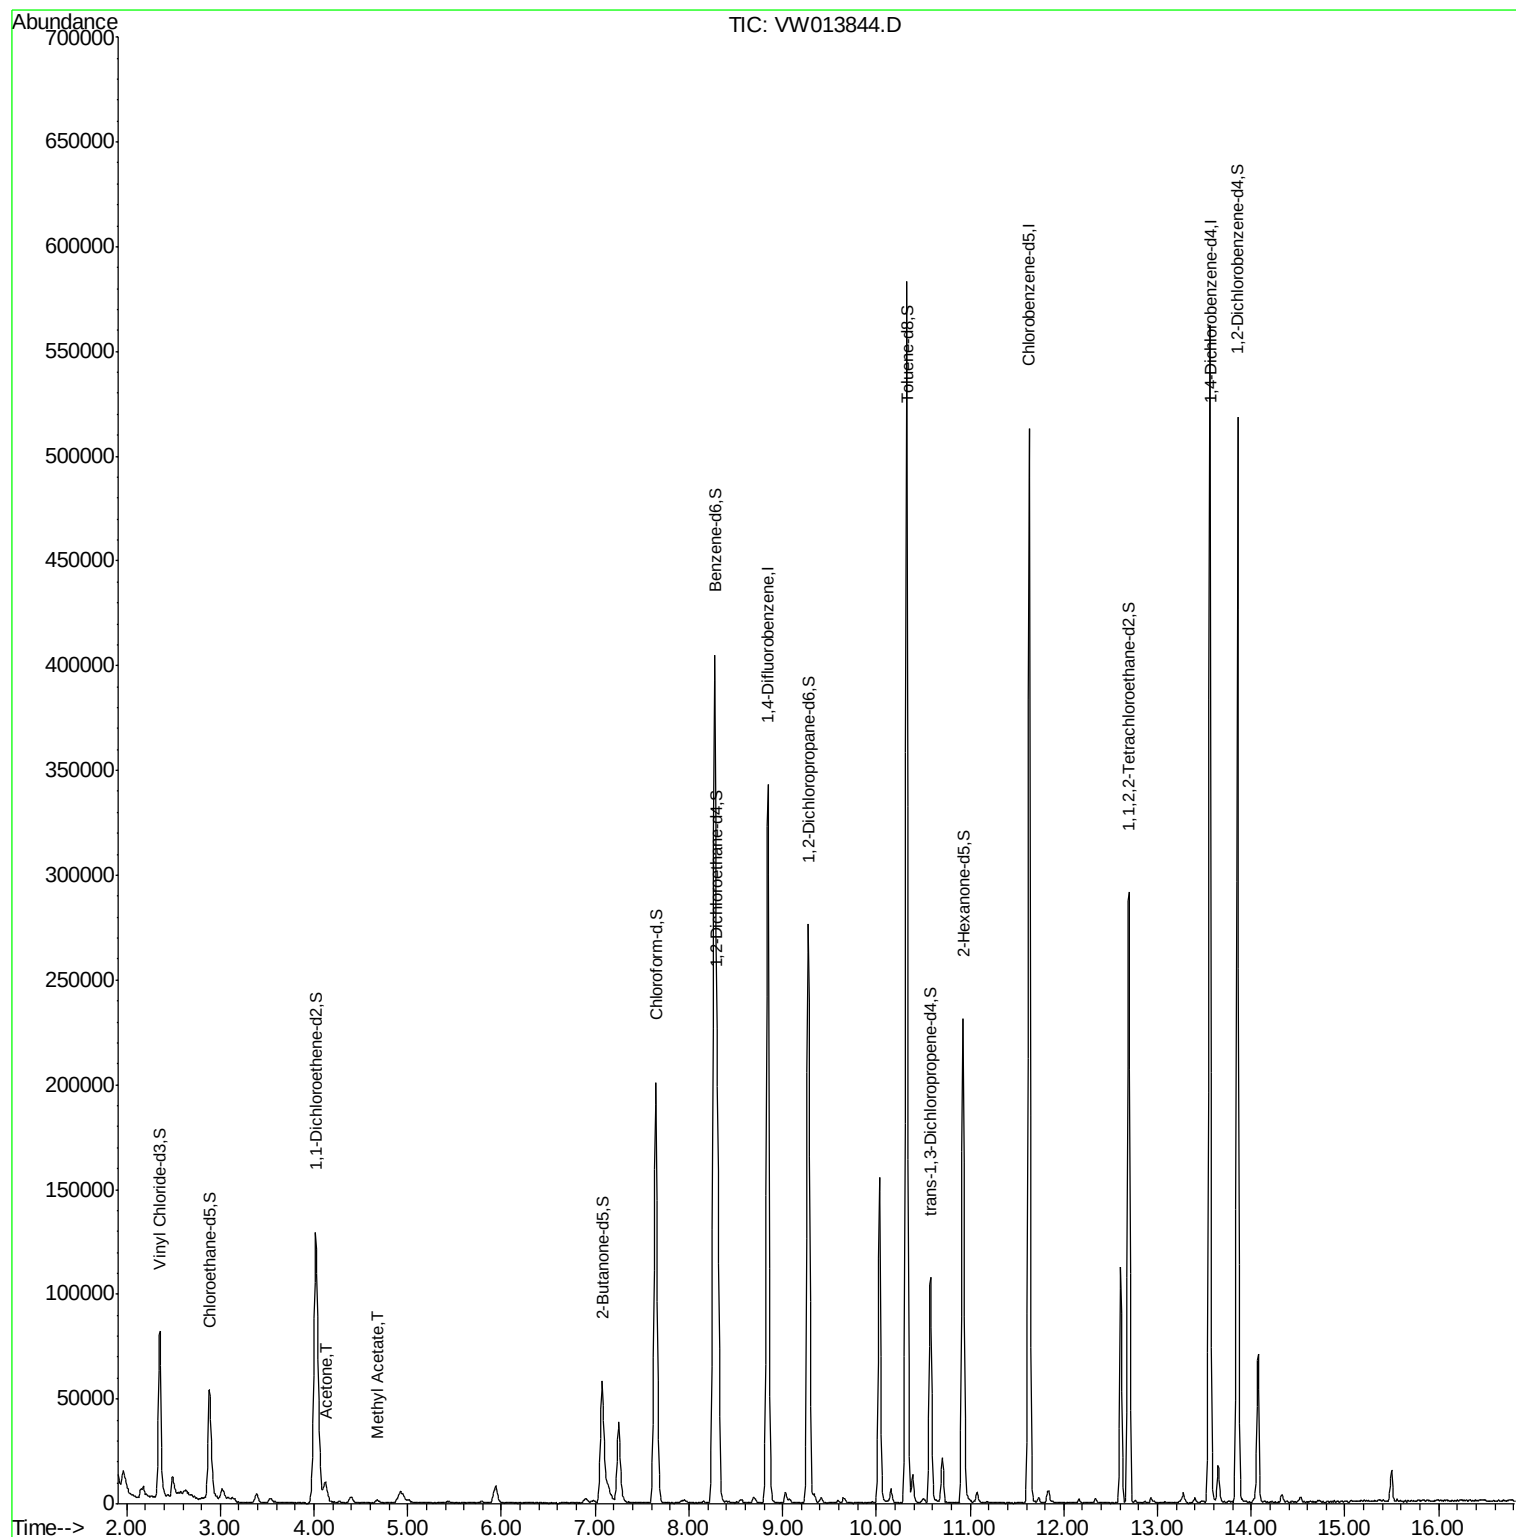

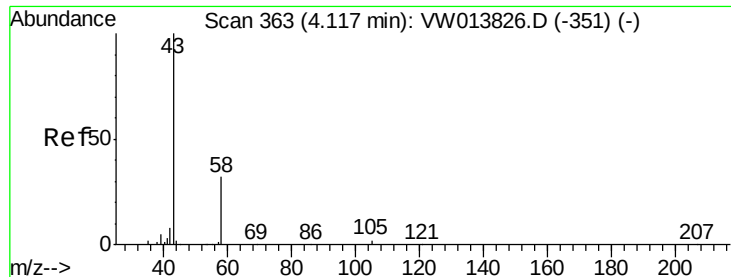

#13

Acetone

Concen: 11.215 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW013844.D

Acq: 30 Oct 2019 18:11

Instrument :

MSVOA_W

ClientSampled :


GAQA7

Tgt Ion: 43 Resp: 16657

Ion Ratio Lower Upper




43 100

58 33.8 0.0 70.4

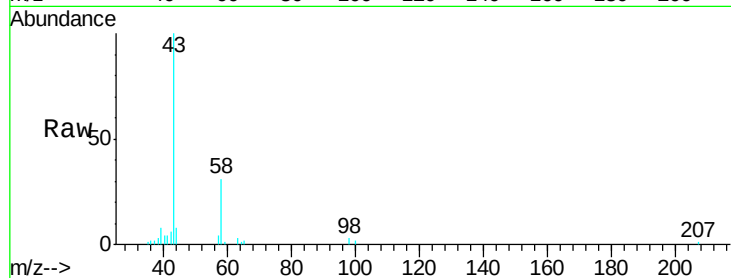

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

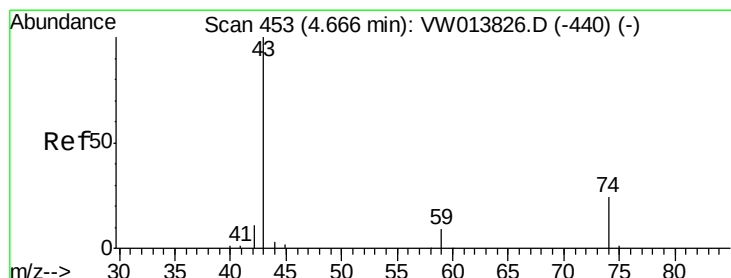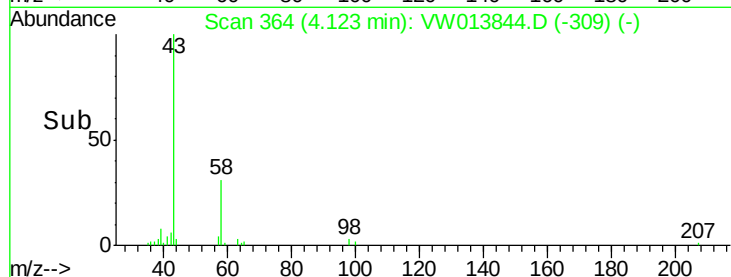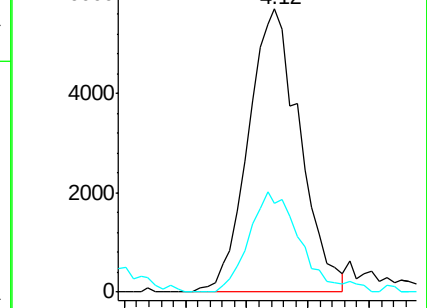

#15

Methyl Acetate

Concen: 1.048 ug/L

RT: 4.67 min Scan# 454

Delta R.T. 0.01 min

Lab File: VW013844.D


Acq: 30 Oct 2019 18:11

Tgt Ion: 43 Resp: 2543

Ion Ratio Lower Upper

43 100

74 7.9 19.2 28.8#

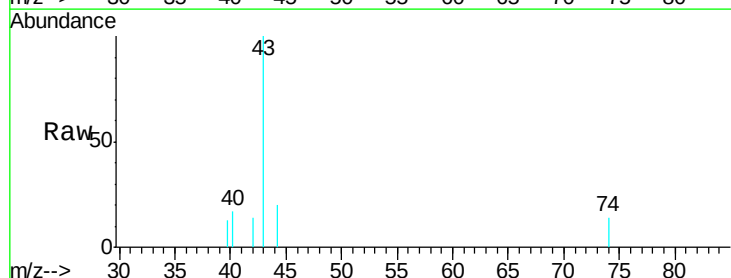

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 74.00 (73.70 to 74.70): VW

