


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW103020\
 Data File : VW017030.D
 Acq On : 30 Oct 2020 09:06
 Operator : SY/VA
 Sample : BFB25
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB25

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Title : VOC Analysis
 Last Update : Mon Nov 02 02:01:09 2020

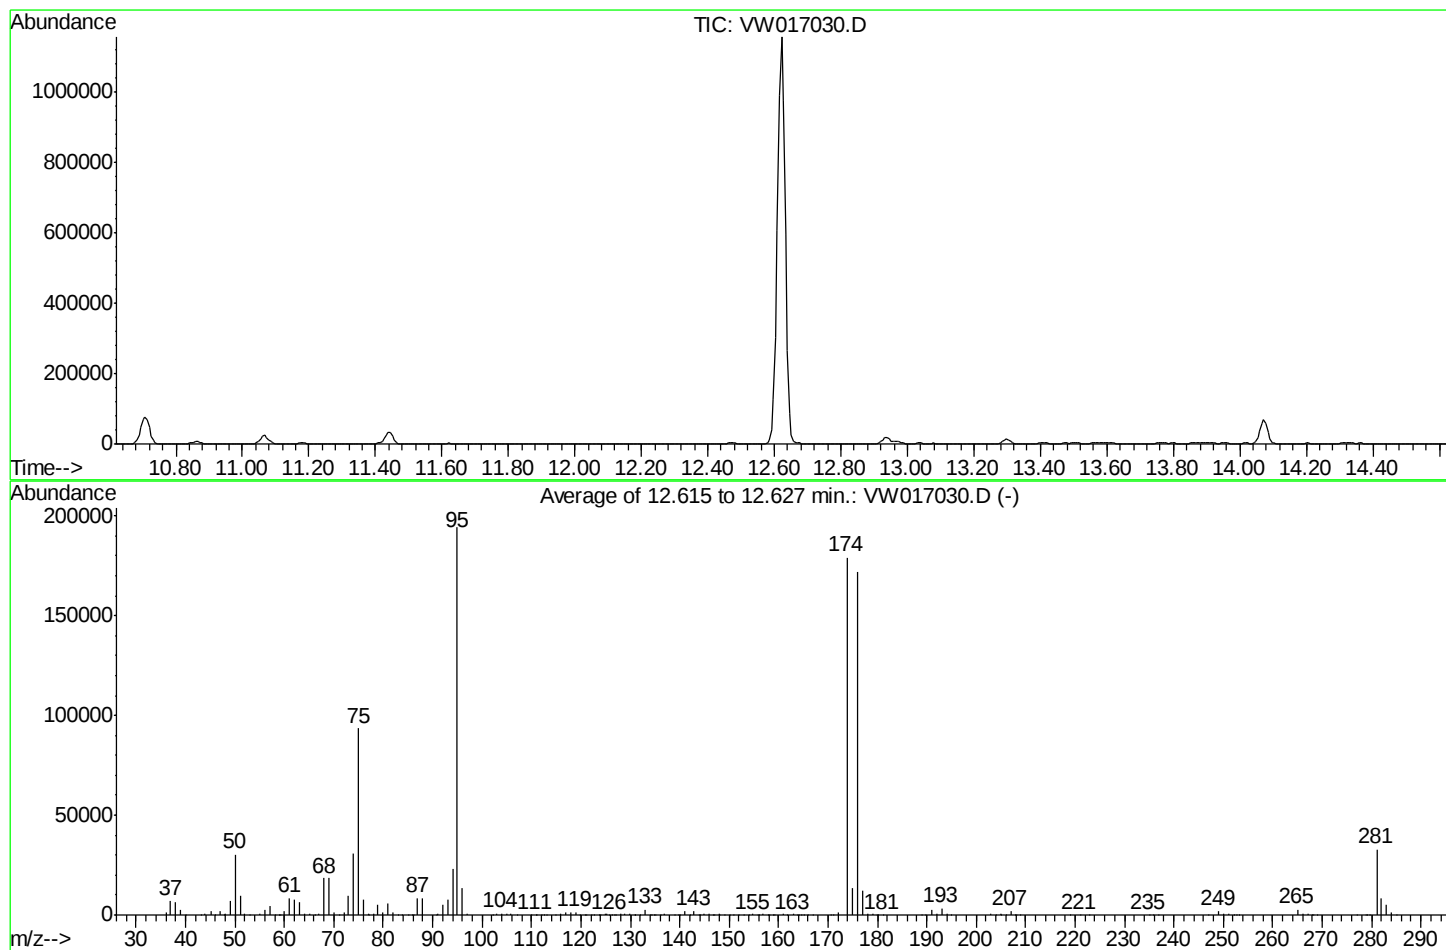

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	30418	PASS
75	95	30	80	48.1	93453	PASS
95	95	100	100	100.0	194282	PASS
96	95	5	9	6.8	13176	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.2	179093	PASS
175	174	5	9	7.4	13338	PASS
176	174	95	101	96.0	171840	PASS
177	176	5	9	7.0	12053	PASS

m/z	Abundance
36.00	1291.0
37.00	6490.0
38.00	5938.0
39.00	2620.0
40.00	226.0
43.10	76.0
43.90	1020.0
45.10	1436.0
46.10	133.0
47.00	1947.0
48.00	801.0
49.00	6148.0
50.00	27576.0
51.00	8420.0
52.00	393.0
55.00	262.0
56.00	2556.0
57.00	3912.0
58.10	276.0
59.20	98.0
60.00	1586.0
61.00	7819.0
62.00	7379.0
63.00	5785.0
64.00	744.0
65.00	660.0
66.10	76.0
66.90	454.0
68.00	16067.0
69.00	16736.0
70.00	1168.0
71.00	97.0
72.00	864.0
73.00	8090.0
74.00	27848.0
75.00	86376.0
76.00	7459.0
77.00	1174.0
78.00	949.0
78.90	4964.0
79.90	1424.0
80.90	5214.0
81.90	1319.0
83.10	195.0
86.00	307.0
87.00	8027.0
87.90	7538.0
90.90	667.0
92.00	5017.0
93.00	7410.0
94.00	20120.0
95.00	185152.0
96.00	12384.0
97.00	299.0
102.80	312.0
103.90	861.0
105.00	336.0
105.90	914.0
106.90	249.0
109.70	144.0
111.00	211.0
111.90	172.0
113.00	169.0
114.80	307.0
115.80	704.0
116.90	1262.0
117.90	730.0
118.80	1011.0
119.90	92.0
124.00	144.0
124.90	369.0
125.20	372.0
127.00	80.0
128.00	697.0
128.80	315.0
129.80	705.0
130.90	257.0
132.90	1028.0
134.00	326.0
134.80	411.0
136.10	114.0
137.00	357.0
140.90	1696.0
142.00	333.0
142.90	2110.0
143.70	88.0
144.10	76.0
144.90	394.0
145.90	318.0
146.80	360.0
148.10	486.0
149.00	136.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

150.00	226.0
150.90	53.0
151.90	81.0
152.90	217.0
153.80	191.0
154.90	557.0
155.80	108.0
156.90	366.0
157.80	143.0
159.00	240.0
160.80	366.0
162.90	202.0
164.10	57.0
164.70	119.0
170.50	83.0
172.00	893.0
173.90	185216.0
174.90	13333.0
175.90	182848.0
176.90	12713.0
178.00	321.0
178.90	352.0
179.80	81.0
188.90	233.0
190.90	1570.0
191.90	326.0
193.10	1537.0
194.10	327.0
195.00	204.0
202.90	151.0
204.90	429.0
206.00	71.0
207.00	1224.0
208.10	229.0
209.00	148.0
235.00	152.0
249.00	1090.0
249.80	269.0
251.00	422.0
252.00	112.0
253.00	69.0
265.10	1491.0
266.10	293.0
266.90	262.0
267.90	133.0
278.90	88.0
281.10	17224.0
282.10	4419.0
283.10	3261.0
284.10	554.0
285.10	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

m/z	Abundance
36.00	1695.0
37.00	7853.0
38.00	7186.0
39.00	2778.0
40.00	195.0
43.20	134.0
44.00	1247.0
45.00	1828.0
46.00	216.0
47.00	2606.0
48.00	1018.0
49.00	7586.0
50.00	33584.0
51.00	10727.0
52.00	513.0
52.80	74.0
55.00	573.0
56.00	2773.0
57.00	5195.0
58.00	217.0
59.00	264.0
60.00	1694.0
61.00	9169.0
62.00	8468.0
63.00	7373.0
64.00	750.0
65.00	569.0
66.10	100.0
67.00	572.0
68.00	20984.0
69.00	20304.0
70.10	1495.0
71.00	110.0
72.10	1184.0
73.00	10437.0
74.00	36216.0
75.00	105208.0
76.10	8753.0
77.10	1365.0
77.90	920.0
78.90	6040.0
79.90	1647.0
80.90	6631.0
81.90	1365.0
83.00	163.0
83.70	92.0
85.80	253.0
86.00	253.0
86.90	9420.0
87.90	9496.0
91.00	669.0
92.00	6149.0
93.00	9102.0
94.00	26984.0
95.00	216000.0
96.00	14912.0
97.00	355.0
102.20	54.0
102.90	521.0
103.90	1148.0
104.90	444.0
105.90	925.0
107.00	364.0
109.80	290.0
110.70	245.0
111.10	186.0
112.00	237.0
112.80	198.0
114.80	348.0
116.00	785.0
116.90	1373.0
118.00	1185.0
118.90	1510.0
119.80	98.0
120.70	84.0
122.00	52.0
122.70	68.0
123.90	132.0
124.90	676.0
125.20	750.0
125.80	345.0
127.10	102.0
127.90	848.0
128.80	385.0
129.80	953.0
131.00	360.0
131.80	83.0
133.00	2883.0
134.40	471.0
134.80	600.0
136.90	554.0
138.90	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

139.90	165.0
140.90	1971.0
141.90	197.0
142.90	2253.0
143.90	123.0
144.90	416.0
145.80	429.0
147.00	448.0
147.90	601.0
148.90	292.0
150.00	294.0
151.70	141.0
152.80	116.0
153.90	172.0
154.90	654.0
156.00	151.0
156.90	526.0
157.70	113.0
158.80	304.0
160.80	465.0
161.70	57.0
162.90	588.0
163.90	173.0
165.00	350.0
171.00	138.0
172.00	1201.0
173.90	200256.0
175.00	14360.0
175.90	192704.0
176.90	13840.0
177.90	617.0
179.00	779.0
180.10	115.0
180.90	71.0
188.90	316.0
191.00	2386.0
192.10	513.0
193.00	2884.0
193.90	532.0
194.80	320.0
203.00	318.0
203.90	111.0
205.10	456.0
206.00	112.0
207.00	2234.0
207.80	436.0
209.00	307.0
219.10	53.0
220.90	146.0
222.80	70.0
235.00	269.0
247.00	65.0
249.10	2182.0
250.00	837.0
251.00	907.0
252.10	219.0
253.10	67.0
265.00	2744.0
266.00	752.0
267.10	722.0
267.90	238.0
269.10	90.0
278.90	239.0
279.50	176.0
281.00	34000.0
282.10	8723.0
283.00	4284.0
284.10	1042.0
285.00	285.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

m/z	Abundance
36.00	1299.0
37.00	7654.0
38.00	6624.0
39.00	2452.0
40.10	225.0
43.20	182.0
44.00	1238.0
45.00	1676.0
46.00	257.0
47.00	1905.0
47.80	1022.0
49.00	6827.0
50.00	30096.0
51.00	9600.0
52.00	483.0
53.00	113.0
54.90	420.0
56.00	2503.0
57.00	4733.0
58.00	190.0
59.00	506.0
60.00	1726.0
61.00	8157.0
62.00	7755.0
63.00	6302.0
63.90	631.0
65.00	622.0
66.10	97.0
66.90	391.0
68.00	17928.0
69.00	17984.0
70.00	1304.0
70.90	152.0
72.00	925.0
73.00	10602.0
74.00	28832.0
75.00	88776.0
76.00	7492.0
76.90	918.0
78.00	783.0
78.90	5194.0
80.00	1536.0
81.00	5576.0
82.00	1151.0
82.90	220.0
83.70	98.0
85.00	74.0
86.10	288.0
87.00	8026.0
88.00	7235.0
90.80	646.0
92.00	5165.0
93.00	7512.0
94.00	22120.0
95.00	181696.0
96.00	12232.0
97.00	424.0
103.00	751.0
104.00	870.0
104.90	380.0
105.80	796.0
107.00	155.0
110.00	366.0
110.90	454.0
112.10	246.0
112.60	165.0
113.00	151.0
114.90	355.0
115.90	630.0
116.90	1437.0
118.00	1128.0
118.90	1652.0
119.90	159.0
121.00	183.0
122.70	62.0
123.70	123.0
125.00	1768.0
126.20	293.0
126.70	99.0
128.00	651.0
129.00	369.0
129.90	644.0
130.80	379.0
131.90	148.0
133.00	4315.0
135.10	628.0
136.00	102.0
137.00	305.0
139.00	82.0
139.70	97.0
140.00	92.0
141.00	1523.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

141.90	189.0
142.90	2051.0
143.90	144.0
144.90	374.0
145.80	338.0
146.70	447.0
147.90	721.0
149.00	296.0
149.90	250.0
150.90	66.0
151.90	123.0
152.90	111.0
153.80	117.0
154.80	558.0
156.10	159.0
156.80	399.0
158.00	90.0
158.80	225.0
159.10	224.0
160.90	493.0
161.80	79.0
162.90	783.0
163.90	107.0
165.00	437.0
166.00	80.0
166.80	76.0
170.90	198.0
172.00	1146.0
173.90	151808.0
175.00	12323.0
175.90	139968.0
176.90	9607.0
178.00	636.0
179.00	1138.0
180.00	137.0
181.10	179.0
189.00	324.0
189.70	87.0
191.00	3600.0
192.00	782.0
193.00	5210.0
194.00	694.0
194.90	481.0
203.10	567.0
203.90	92.0
204.90	750.0
206.10	222.0
207.00	3377.0
207.90	550.0
209.00	406.0
219.00	79.0
221.00	212.0
223.00	95.0
235.00	467.0
235.90	121.0
236.90	87.0
247.10	82.0
249.00	3470.0
250.00	635.0
251.00	1478.0
252.00	310.0
252.70	159.0
265.00	3558.0
266.10	1050.0
267.00	727.0
268.20	186.0
269.00	85.0
276.90	71.0
279.20	339.0
281.10	48296.0
282.00	12709.0
283.10	8112.0
284.10	1827.0
285.20	489.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25

Scan 1750 (12.573 min): VW017030.D
BFB25

m/z	Abundance
40.00	158.0
41.10	72.0
42.90	52.0
44.00	269.0
55.10	53.0
57.10	65.0
206.90	72.0
281.10	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB25