

Data File : VW006472.D
Acq On : 30 Oct 2018 01:00
Operator : SY/AP
Sample : J5624-08RE
Misc : 4.53G/5ML/MSVOA_W/SOIL
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
PA-SB-02BRE

Quant Time: Nov 04 01:28:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	150185	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	216438	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	128688	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	24192	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	76474	61.42	ug/l	0.00
Spiked Amount 50.000			Recovery	=	122.84%	
35) Dibromofluoromethane	7.88	113	80240	62.74	ug/l	0.00
Spiked Amount 50.000			Recovery	=	125.48%	
50) Toluene-d8	10.33	98	214270	44.04	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.08%	
62) 4-Bromofluorobenzene	12.62	95	35706	19.54	ug/l	0.00
Spiked Amount 50.000			Recovery	=	39.08%	
Target Compounds						
20) Methylene Chloride	4.92	84	5187	2.387	ug/l #	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW006472.D
Acq On : 30 Oct 2018 01:00
Operator : SY/AP
Sample : J5624-08RE
Misc : 4.53G/5ML/MSVOA_W/SOIL
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
PA-SB-02BRE

Quant Time: Nov 04 01:28:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration

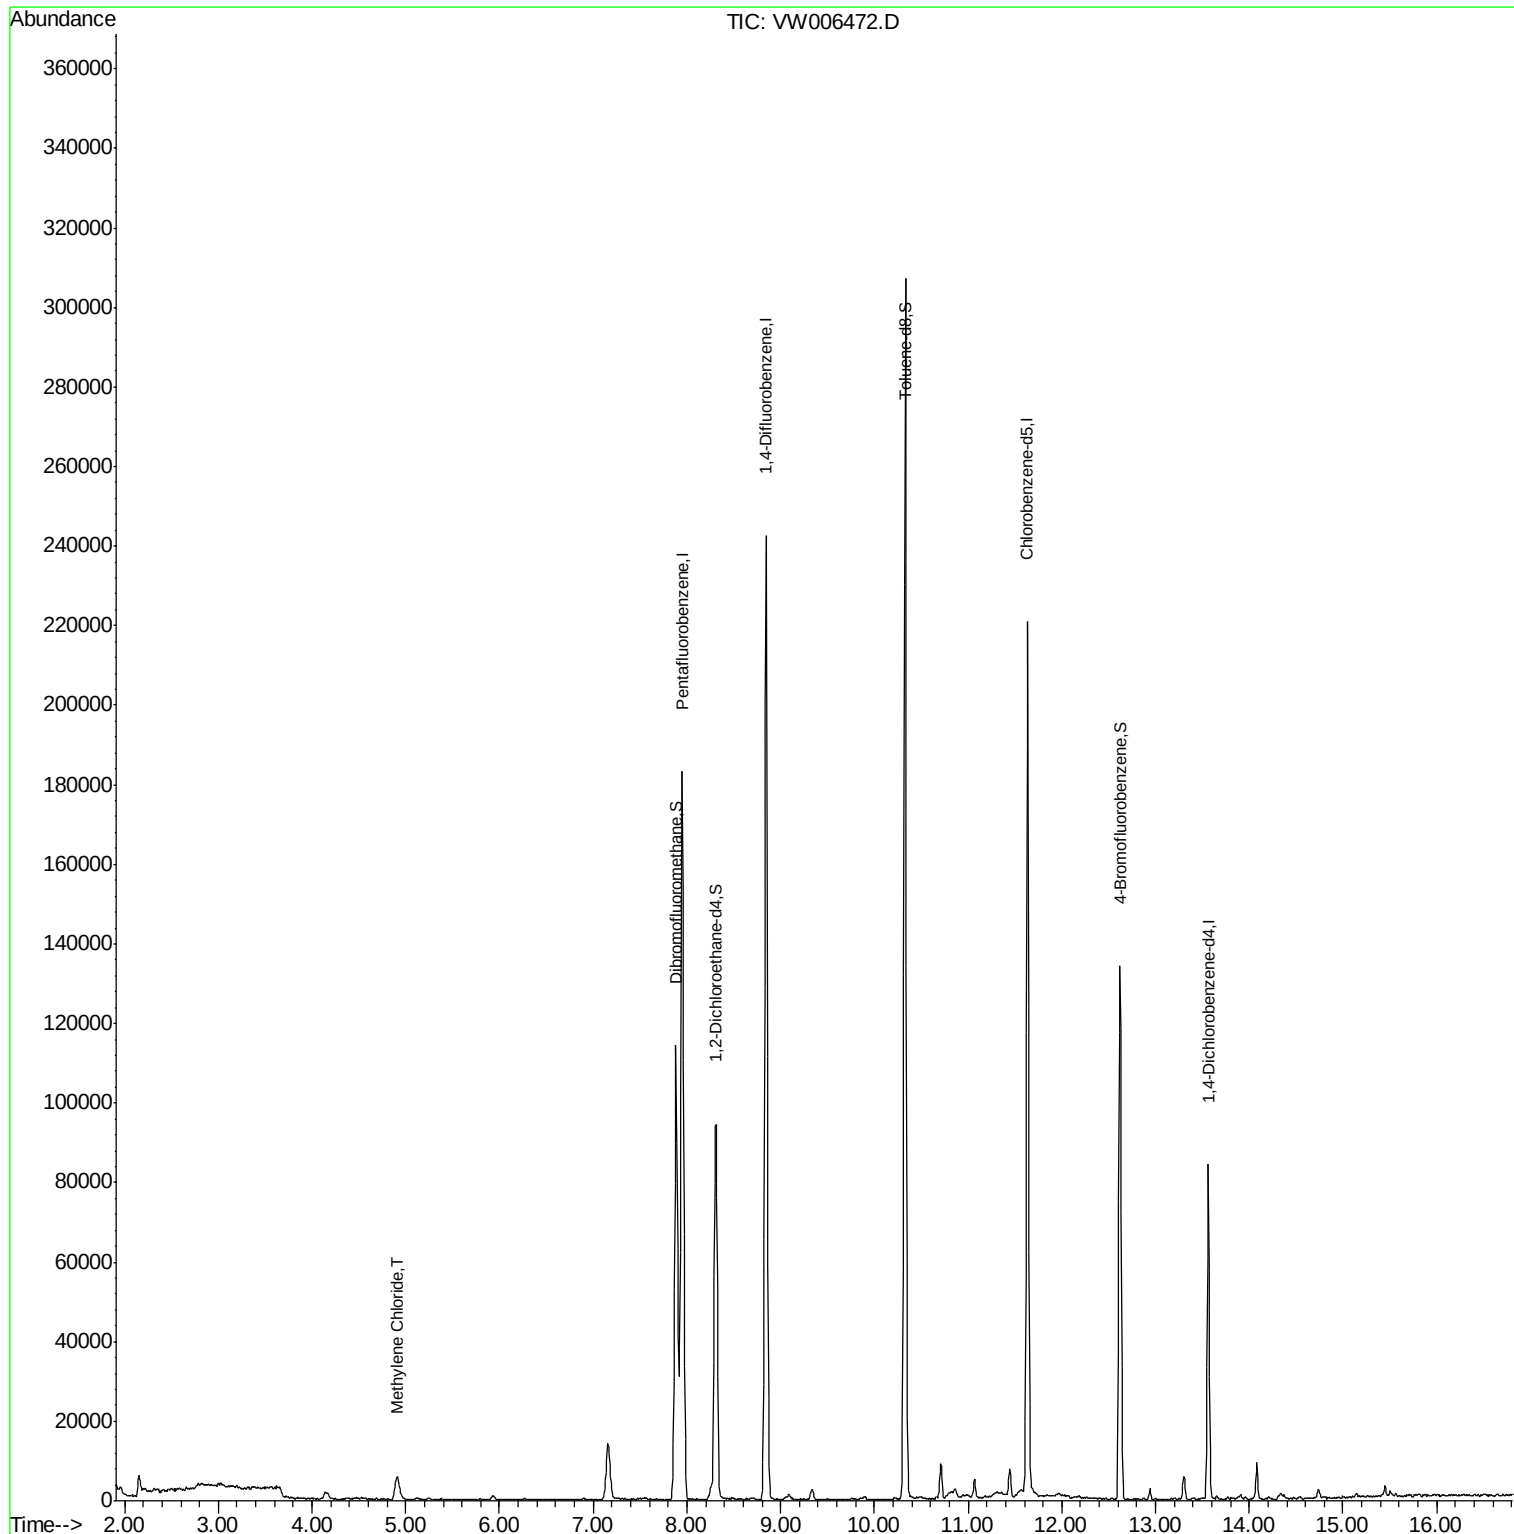

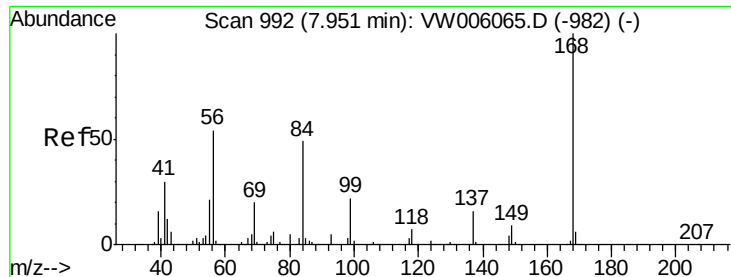

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW006472.D

Acq: 30 Oct 2018 01:00

Instrument :

MSVOA_W

ClientSampleId :


PA-SB-02BRE

Tgt Ion:168 Resp: 150185

Ion Ratio Lower Upper

168 100

99 46.3 39.9 59.9

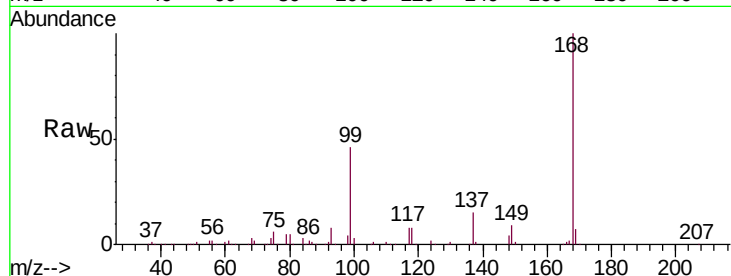

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

80000

60000



40000

20000

0

7.90 8.00 8.10

Time-->

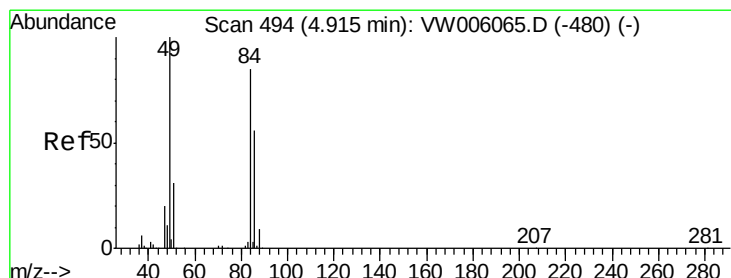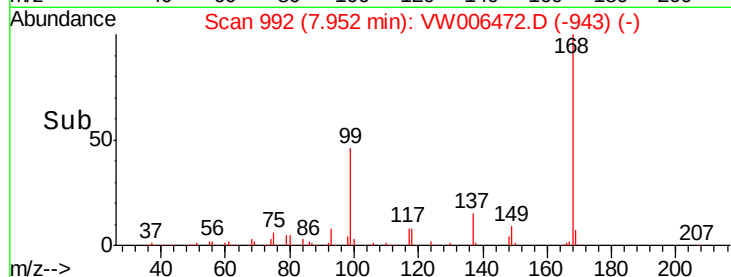

#20

Methylene Chloride

Concen: 2.387 ug/l

RT: 4.92 min Scan# 494

Delta R.T. 0.00 min

Lab File: VW006472.D

Acq: 30 Oct 2018 01:00

Tgt Ion: 84 Resp: 5187


Ion Ratio Lower Upper

84 100

49 94.6 93.6 140.4

51 27.9 29.0 43.4#

86 52.6 52.6 79.0#

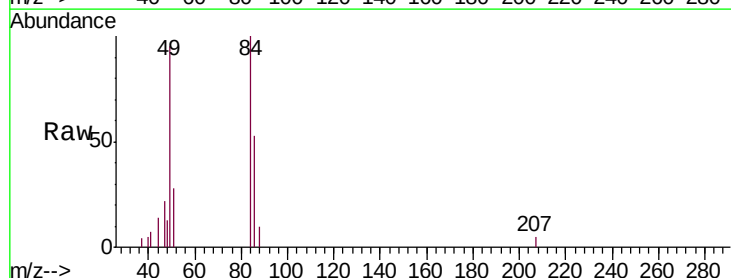

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

2500

2000

1500


1000


500

0

4.80 4.90 5.00

Time-->




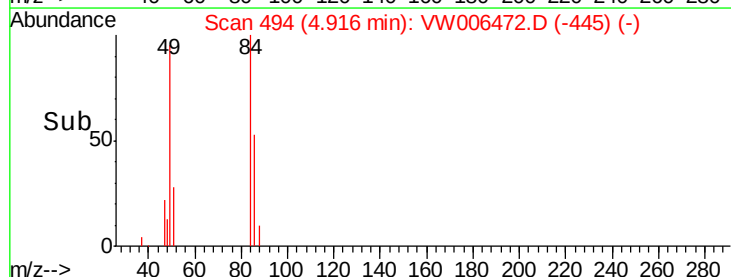


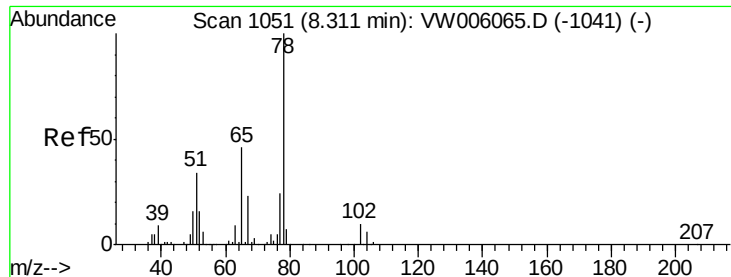

#33
 1,2-Dichloroethane-d4
 Concen: 61.419 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. 0.00 min
 Lab File: VW006472.D
 Acq: 30 Oct 2018 01:00




Instrument :
 MSVOA_W
 ClientSampleId :
 PA-SB-02BRE


Tgt Ion: 65 Resp: 76474
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 101.0

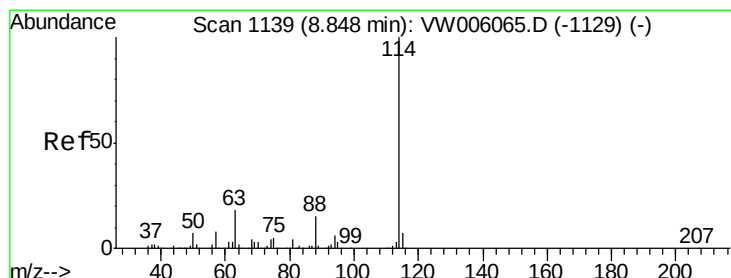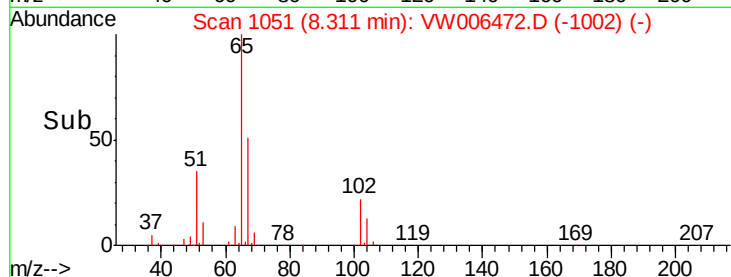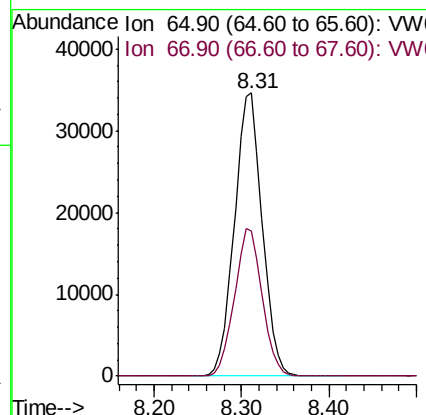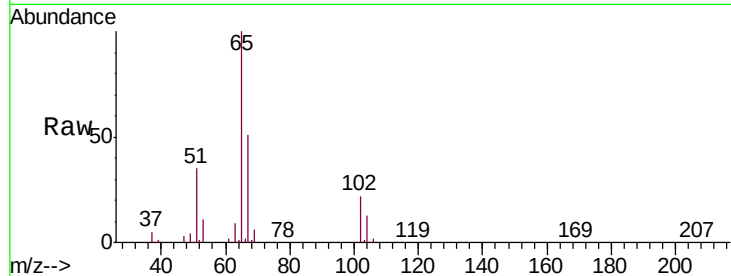

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.01 min
 Lab File: VW006472.D
 Acq: 30 Oct 2018 01:00

Tgt Ion: 114 Resp: 216438
 Ion Ratio Lower Upper
 114 100
 63 17.6 0.0 36.8
 88 14.8 0.0 29.0

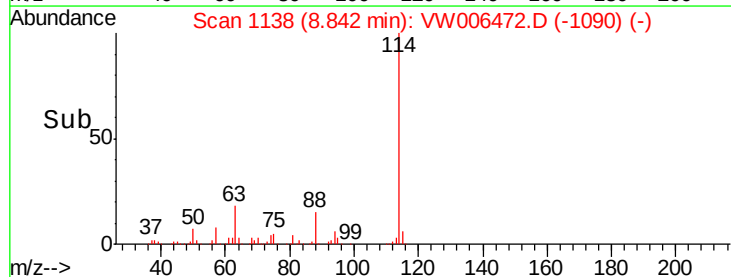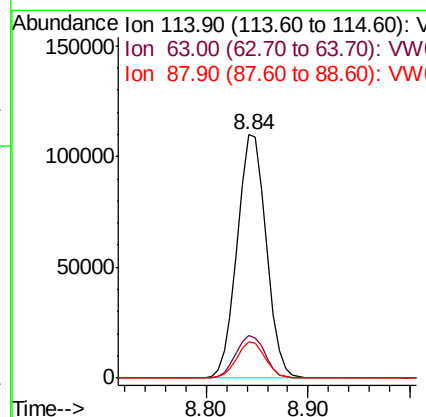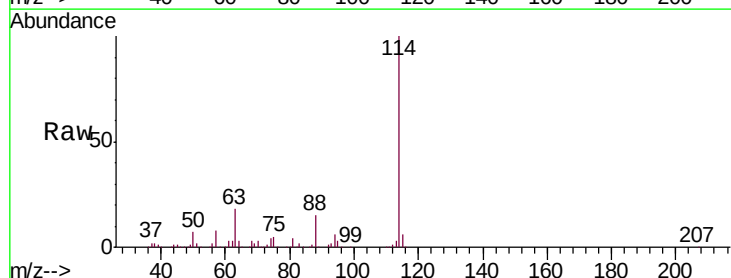

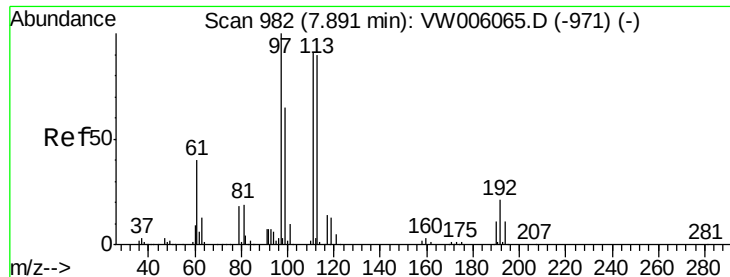

#35

Dibromofluoromethane

Concen: 62.740 ug/l

RT: 7.88 min Scan# 981

Delta R.T. -0.01 min

Lab File: VW006472.D

Acq: 30 Oct 2018 01:00

Instrument :

MSVOA_W

ClientSampleId :

PA-SB-02BRE


Tgt Ion:113 Resp: 80240

Ion Ratio Lower Upper

113 100

111 101.4 81.4 122.0




192 23.7 18.7 28.1

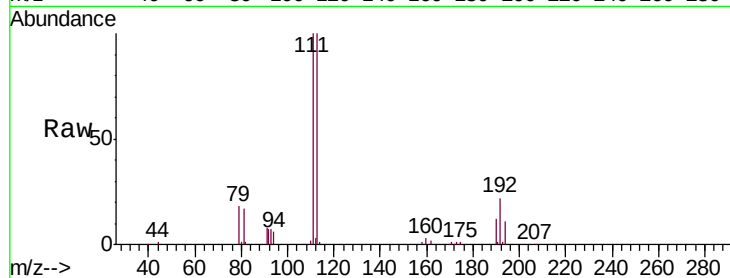

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

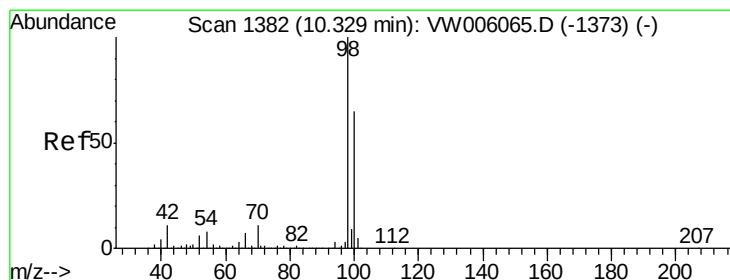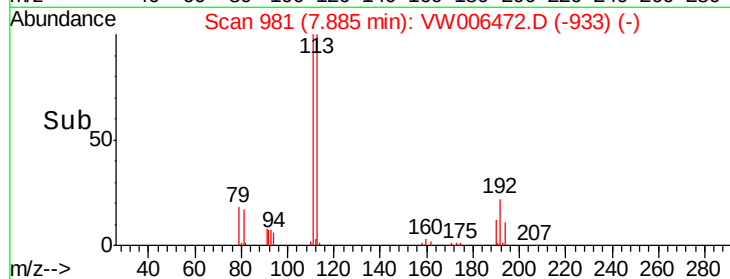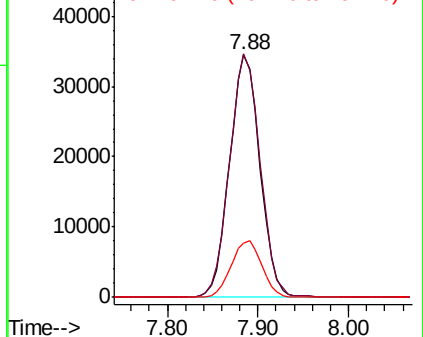

#50

Toluene-d8

Concen: 44.037 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.00 min

Lab File: VW006472.D


Acq: 30 Oct 2018 01:00

Tgt Ion: 98 Resp: 214270

Ion Ratio Lower Upper



98 100


100 64.7 51.6 77.4

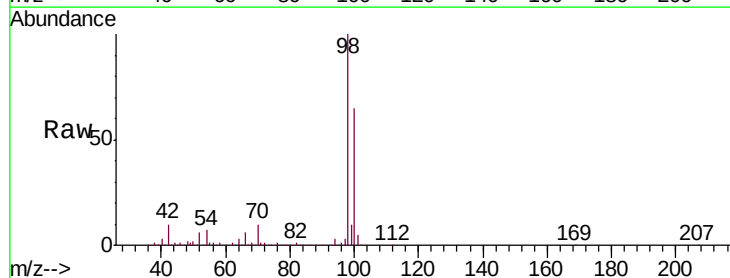

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

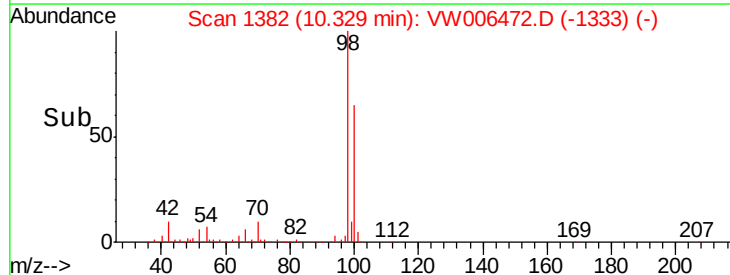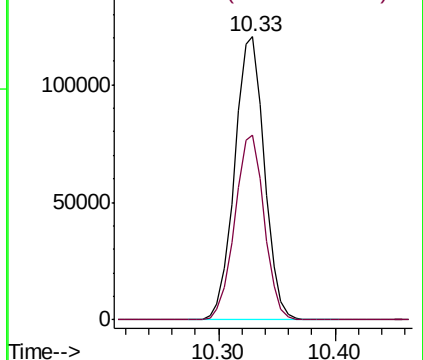

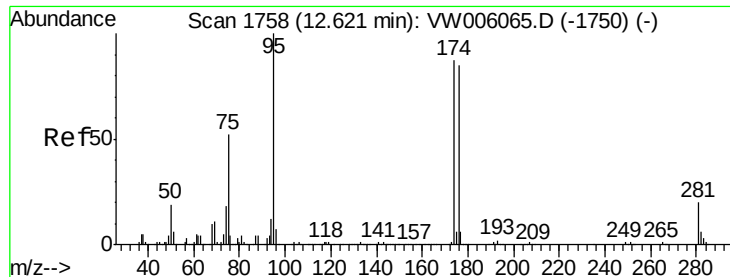

#62

4-Bromofluorobenzene

Concen: 19.538 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW006472.D

Acq: 30 Oct 2018 01:00

Instrument :

MSVOA_W

ClientSampleId :

PA-SB-02BRE


Tgt Ion: 95 Resp: 35706

Ion Ratio Lower Upper

95 100

174 100.4 0.0 186.0




176 94.8 0.0 181.6

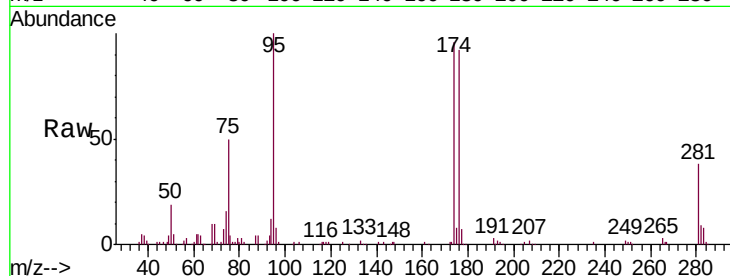

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

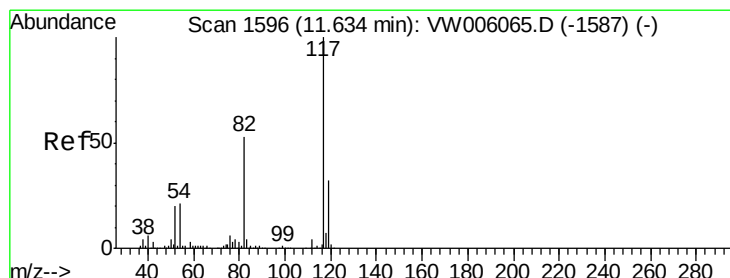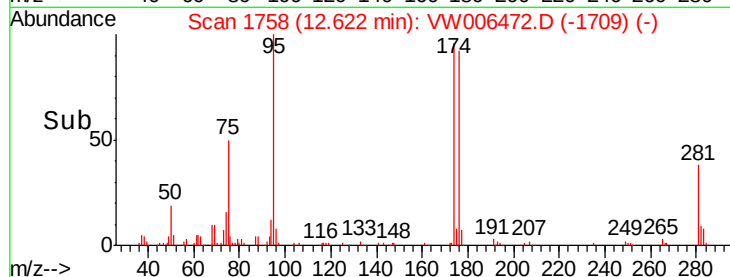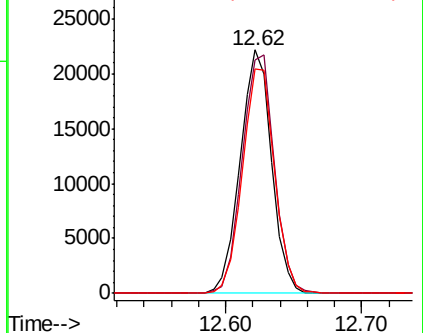

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.00 min

Lab File: VW006472.D

Acq: 30 Oct 2018 01:00


Tgt Ion: 117 Resp: 128688

Ion Ratio Lower Upper

117 100

82 50.8 42.1 63.1



119 30.9 25.8 38.6

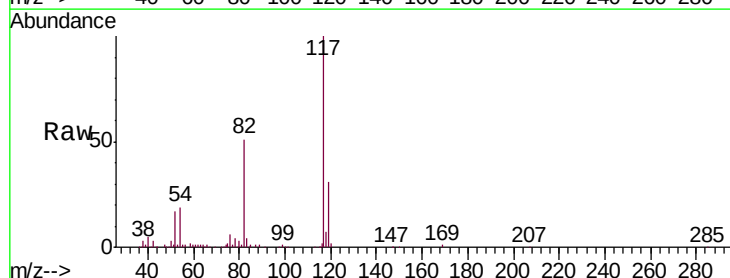


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

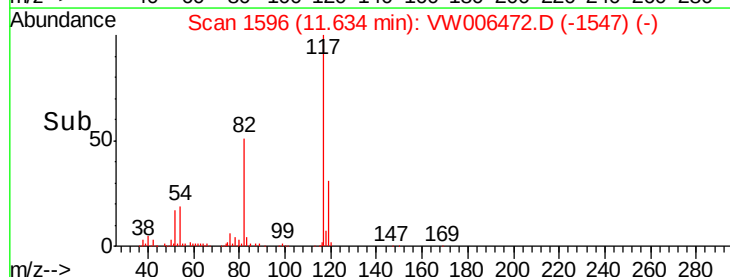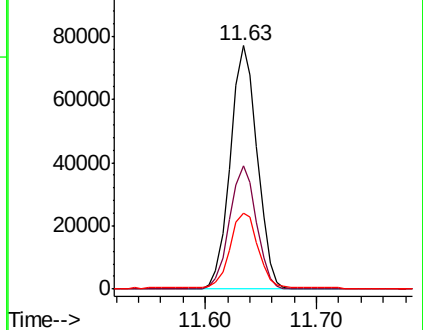

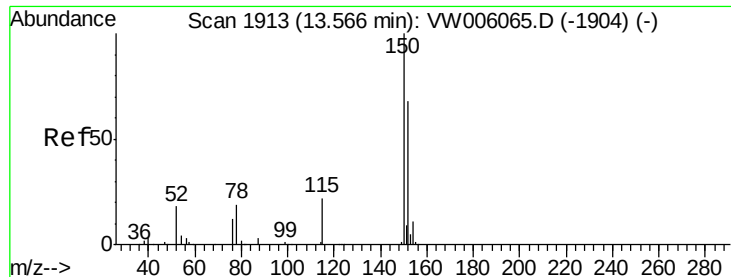

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.01 min

Lab File: VW006472.D

Acq: 30 Oct 2018 01:00

Instrument :

MSVOA_W

ClientSampleId :

PA-SB-02BRE


Tgt Ion:152 Resp: 24192

Ion Ratio Lower Upper

152 100

115 52.1 27.8 83.3

150 157.8 0.0 349.2

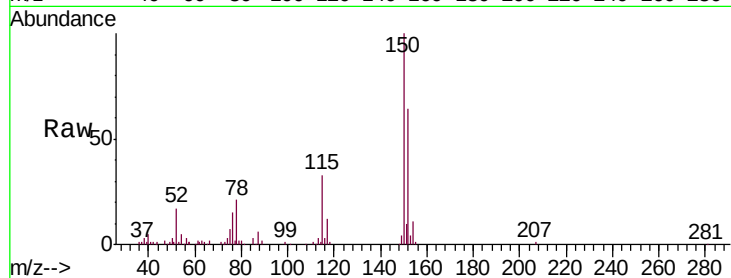

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

