


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW103118\
 Data File : VW006466.D
 Acq On : 29 Oct 2018 20:42
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Title : SW846 8260
 Last Update : Thu Oct 18 17:01:24 2018

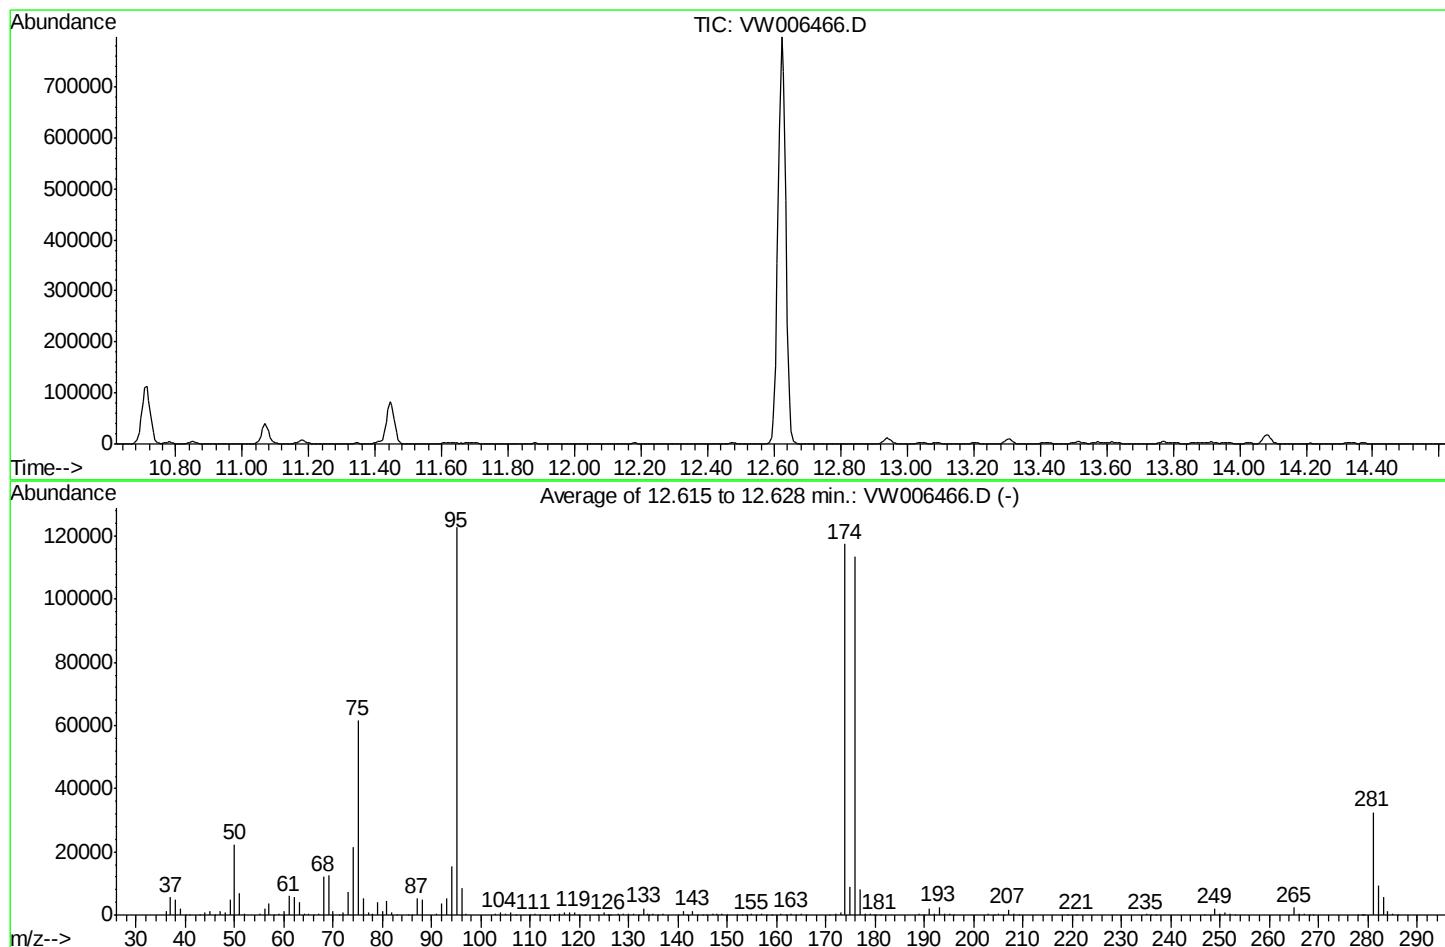

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	22253	PASS
75	95	30	60	50.1	61469	PASS
95	95	100	100	100.0	122786	PASS
96	95	5	9	6.9	8521	PASS
173	174	0.00	2	0.8	943	PASS
174	95	50	100	95.7	117448	PASS
175	174	5	9	7.5	8827	PASS
176	174	95	101	96.8	113706	PASS
177	176	5	9	7.3	8295	PASS