

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110119\
 Data File : VW013896.D
 Acq On : 01 Nov 2019 14:07
 Operator : SY/VA
 Sample : VW1101SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 02 00:16:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 02 00:12:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	302040	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	292734	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	167663	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	112288	23.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.56%
7) Chloroethane-d5	2.89	69	89462	23.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.32%
10) 1,1-Dichloroethene-d2	4.03	63	164471	17.18	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.72%
20) 2-Butanone-d5	7.08	46	88981	52.62	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.24%
24) Chloroform-d	7.65	84	220890	23.21	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.84%
26) 1,2-Dichloroethane-d4	8.30	65	126835	24.76	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.04%
29) Benzene-d6	8.27	84	488318	24.90	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.60%
33) 1,2-Dichloropropane-d6	9.27	67	145716	24.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.20%
37) Toluene-d8	10.32	98	455848	24.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.00%
38) trans-1,3-Dichloropropene-	10.58	79	62664	23.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.48%
39) 2-Hexanone-d5	10.92	63	71484	53.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.02%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129792	24.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.88%
61) 1,2-Dichlorobenzene-d4	13.85	152	164104	24.73	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.92%


Target Compounds					Ovalue
42) cis-1,3-Dichloropropene	10.04	75	3690	0.449 ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW110119\
Data File : VW013896.D
Acq On : 01 Nov 2019 14:07
Operator : SY/VA
Sample : VW1101SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 02 00:16:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110119S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 02 00:12:22 2019
Response via : Initial Calibration

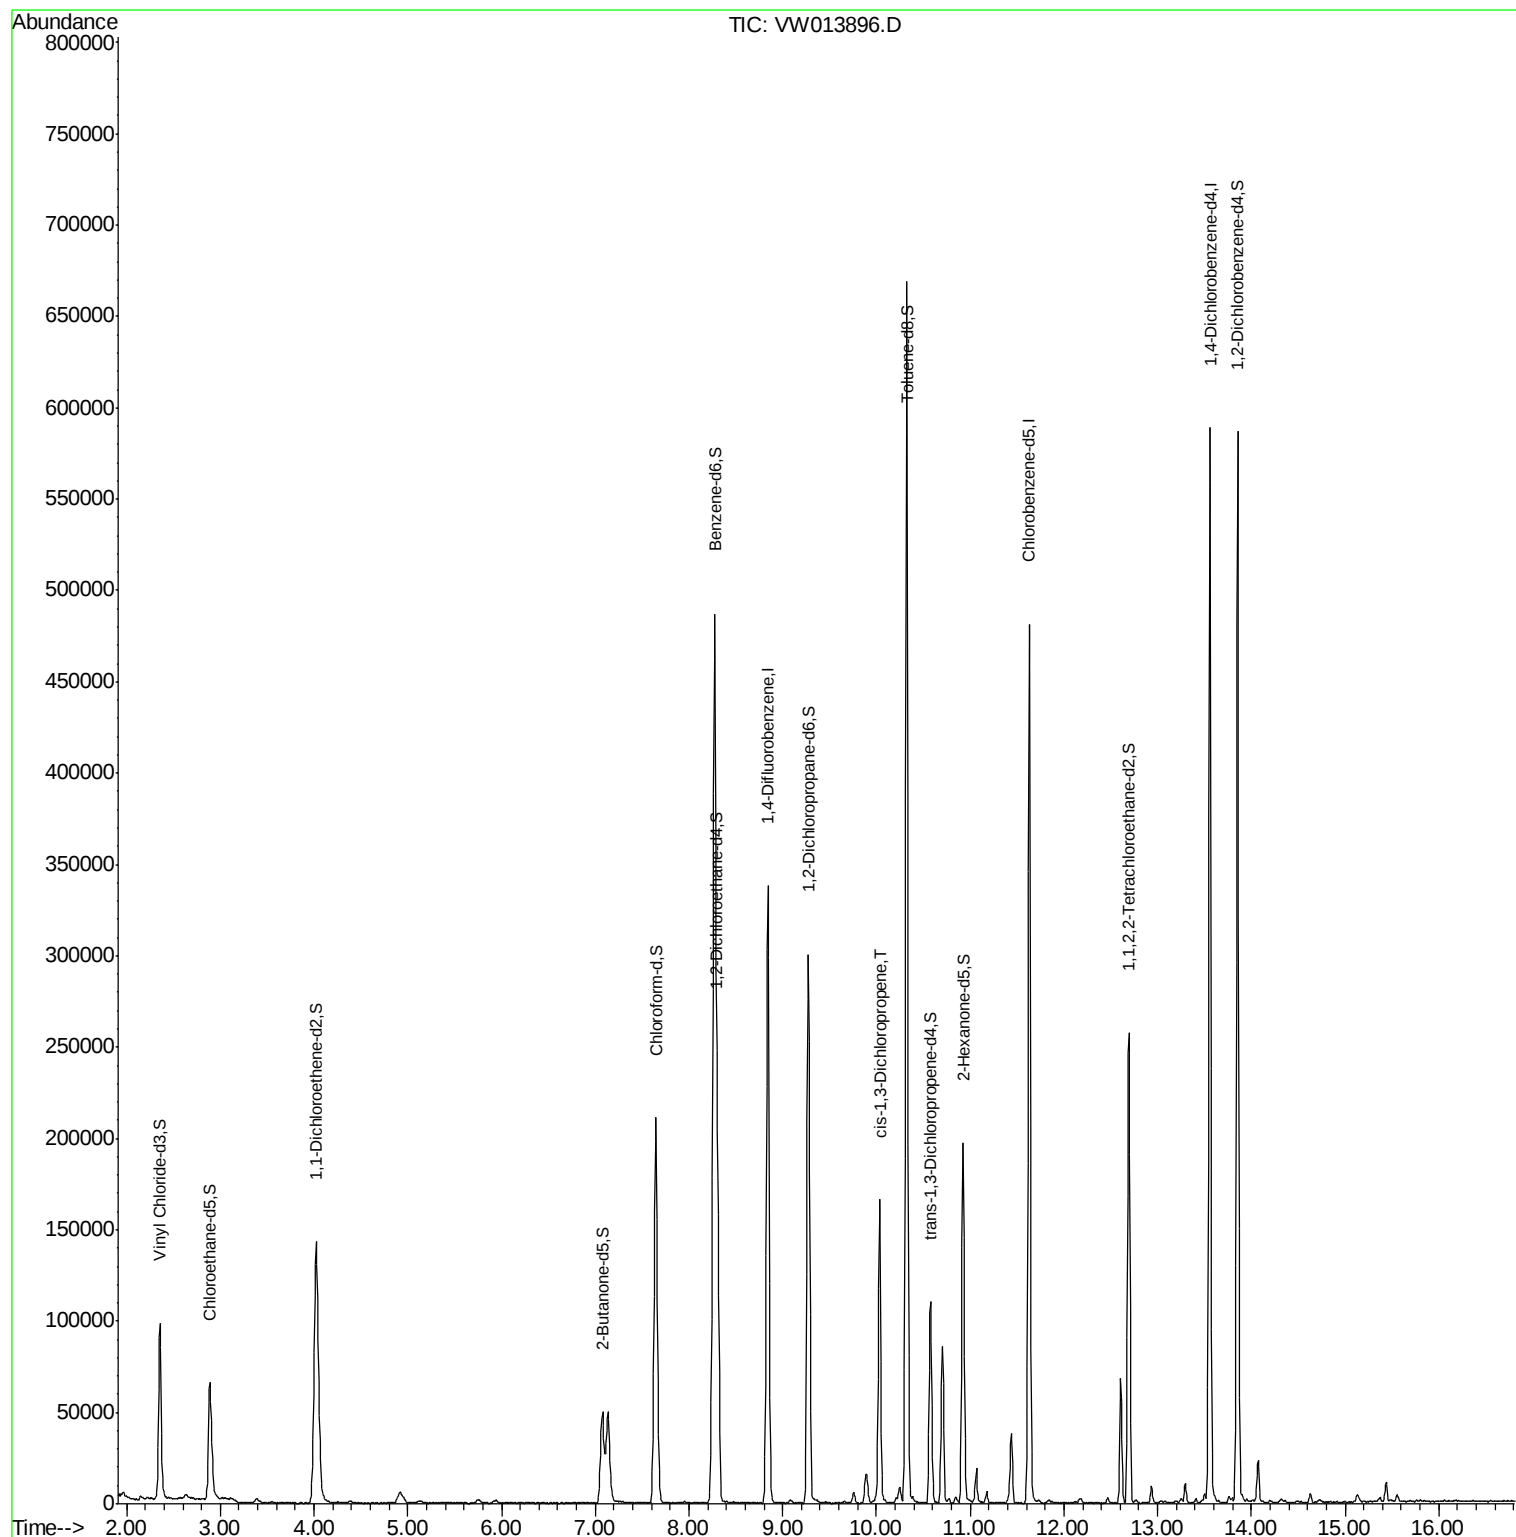

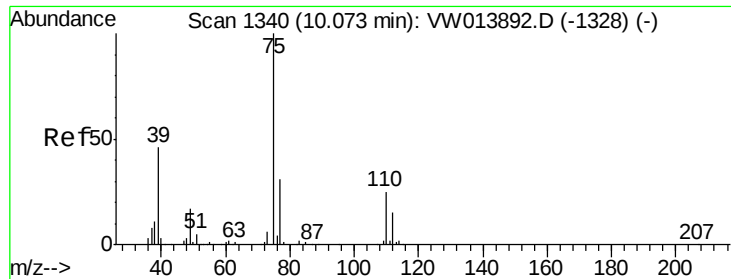

#42
 cis-1,3-Dichloropropene
 Concen: 0.449 ug/L
 RT: 10.04 min Scan# 1334
 Delta R.T. -0.04 min
 Lab File: VW013896.D
 Acq: 01 Nov 2019 14:07

Instrument :
 MSVOA_W
 ClientSampleId :

Tot Ion: 75 Resp: 3690
 Ion Ratio Lower Upper
 75 100
 77 43.0 21.8 40.4#

