



Dichlorodifluoromethane

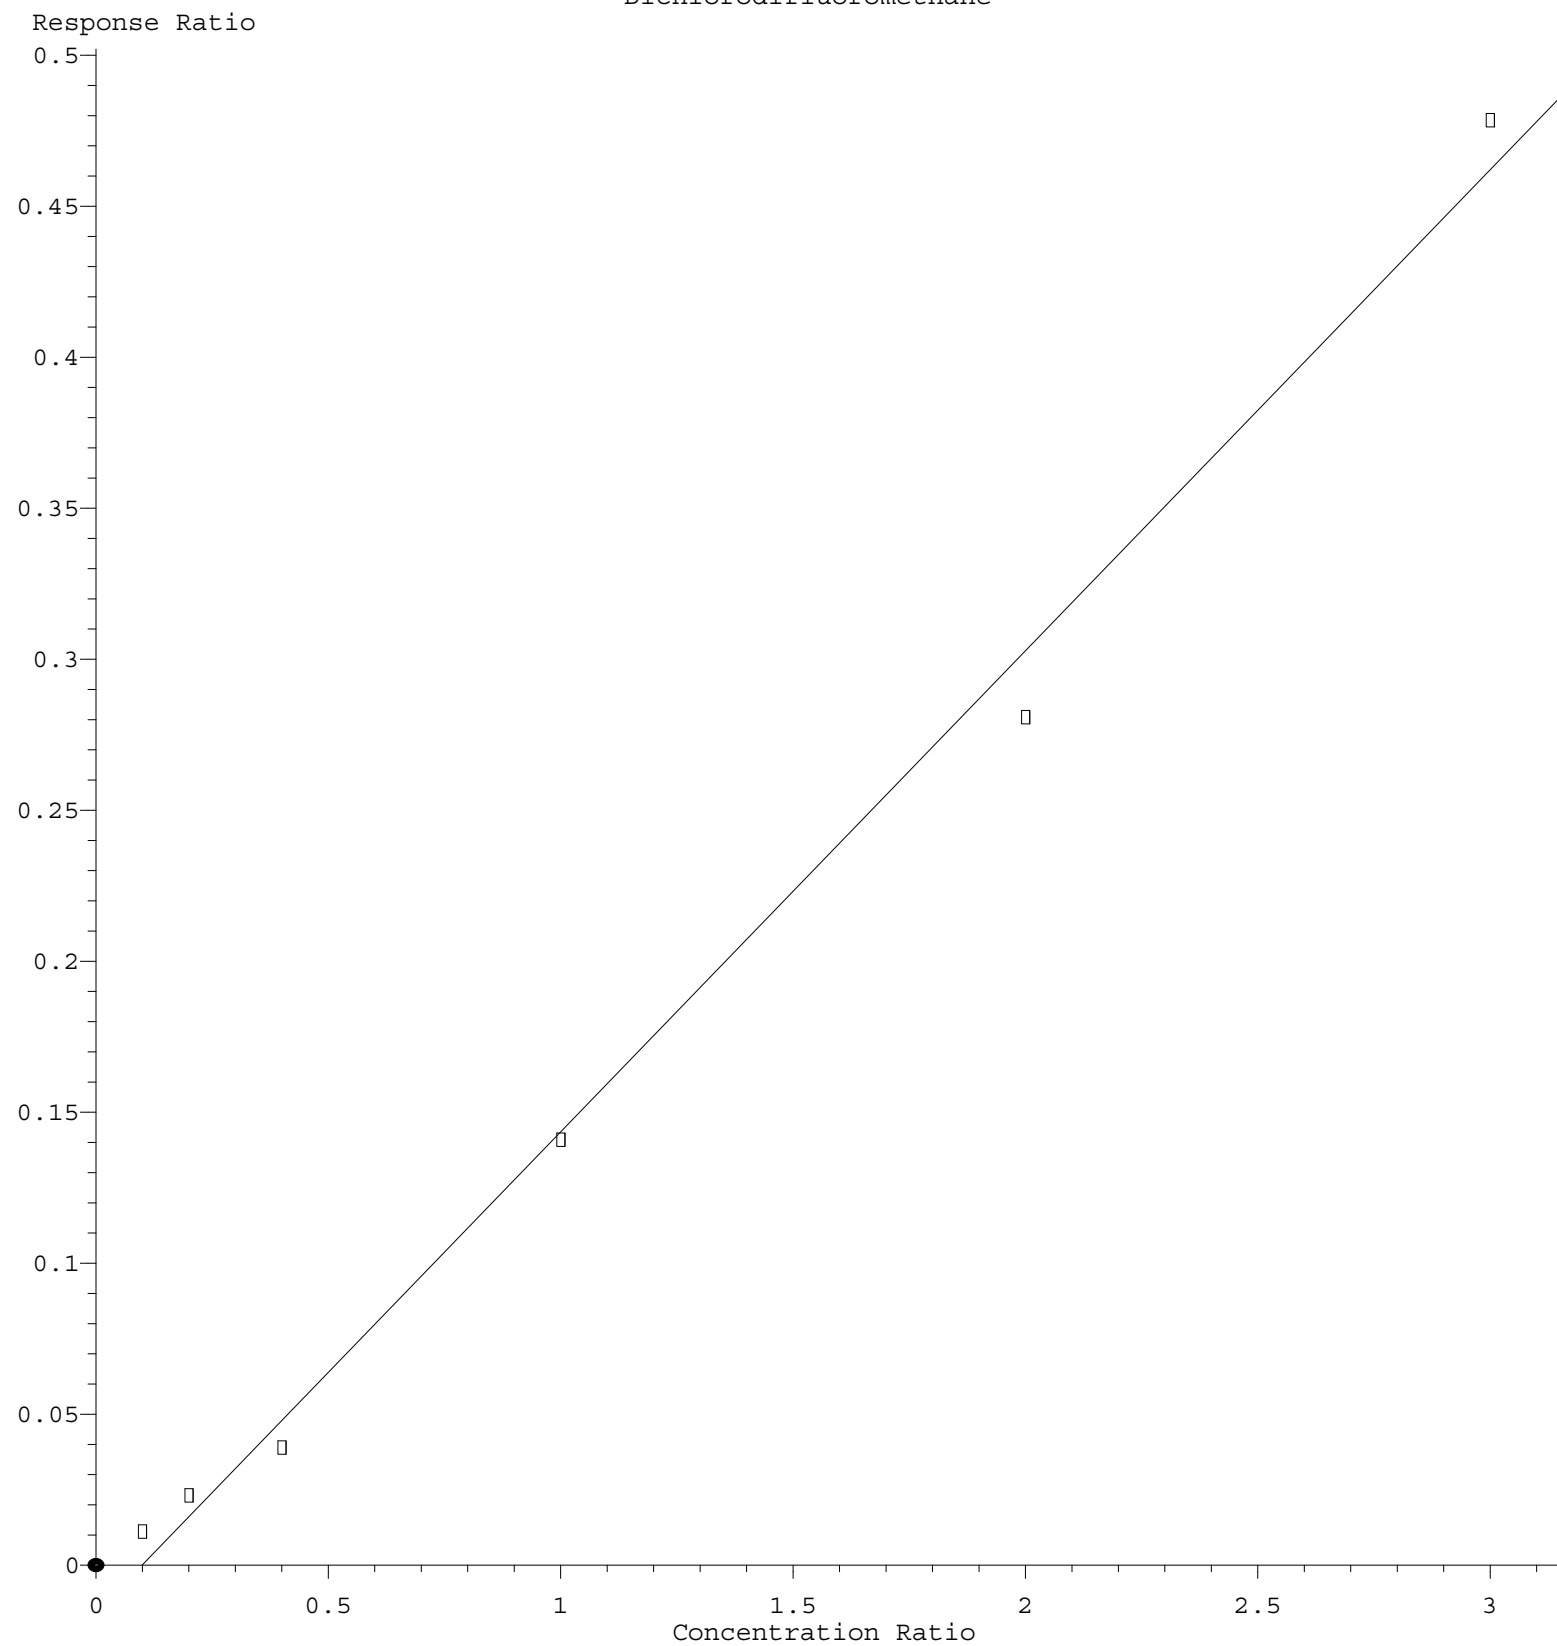

Response = 1.594e-001 * Amt - 1.574e-002
 Coef of Det (r^2) = 0.994119 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
 Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

Acetone


Response Ratio

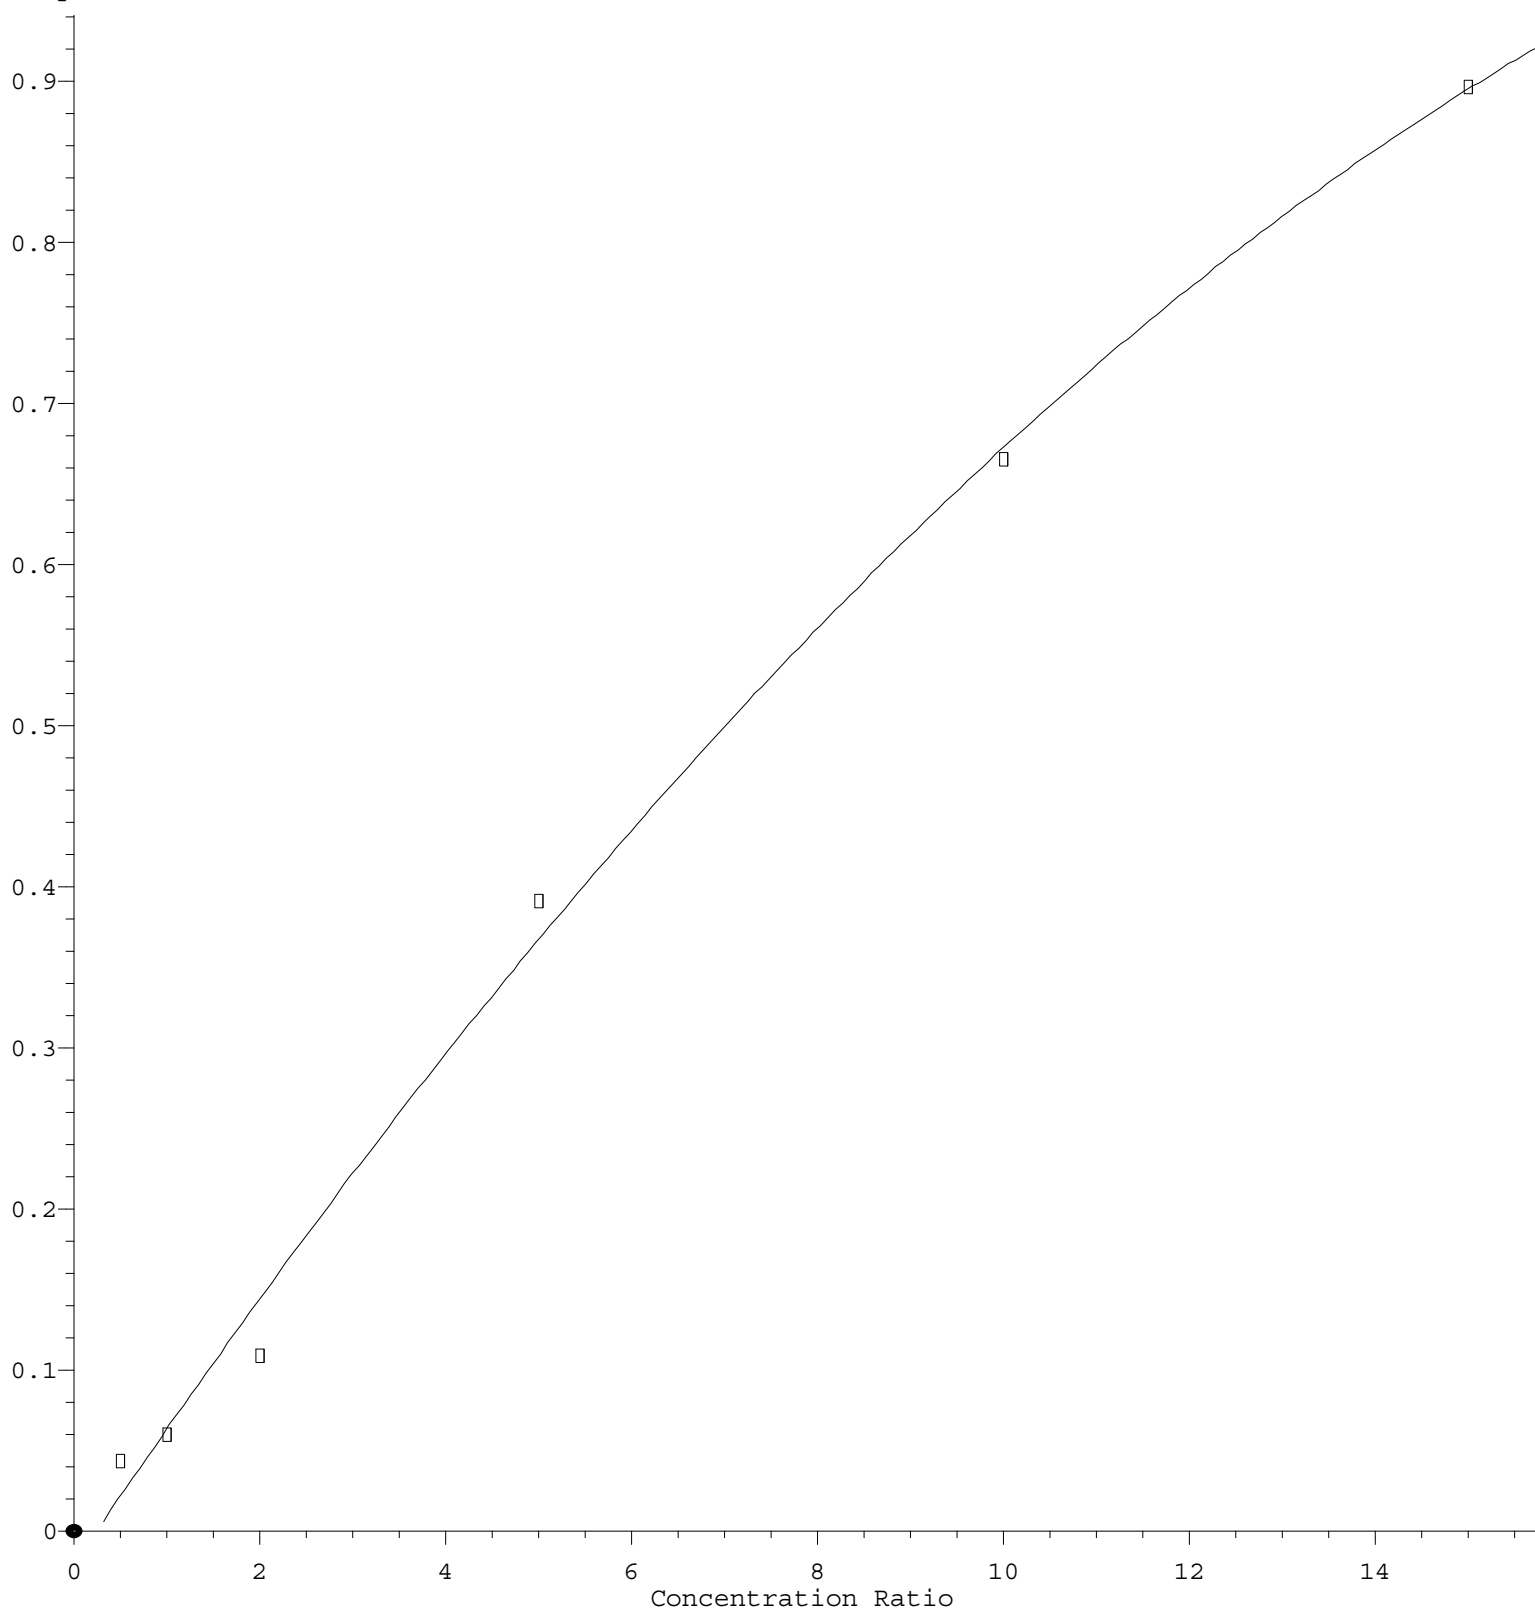

$R = -1.655e-003 A^2 + 8.588e-002 A - 2.067e-002$
 Coef of Det (r^2) = 0.996266 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
 Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

N-amyl acetate

Response Ratio

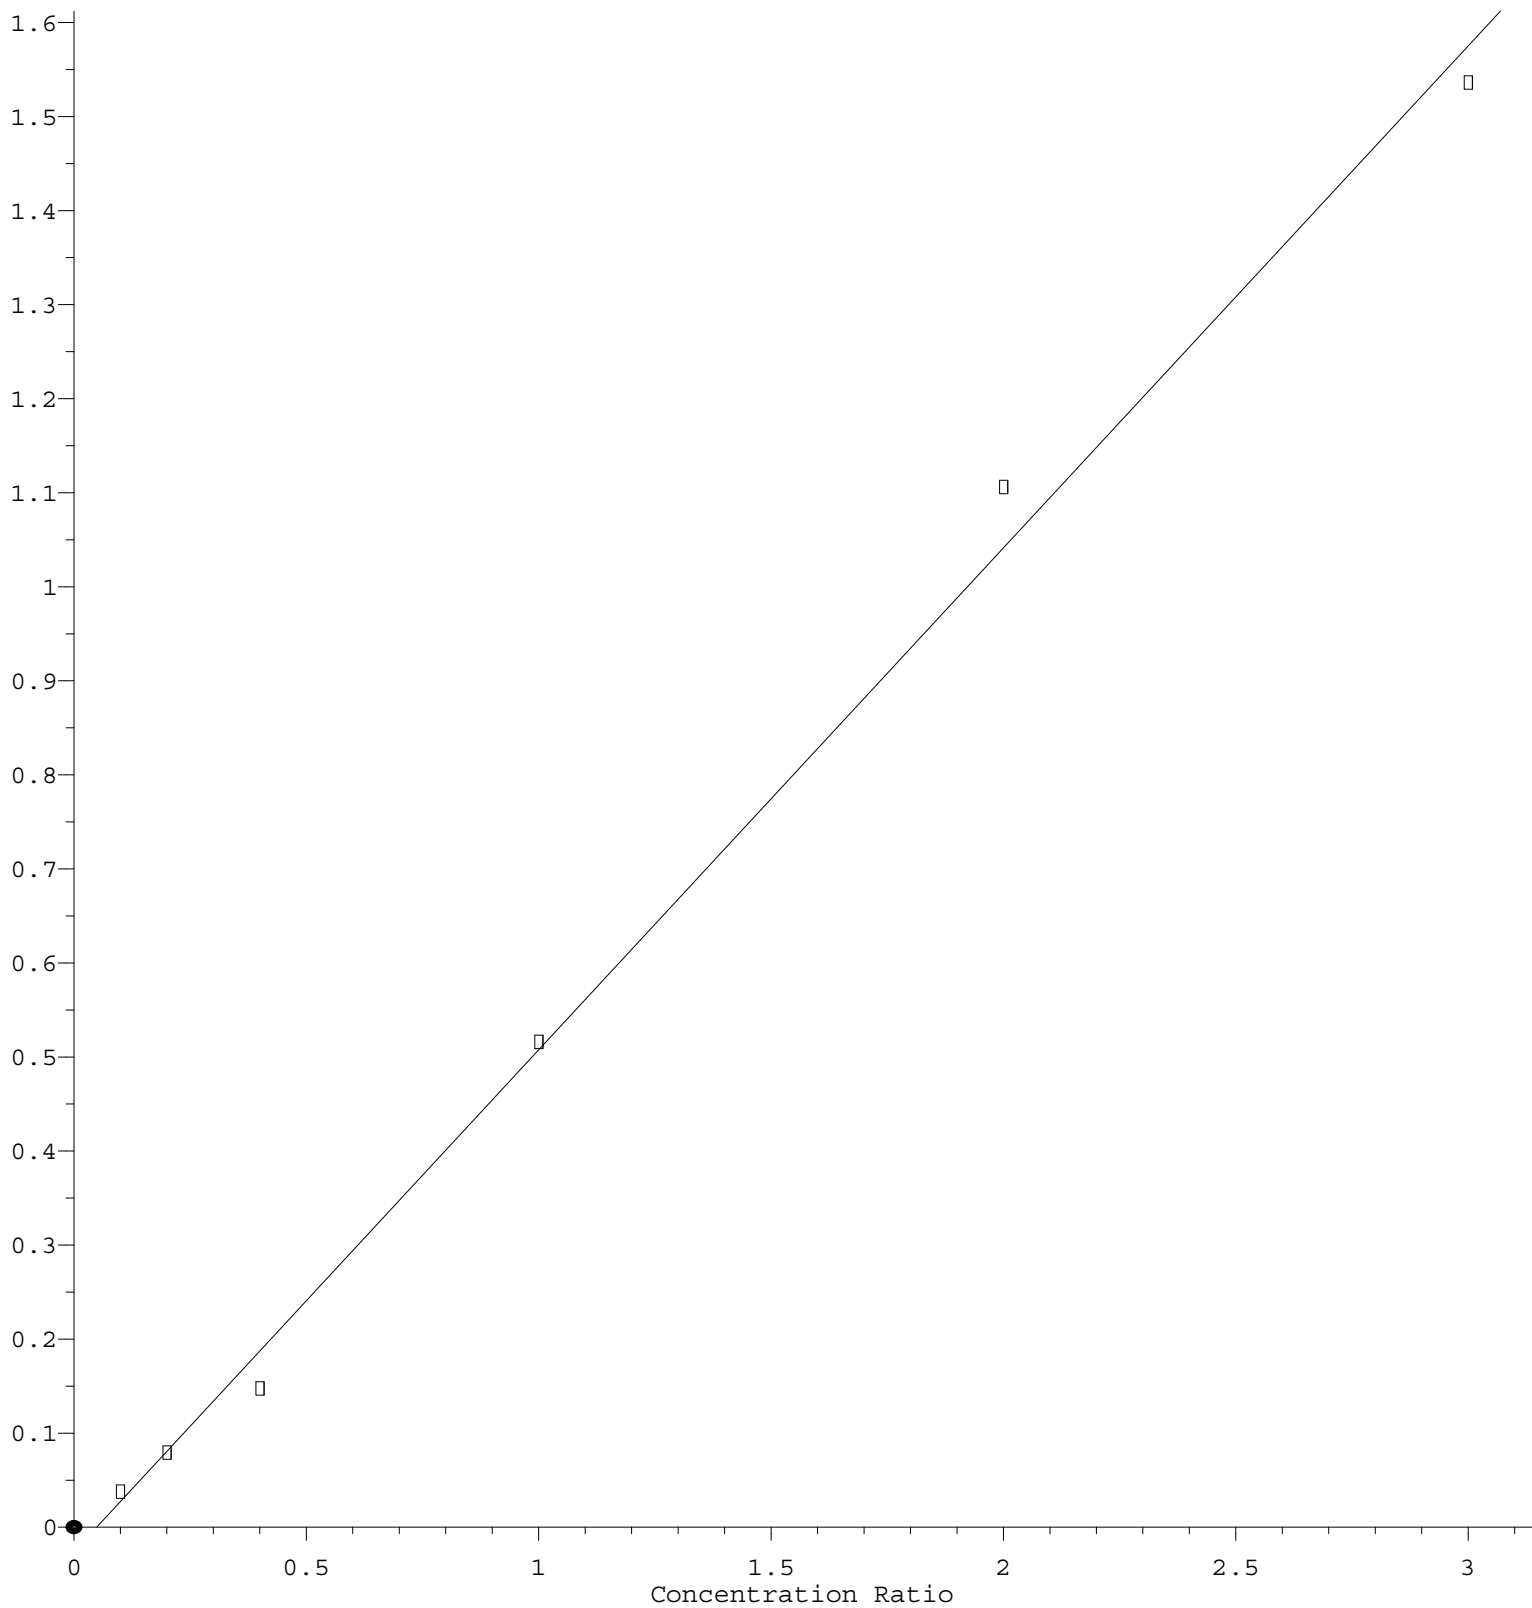


$$\text{Response} = 5.340\text{e-}001 * \text{Amt} - 2.591\text{e-}002$$

Coef of Det (r^2) = 0.996120 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M


Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

trans-1,4-Dichloro-2-butene

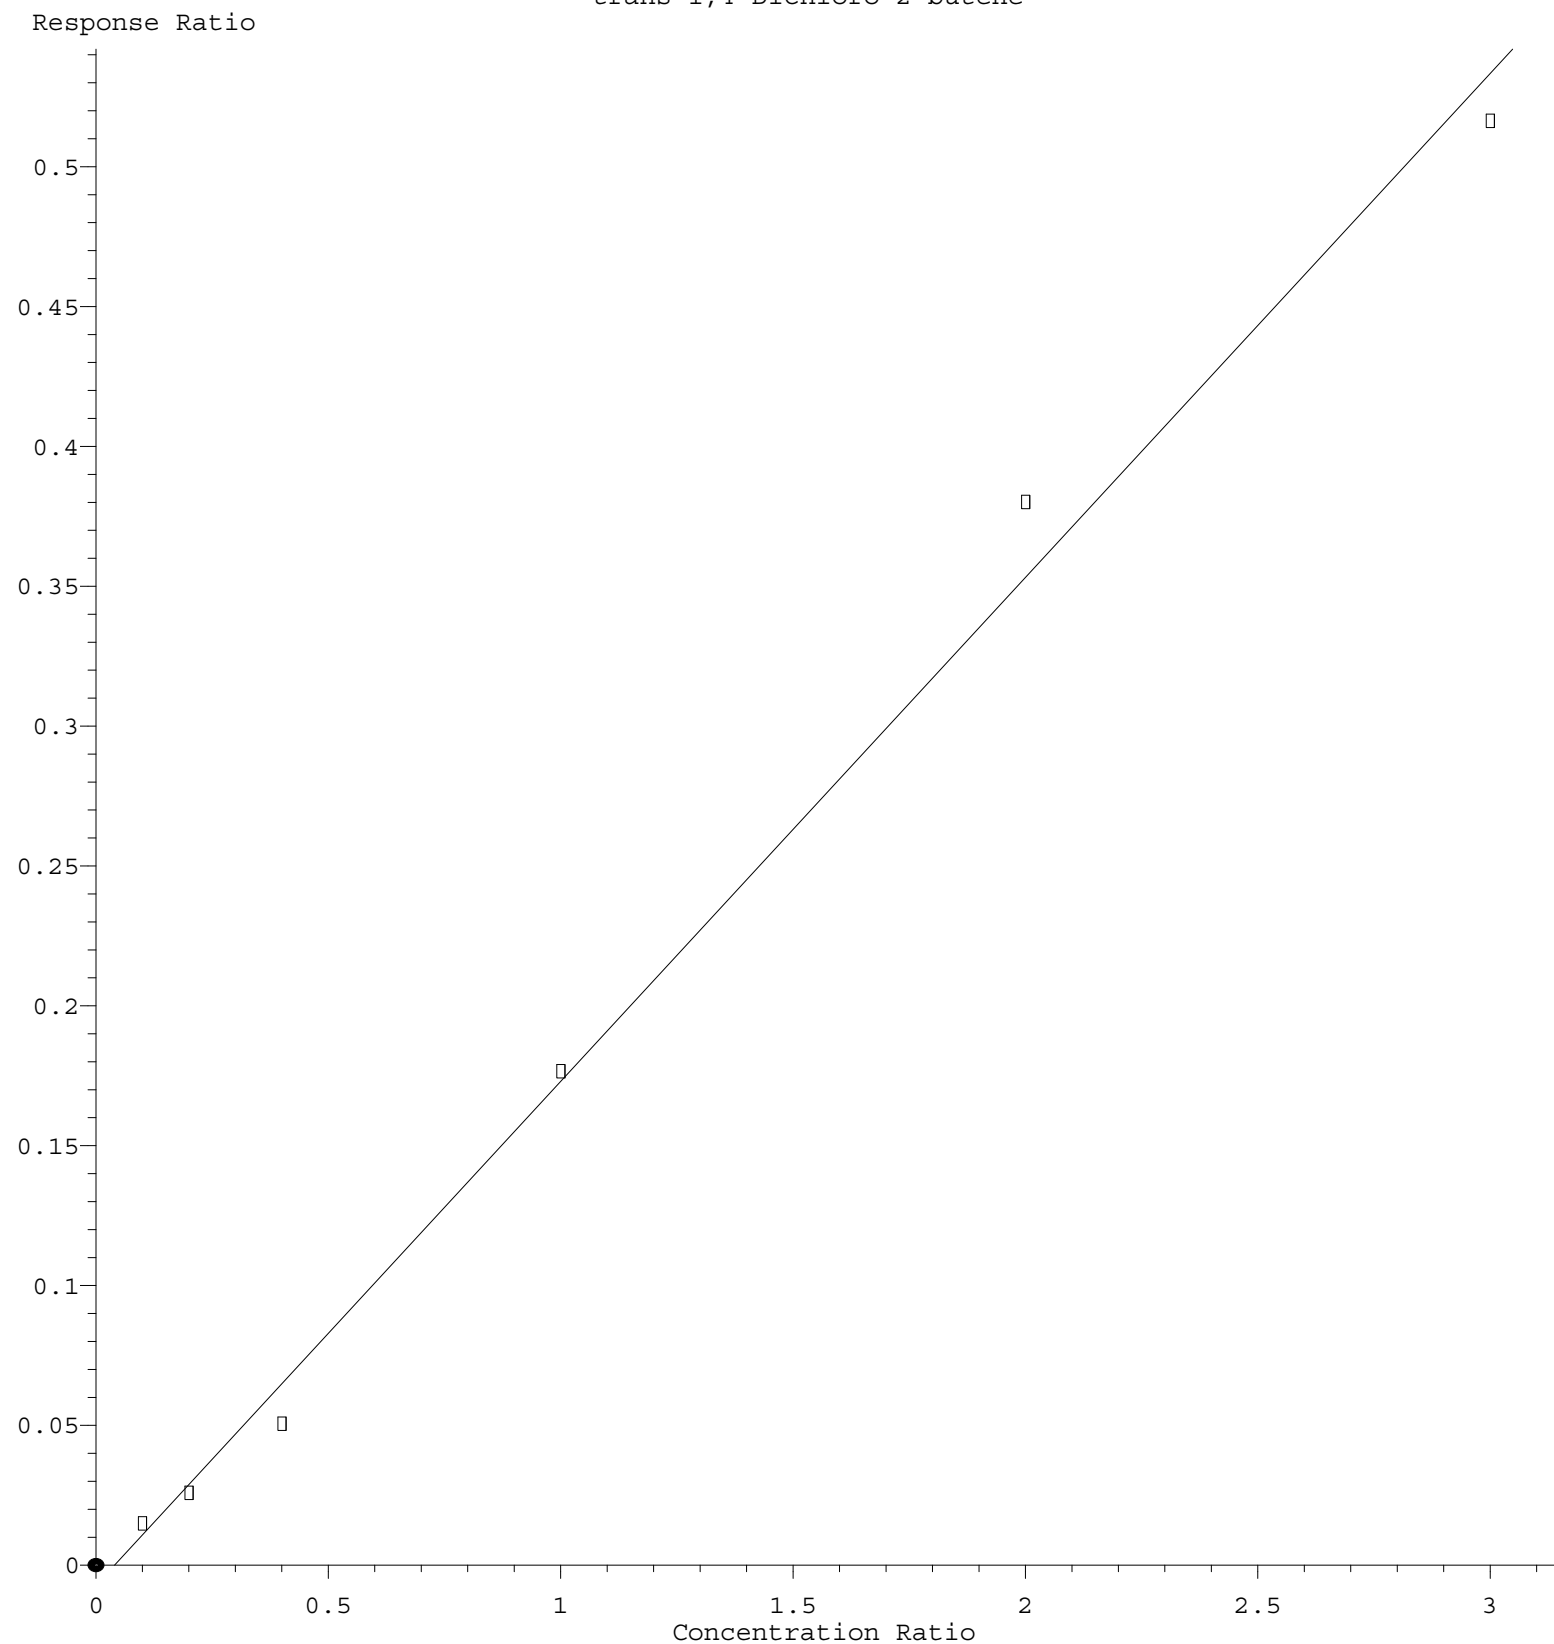

Response = $1.802 \times 10^{-1} \times \text{Amt} - 7.167 \times 10^{-3}$
Coef of Det (r^2) = 0.994280 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
Calibration Table Last Updated: Tue Nov 02 04:55:07 2021


1,2-Dibromo-3-Chloropropane

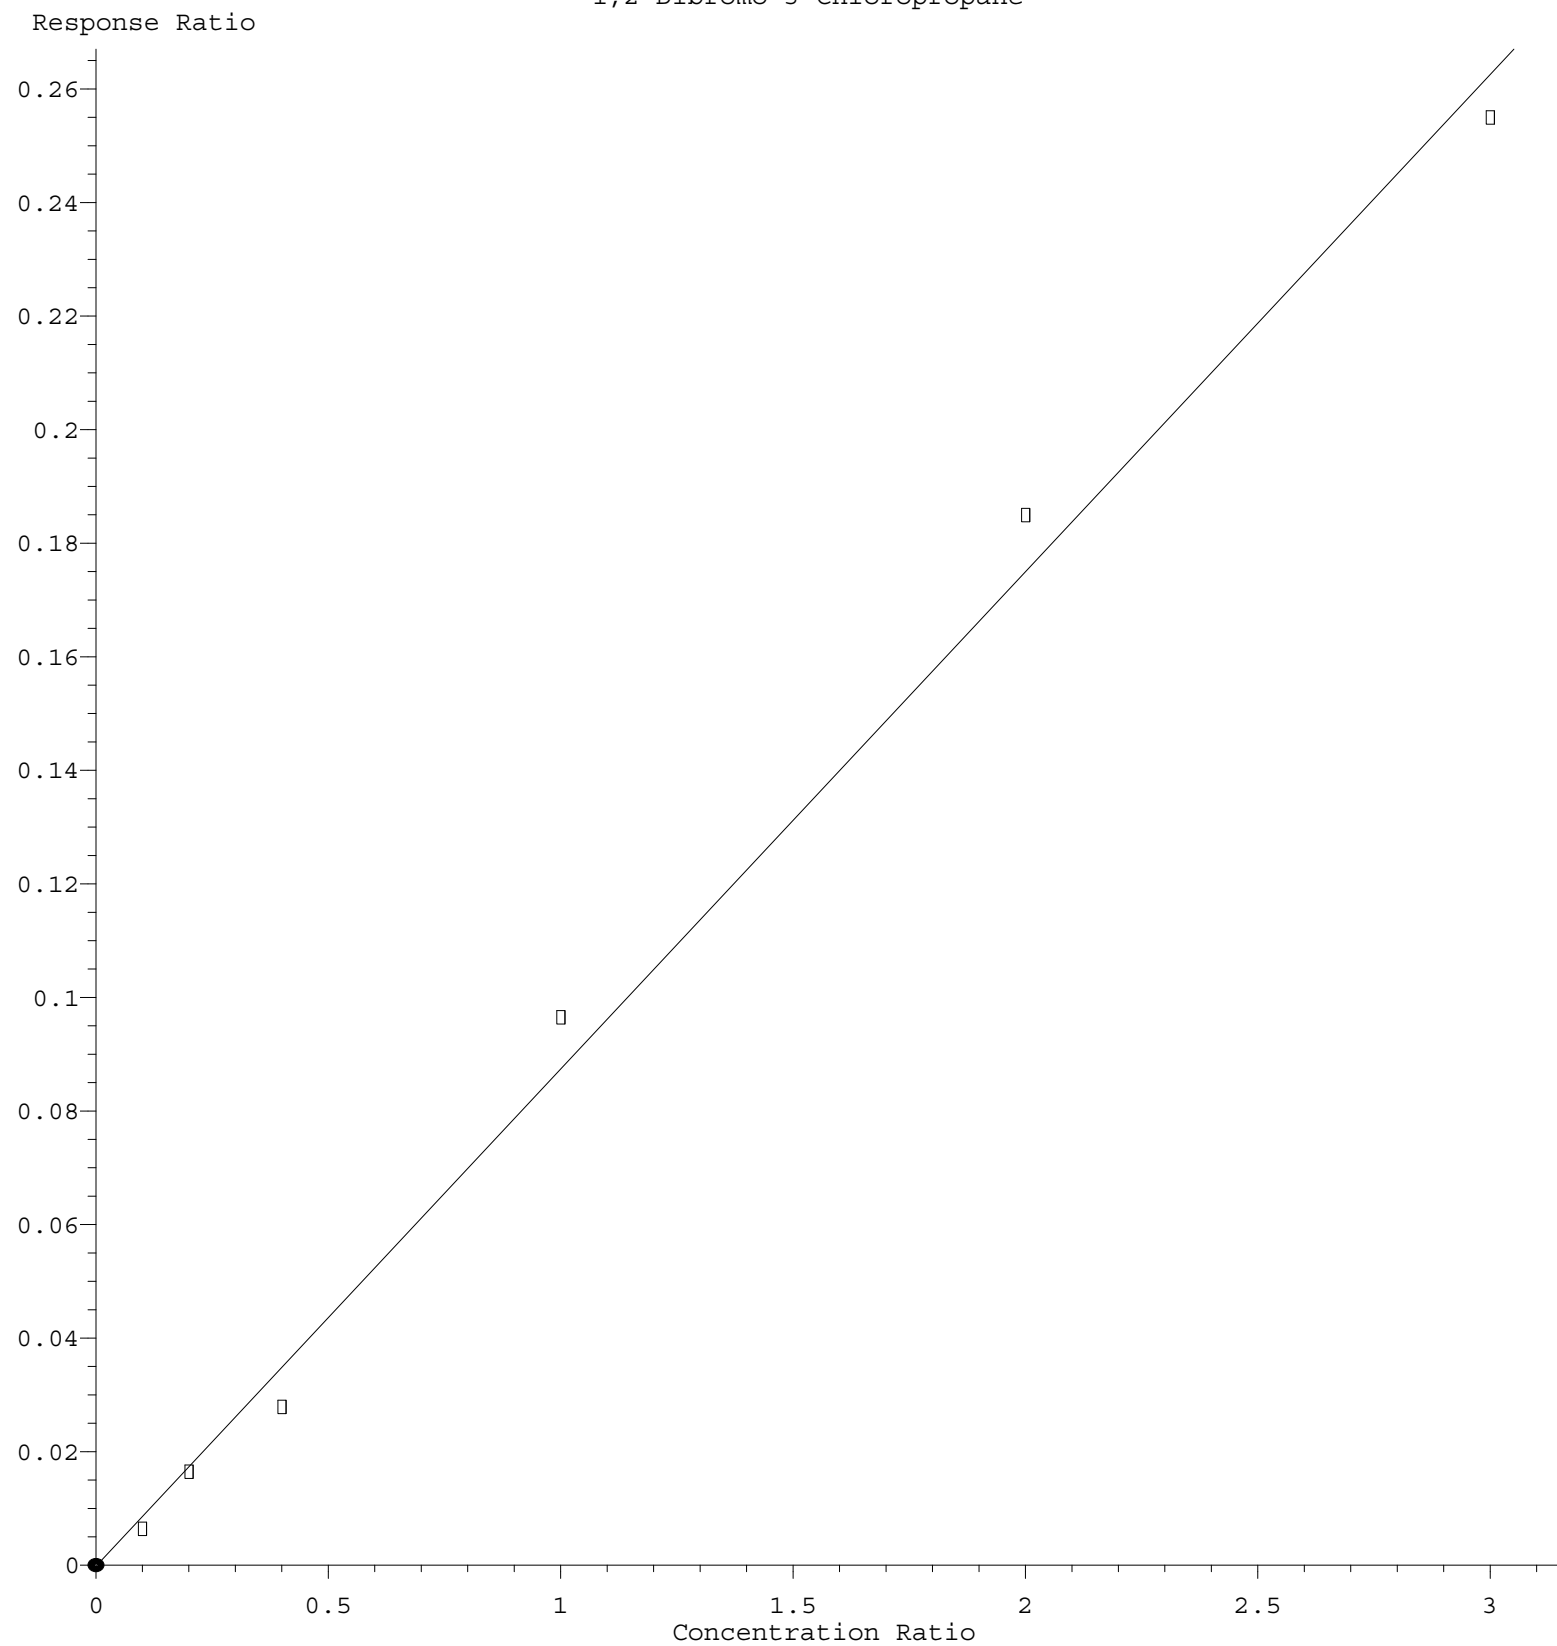

Response = $8.779 \times 10^{-2} \times \text{Amt} - 1.804 \times 10^{-4}$
 Coef of Det (r^2) = 0.994372 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
 Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

Naphthalene

Response Ratio

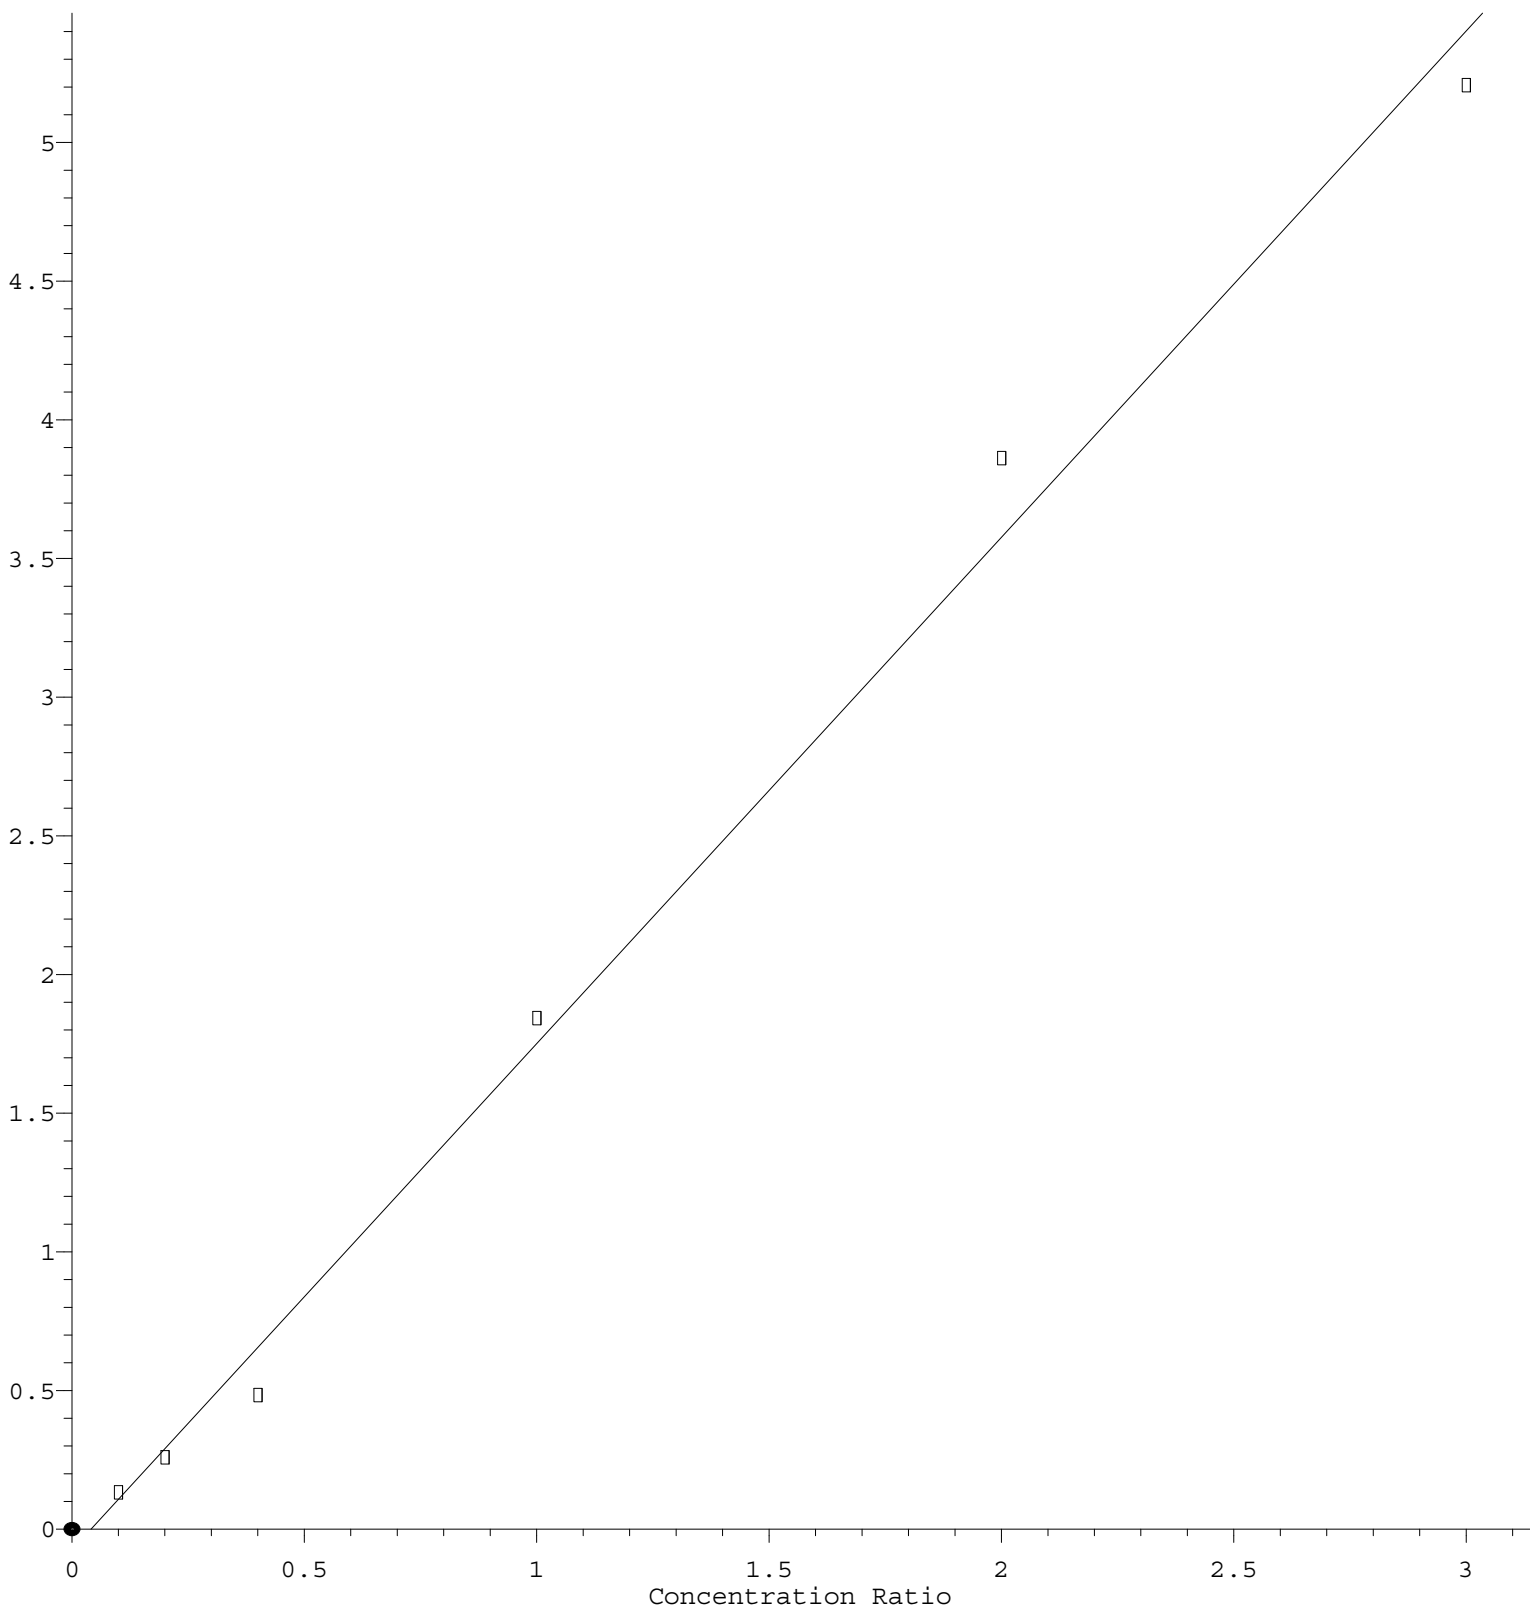

$$\text{Response} = 1.826\text{e}+000 * \text{Amt} - 7.410\text{e}-002$$


Coef of Det (r^2) = 0.992939 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M

Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

Methylene Chloride

Response Ratio

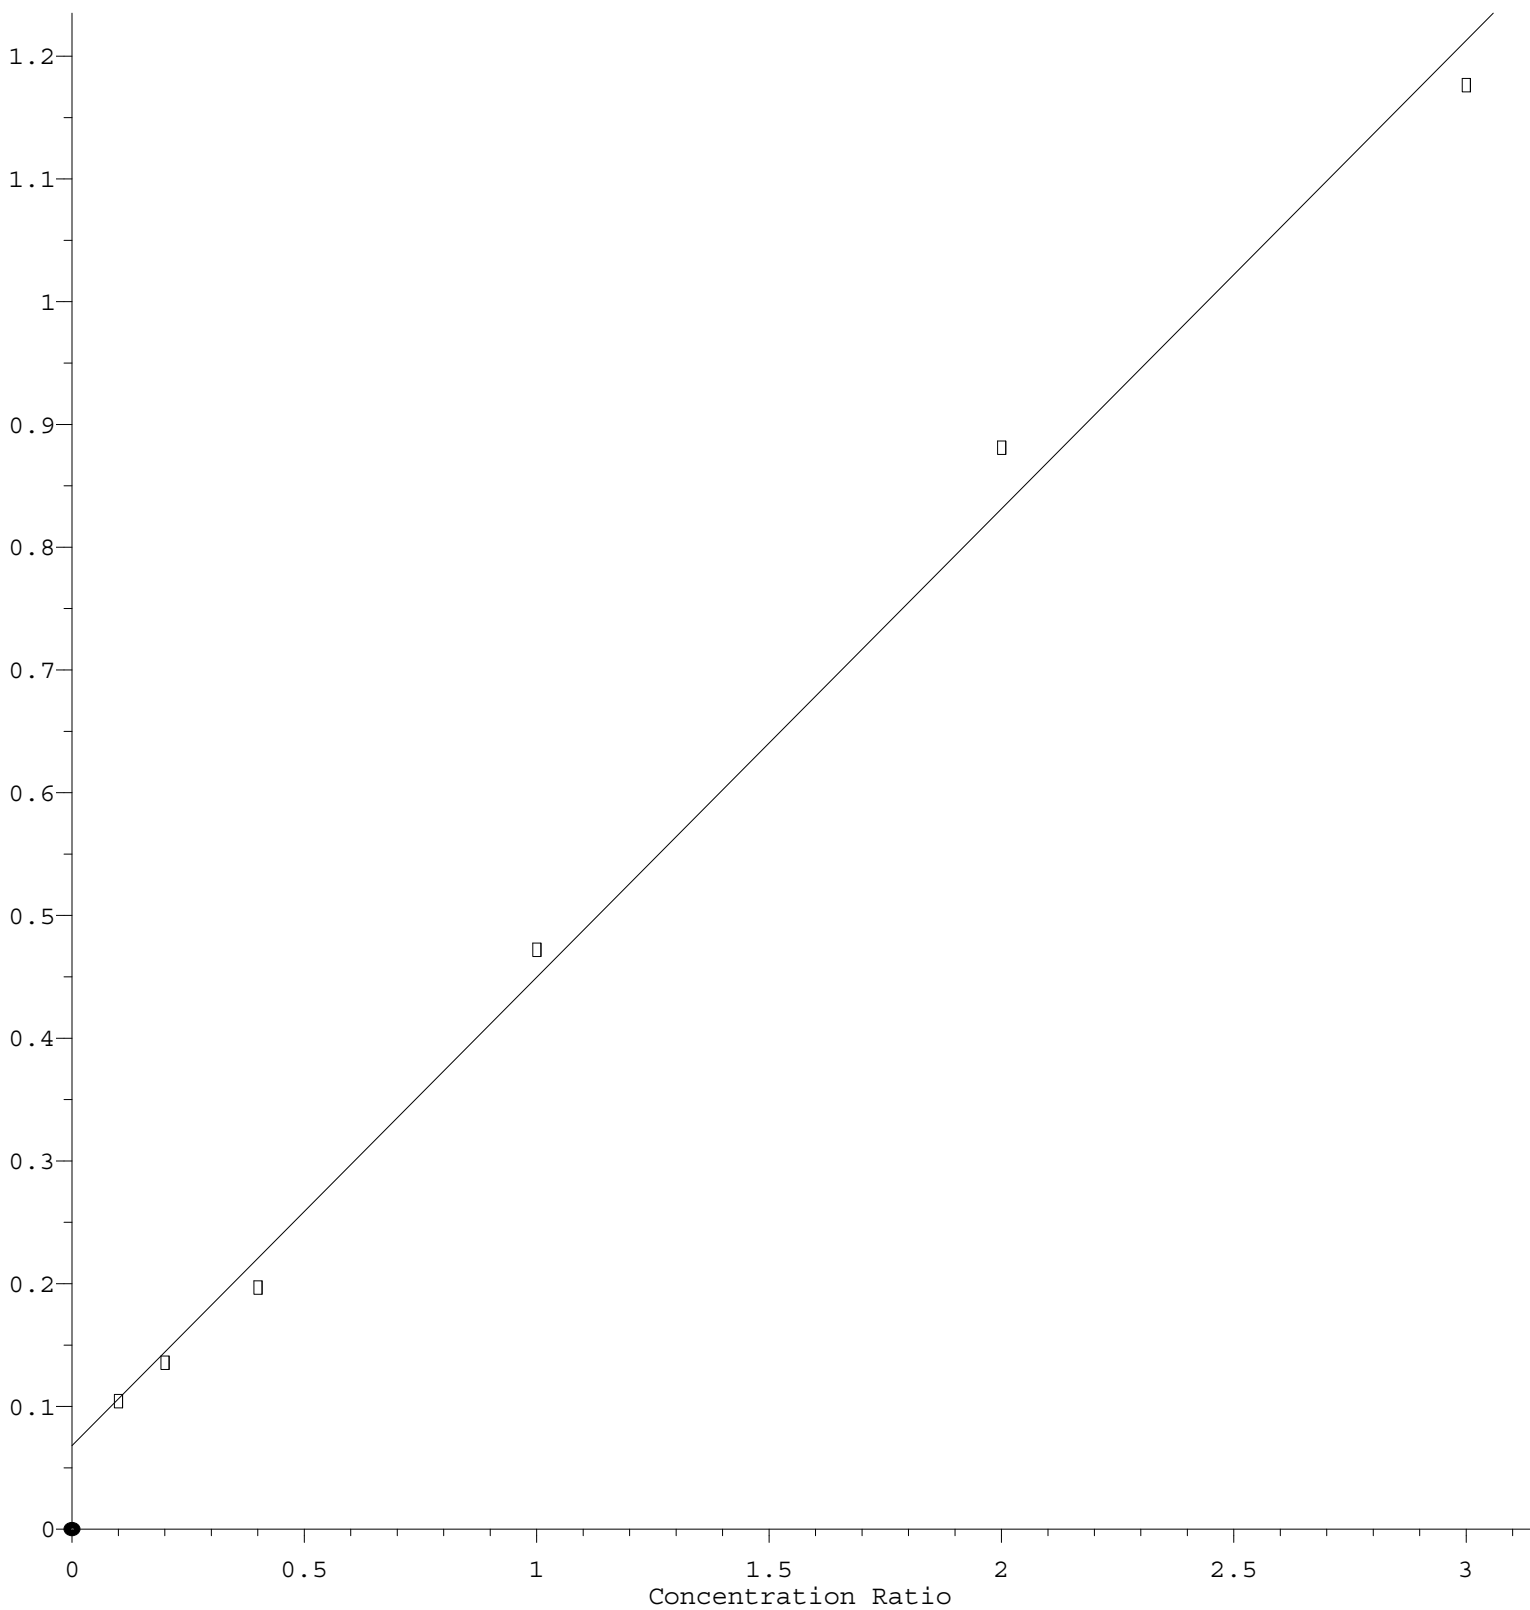

$$\text{Response} = 3.816\text{e-}001 * \text{Amt} + 6.826\text{e-}002$$


Coef of Det (r^2) = 0.994972 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M

Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

Cyclohexane

Response Ratio

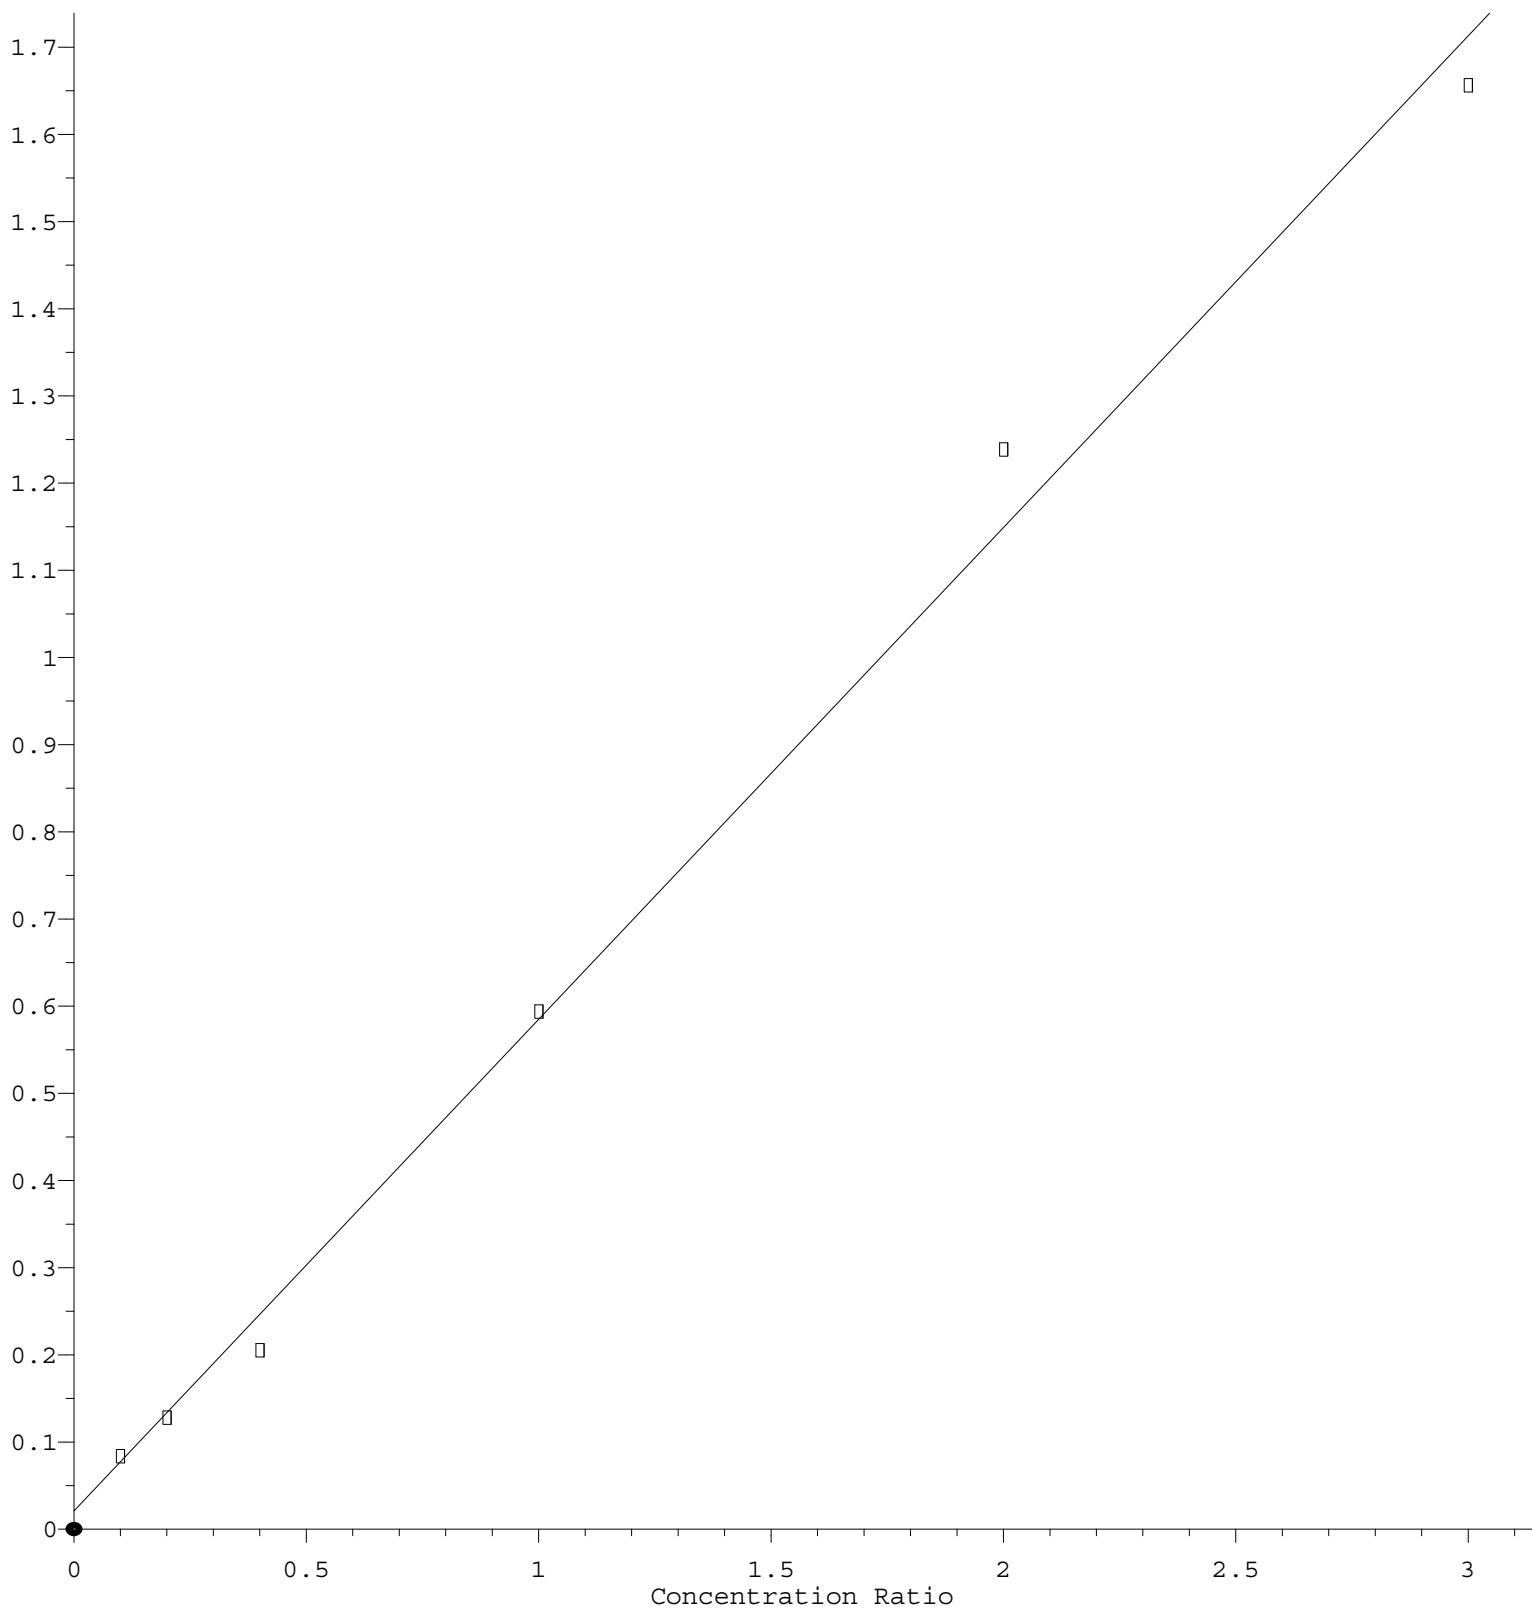

$$\text{Response} = 5.640\text{e-}001 * \text{Amt} + 2.103\text{e-}002$$


Coef of Det (r^2) = 0.993925 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M

Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

1,2-Dichloroethane-d4

Response Ratio

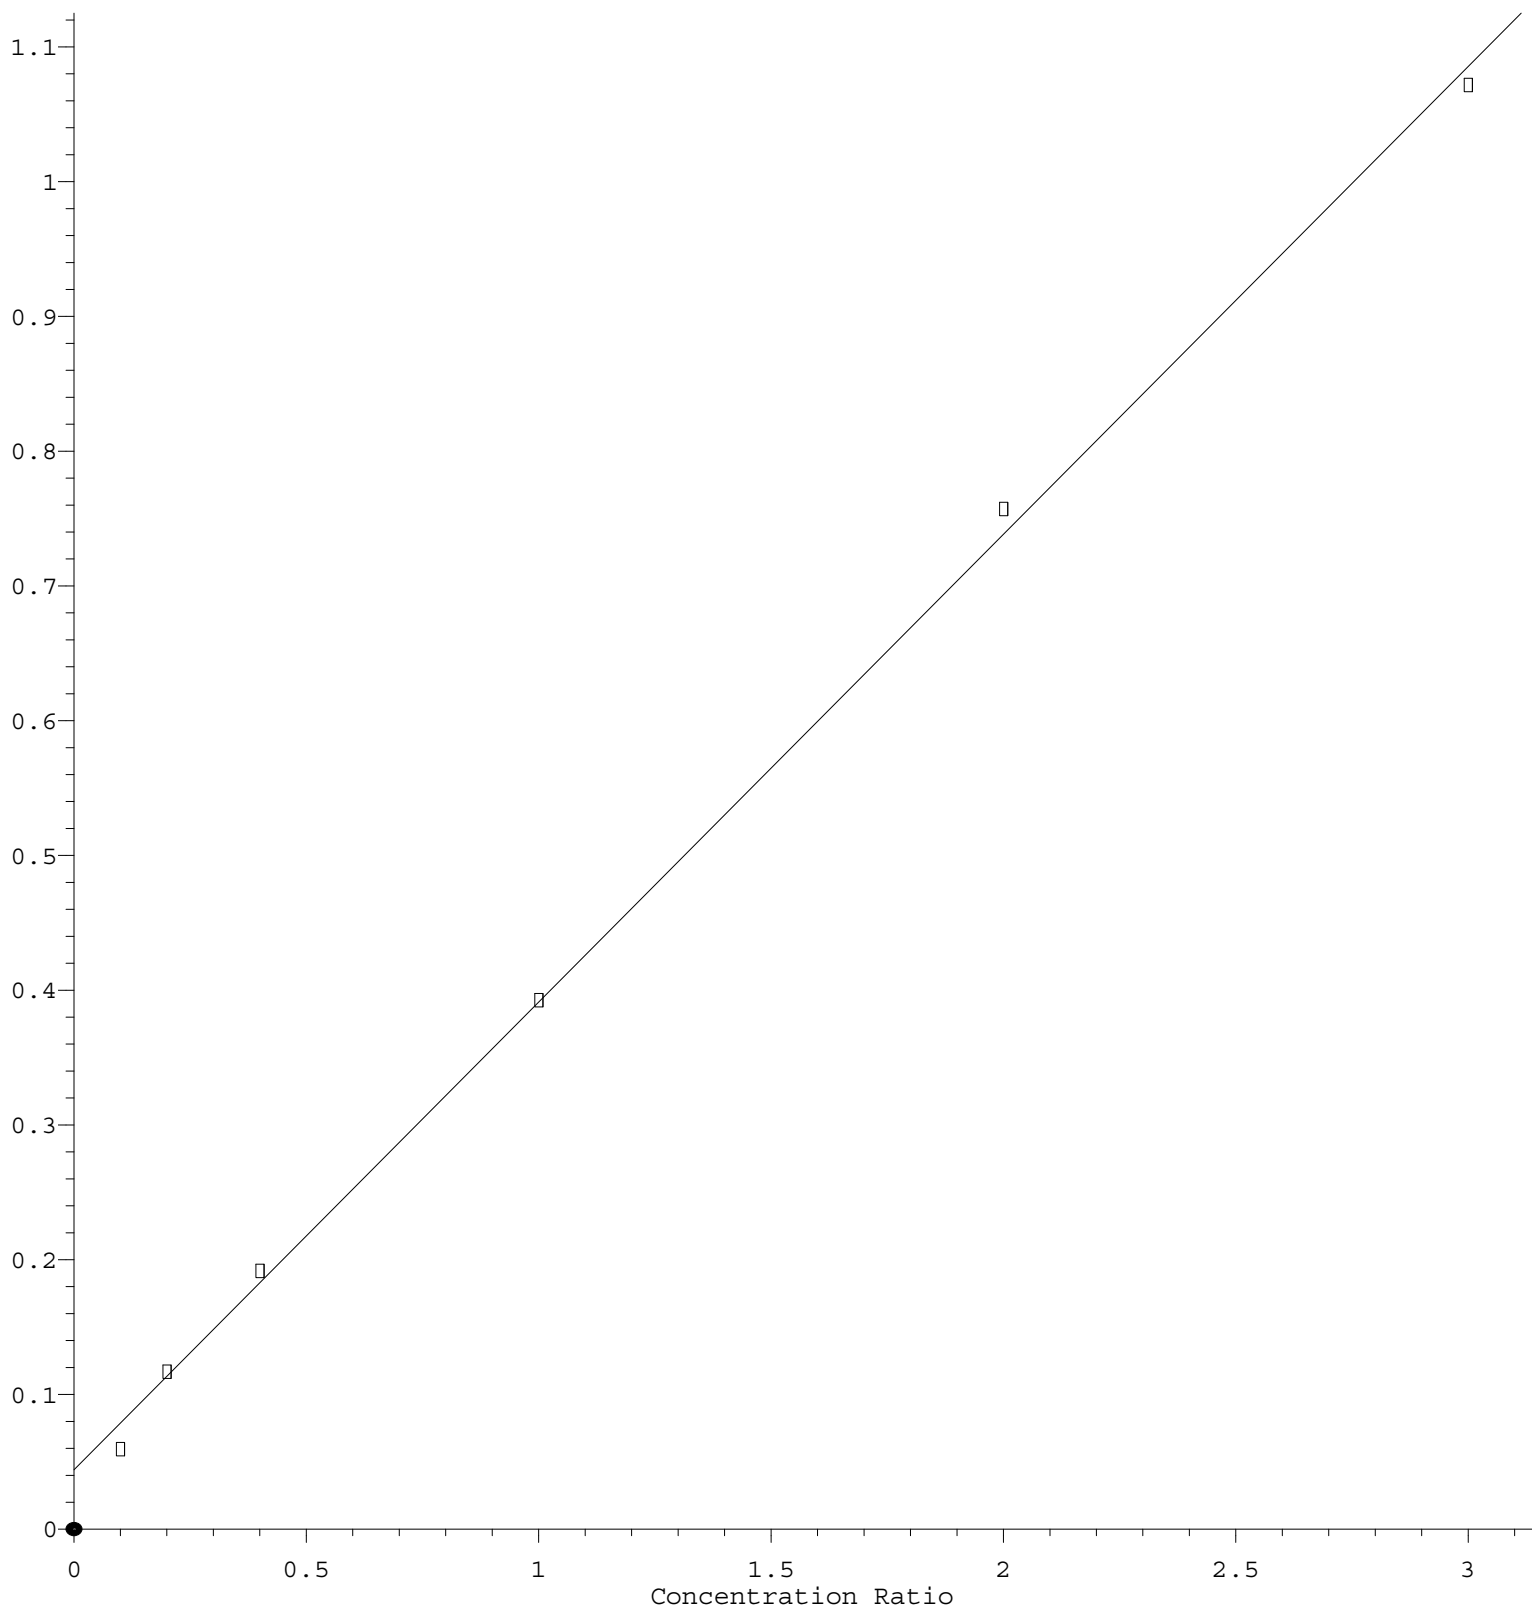


$$\text{Response} = 3.473\text{e-}001 * \text{Amt} + 4.376\text{e-}002$$

Coef of Det (r^2) = 0.998763 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M


Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

Methacrylonitrile

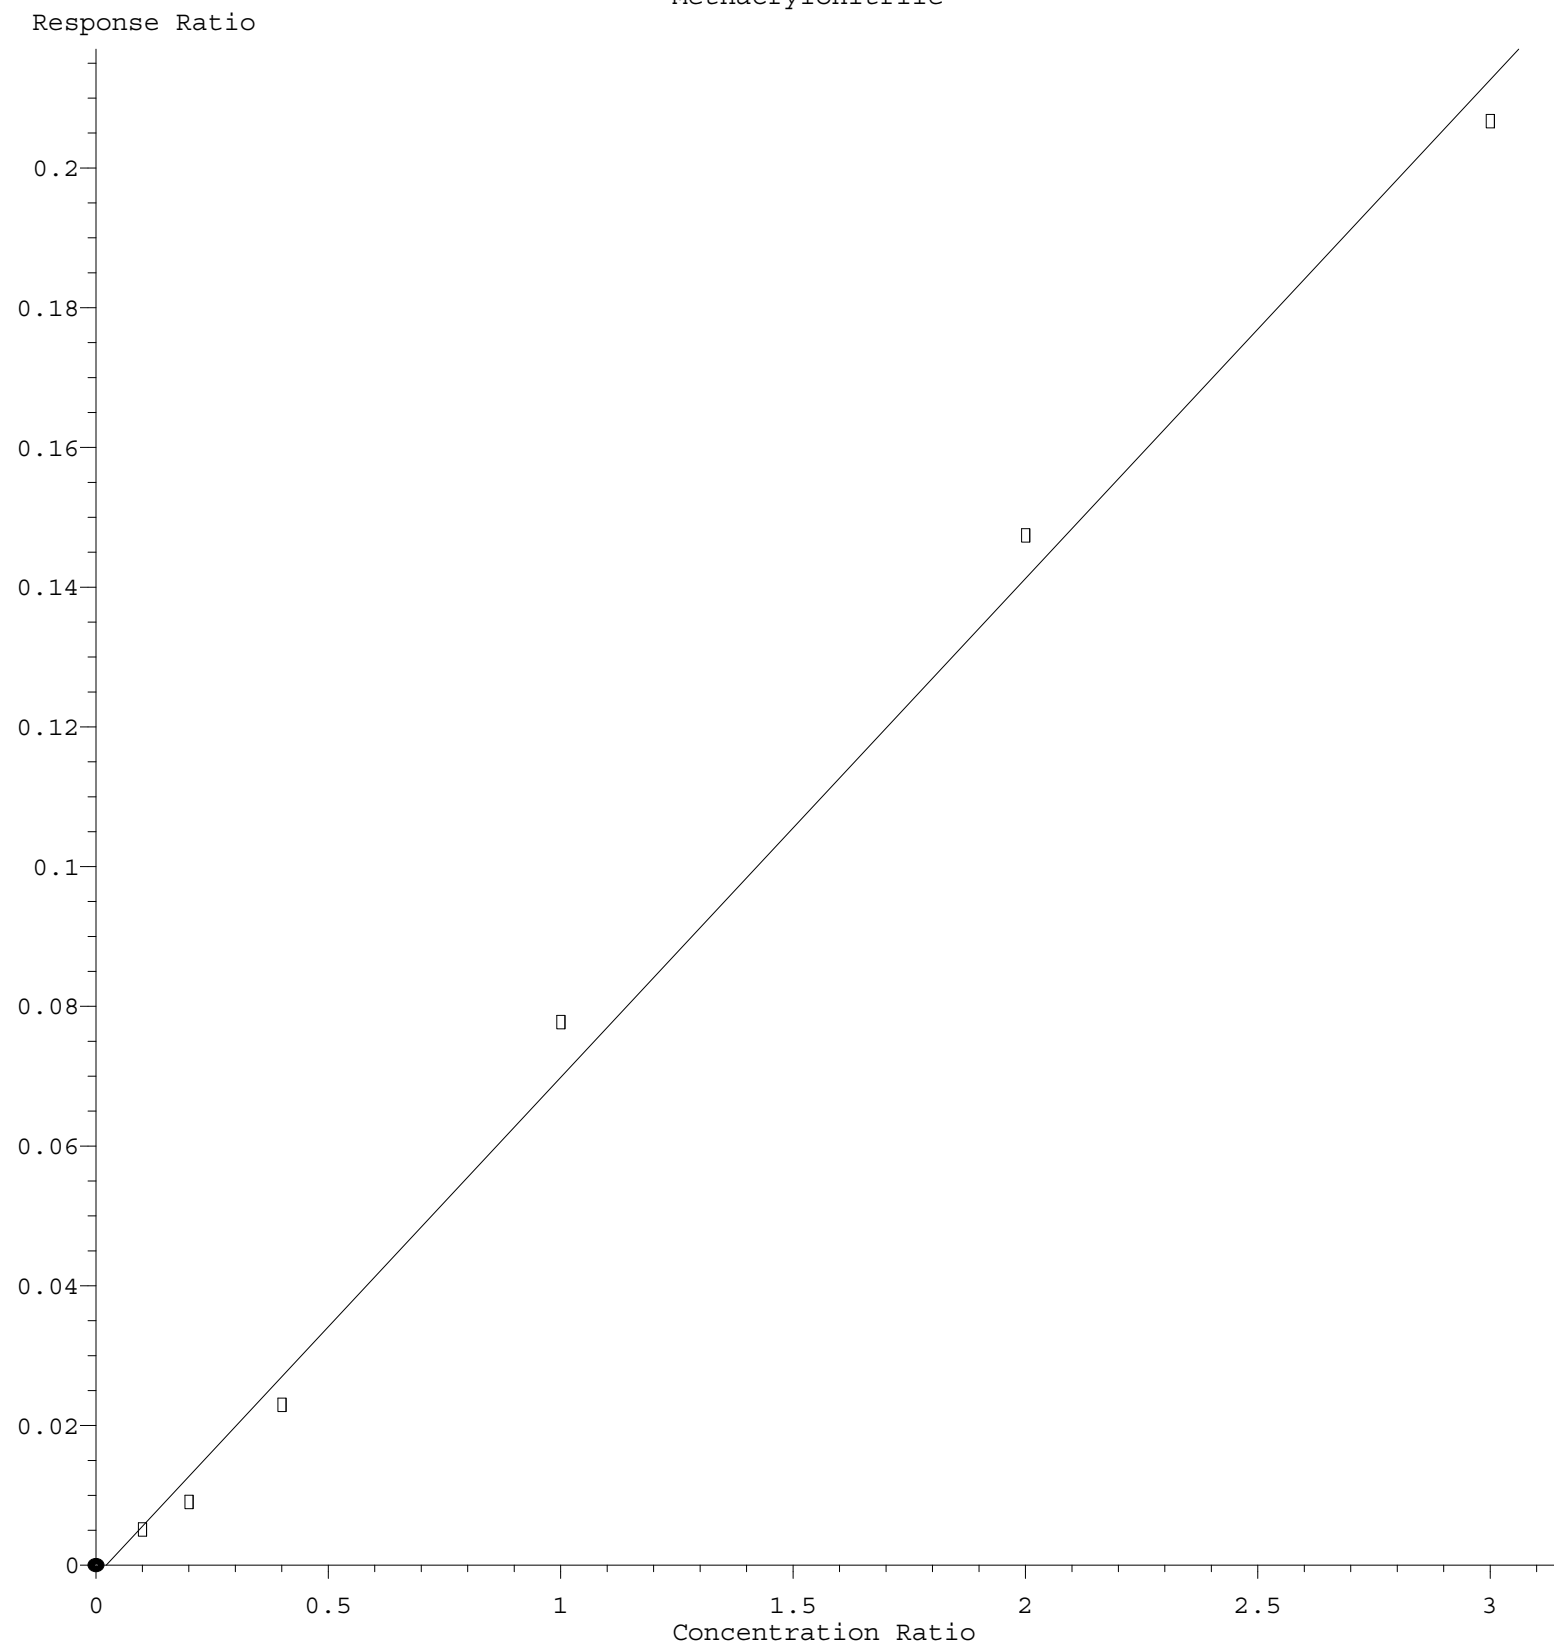

Response = $7.141\text{e-}002 * \text{Amt} - 1.589\text{e-}003$
Coef of Det (r^2) = 0.995196 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
Calibration Table Last Updated: Tue Nov 02 04:55:07 2021


1,4-Dioxane

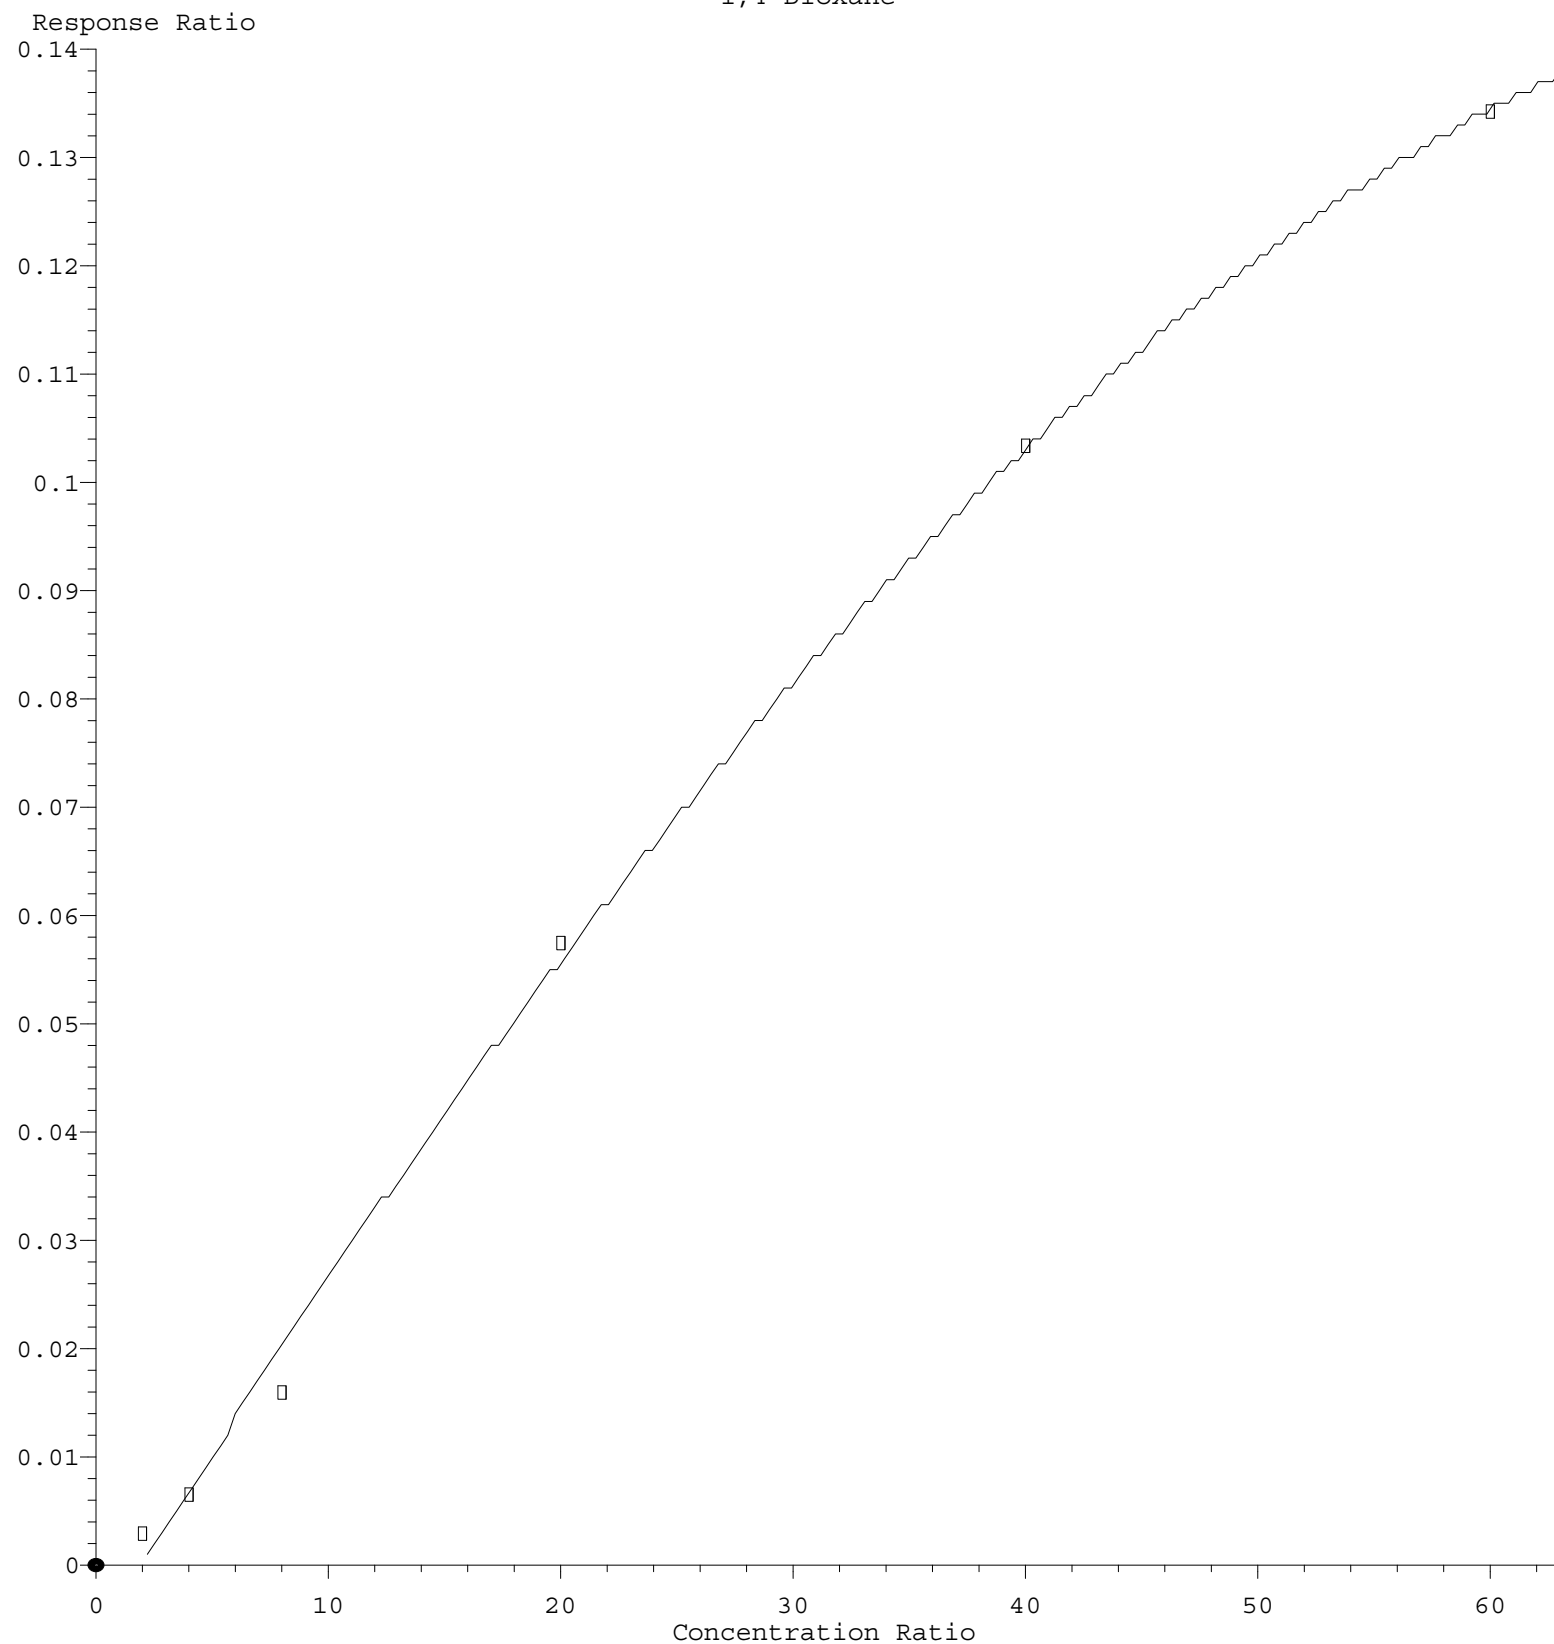

$R = -1.968e-005 A^2 + 3.538e-003 A - 6.972e-003$
Coef of Det (r^2) = 0.998160 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
Calibration Table Last Updated: Tue Nov 02 04:55:07 2021


4-Methyl-2-Pentanone

Response Ratio

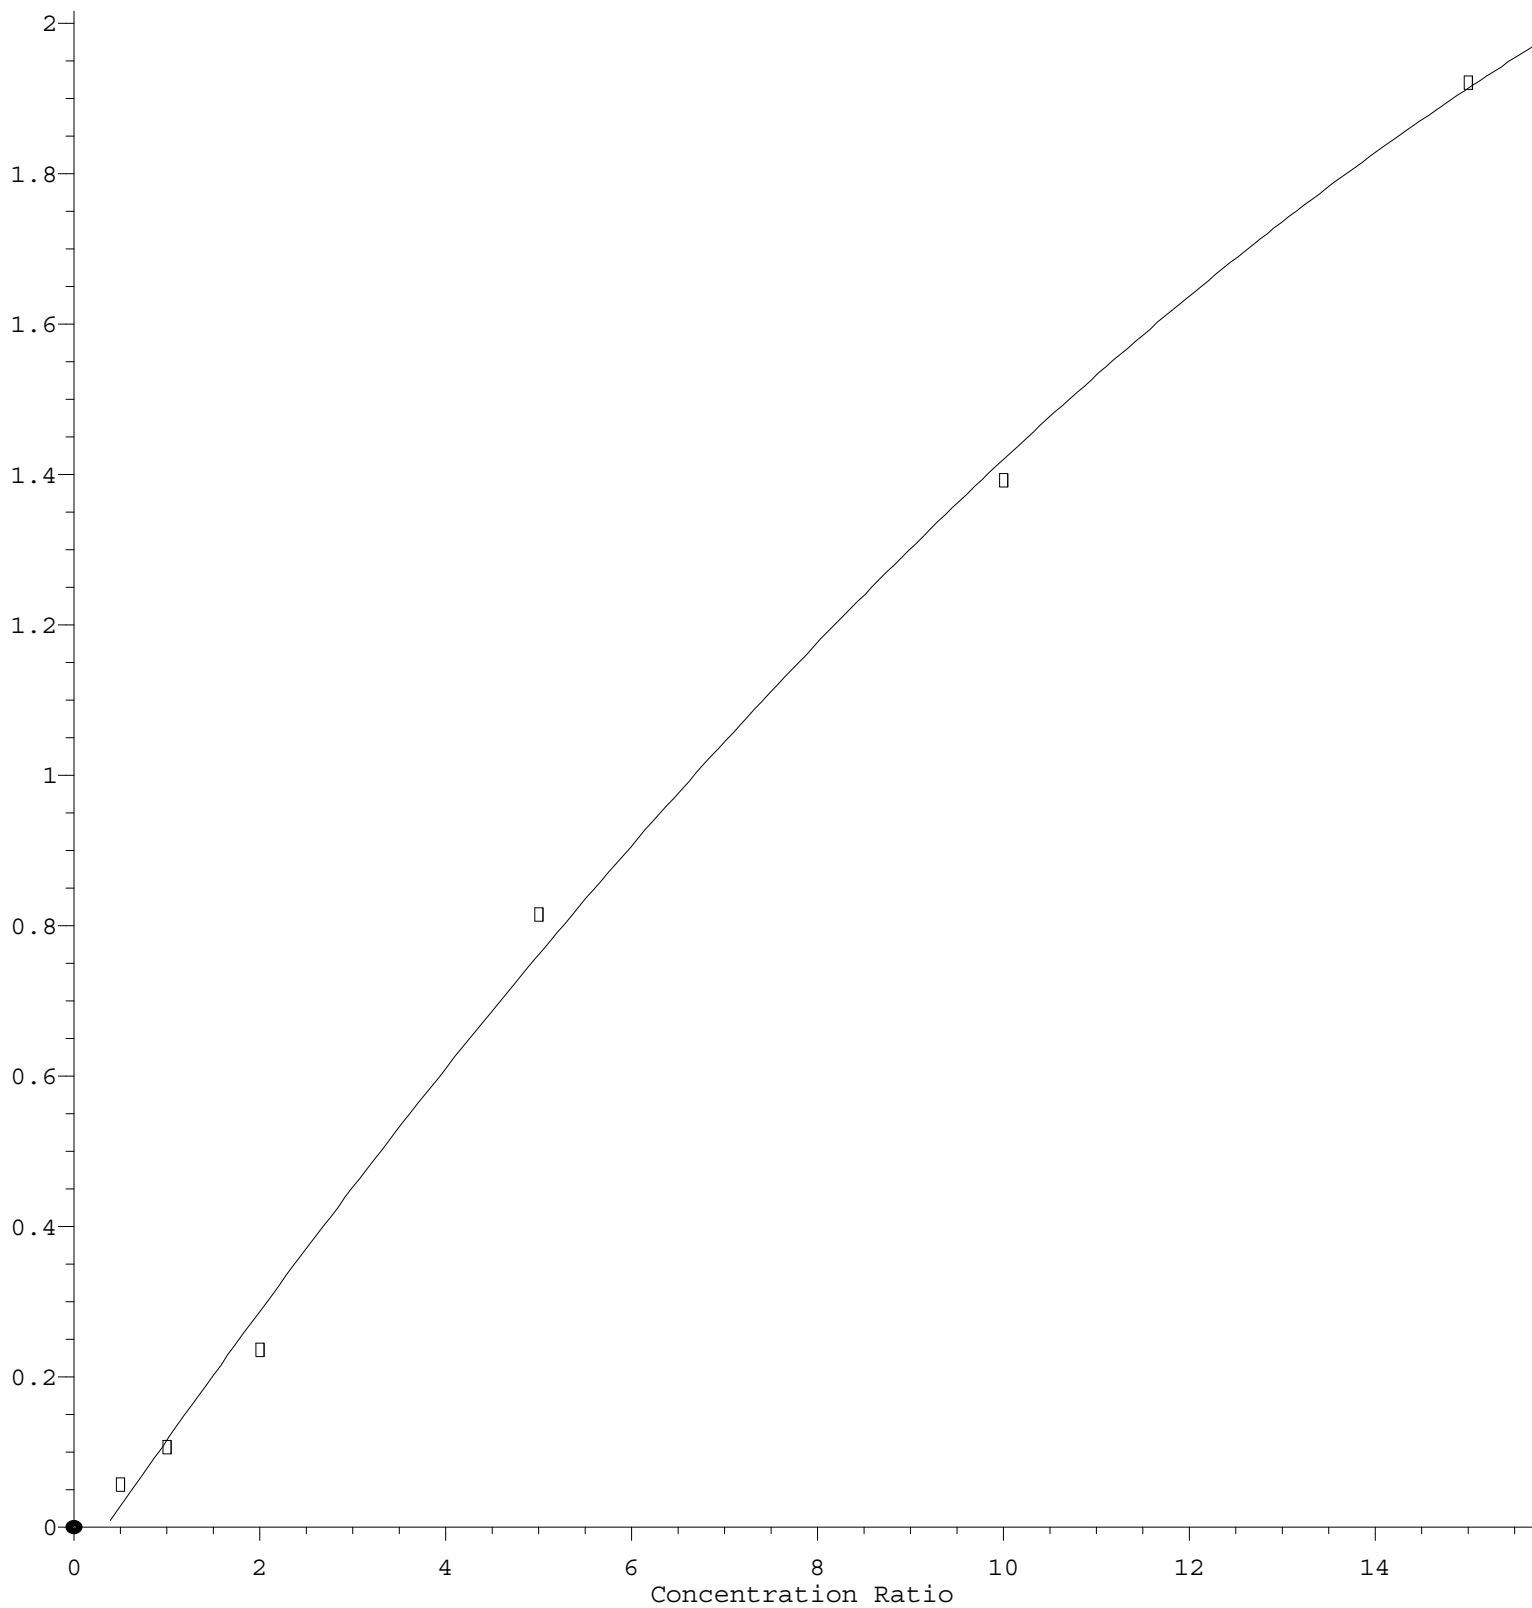

$R = -3.298e-003 A^2 + 1.812e-001 A - 6.179e-002$
Coef of Det (r^2) = 0.997550 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
Calibration Table Last Updated: Tue Nov 02 04:55:07 2021


Ethyl methacrylate

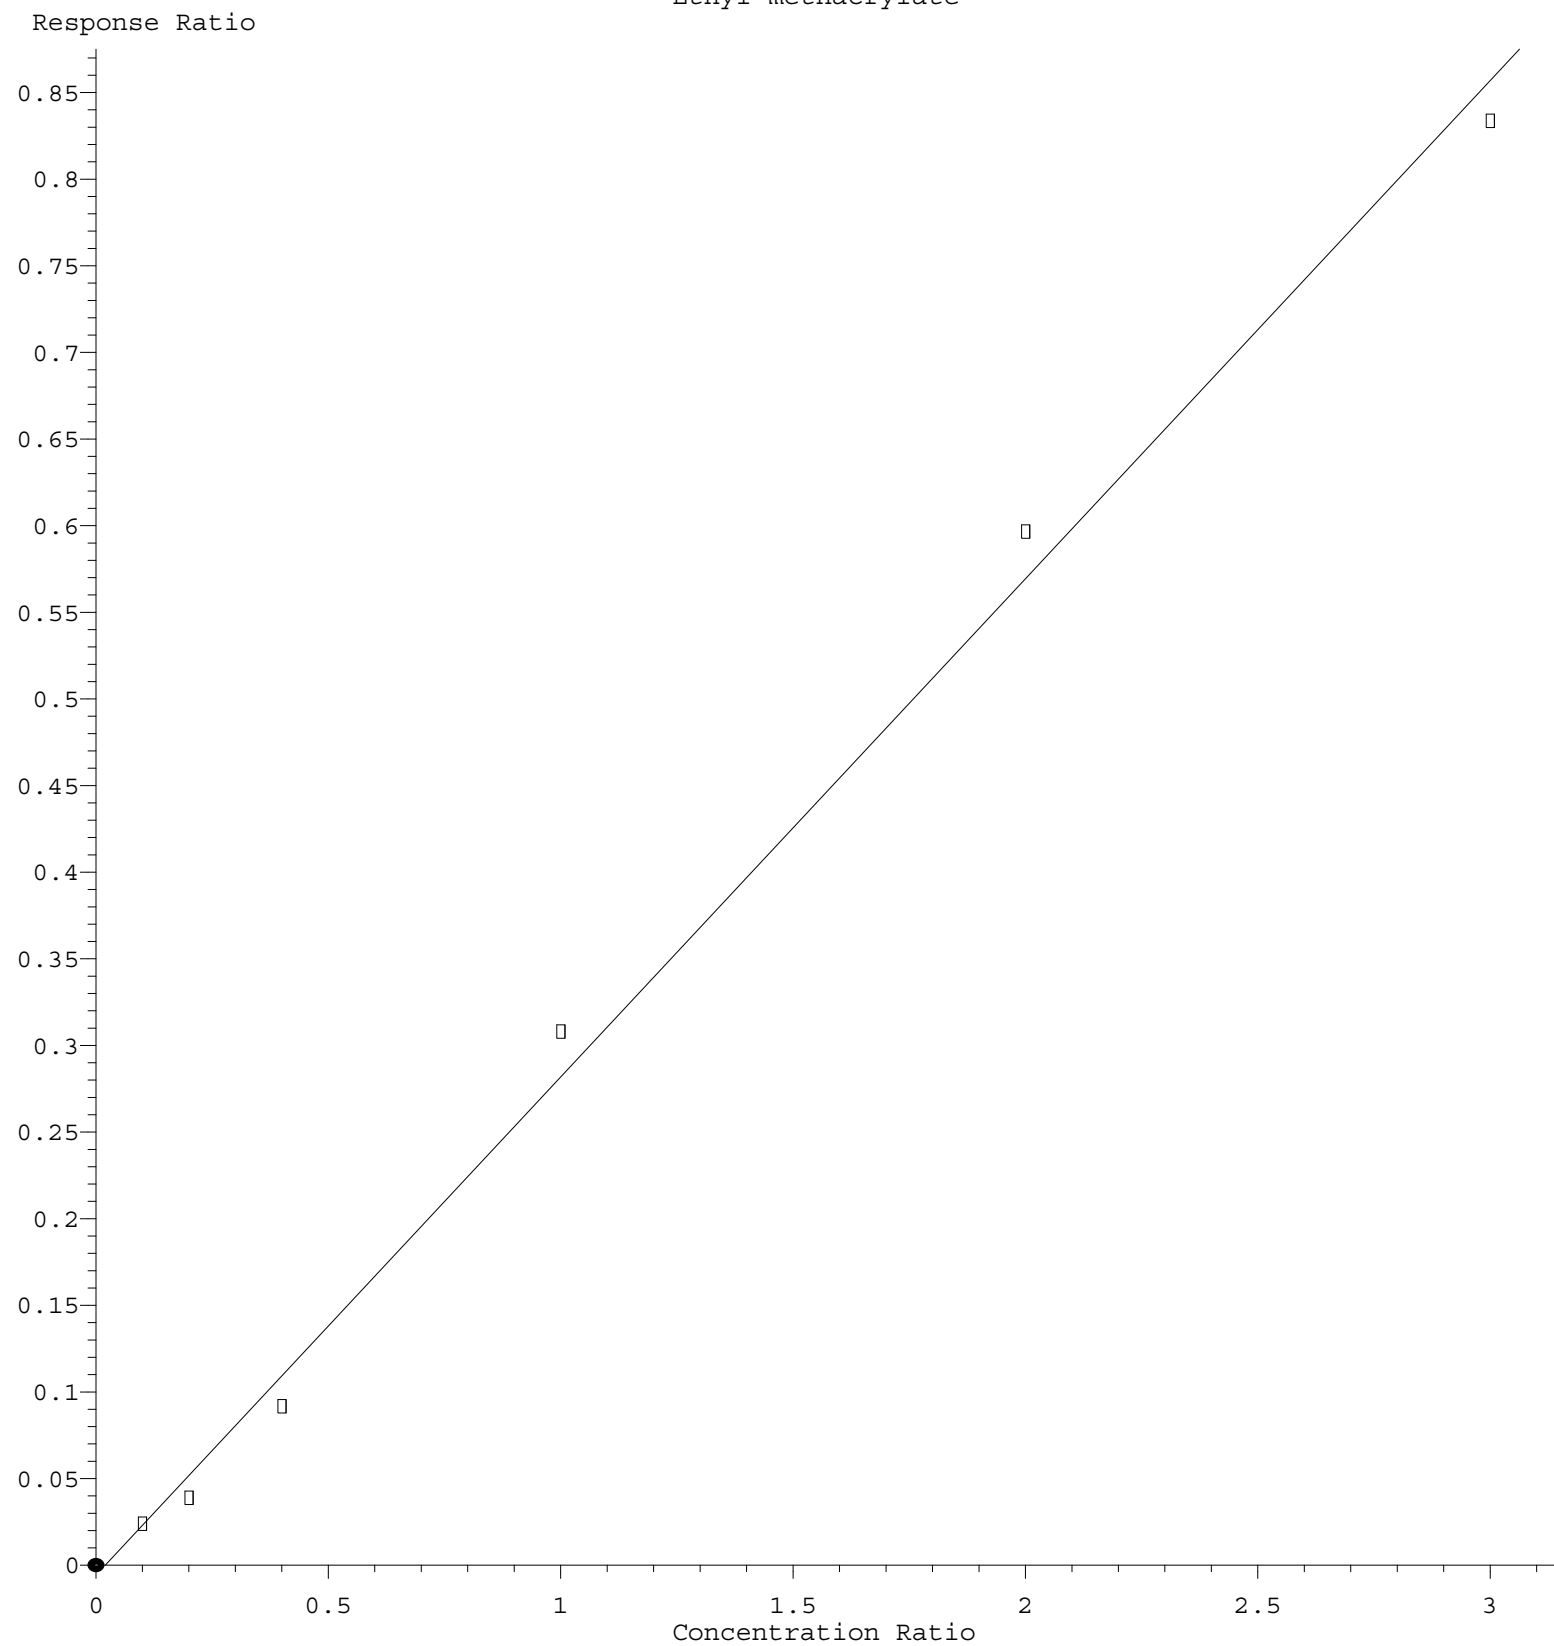

Response = $2.876 \times 10^{-1} \times \text{Amt} - 5.750 \times 10^{-3}$
Coef of Det (r^2) = 0.995631 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
Calibration Table Last Updated: Tue Nov 02 04:55:07 2021

2-Hexanone

Response Ratio

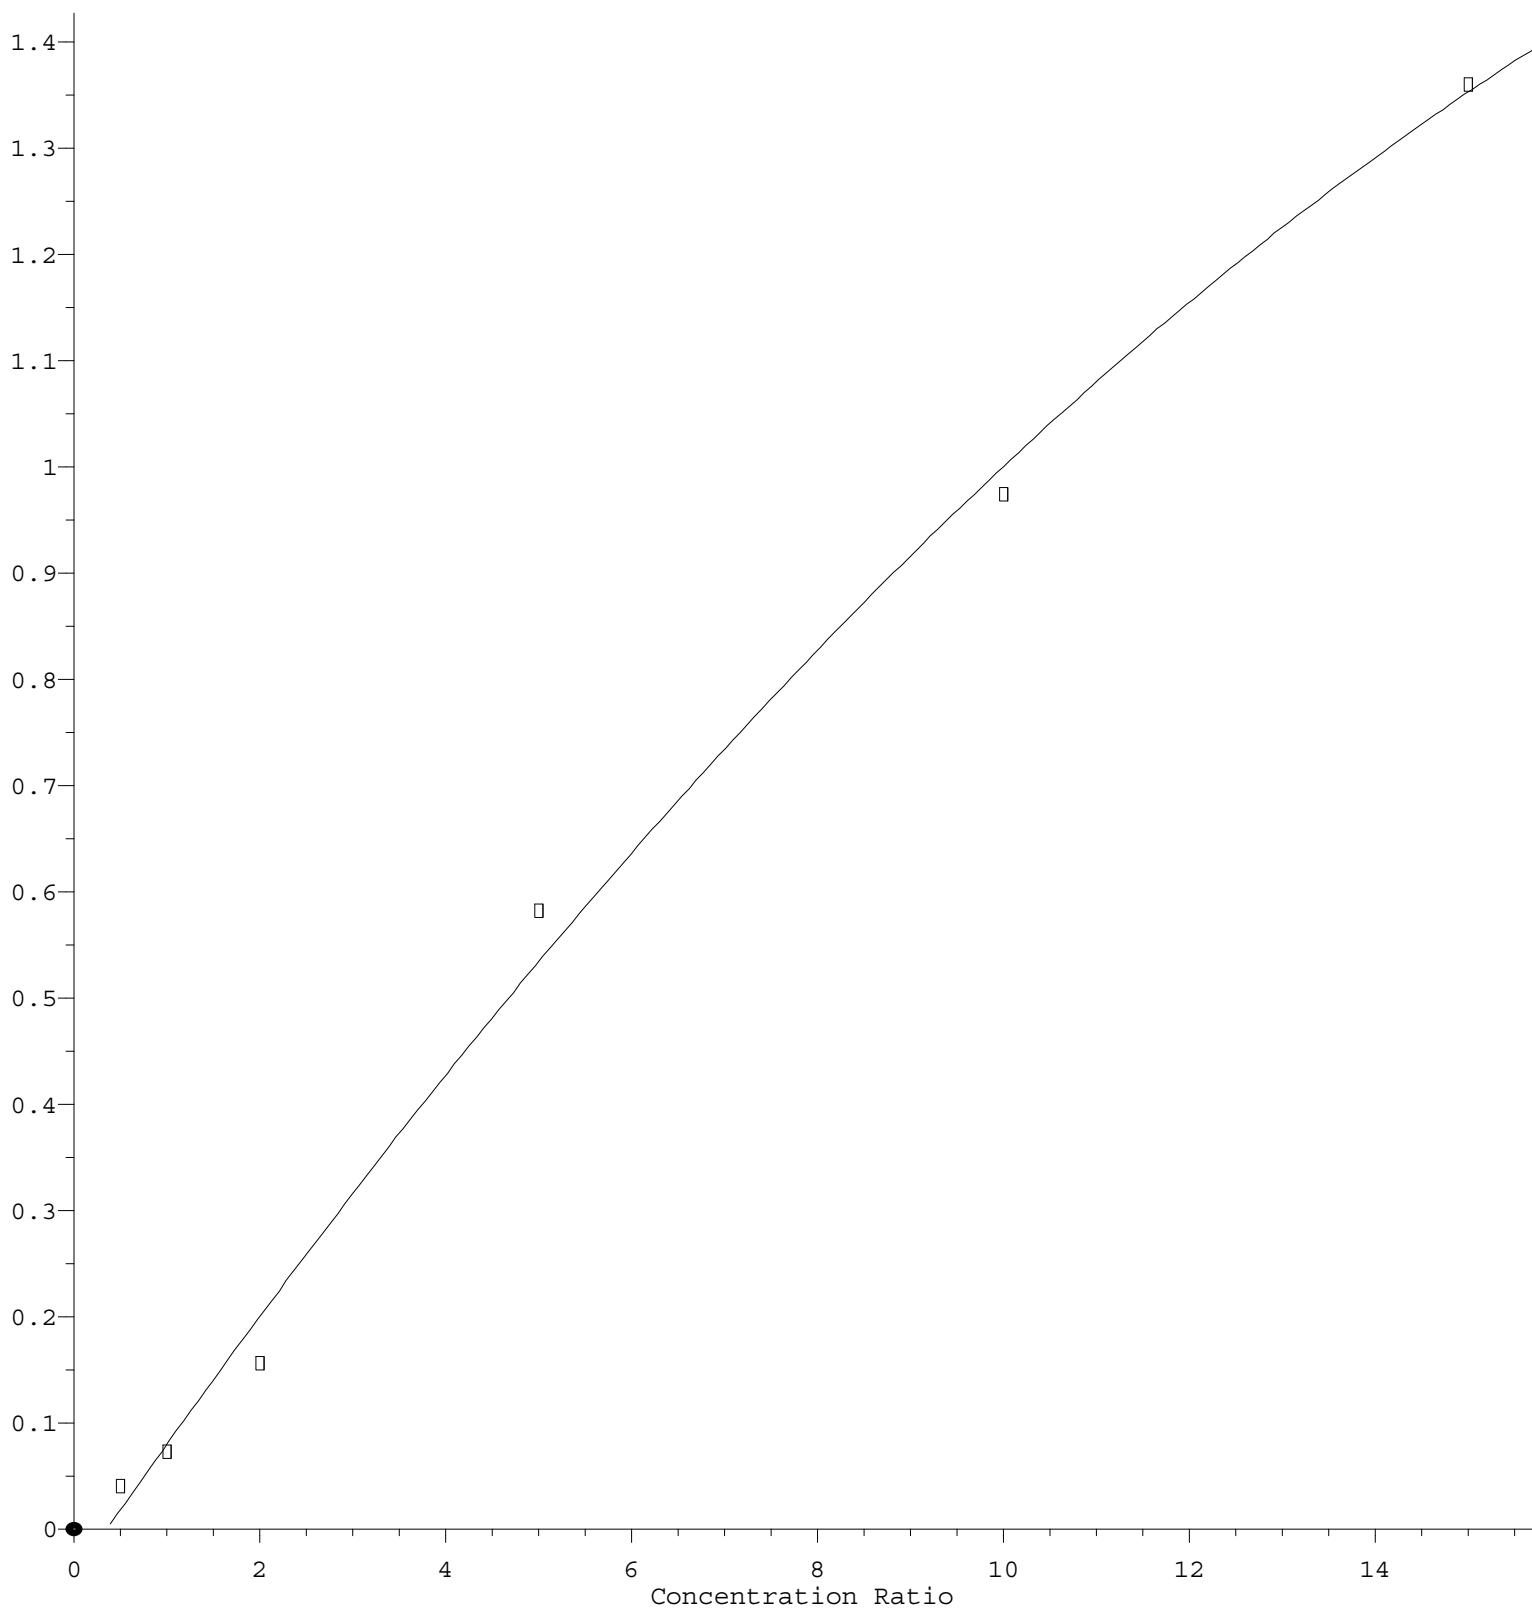

$R = -2.268e-003 A^2 + 1.272e-001 A - 4.497e-002$
Coef of Det (r^2) = 0.996263 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W110121S.M
Calibration Table Last Updated: Tue Nov 02 04:55:07 2021