
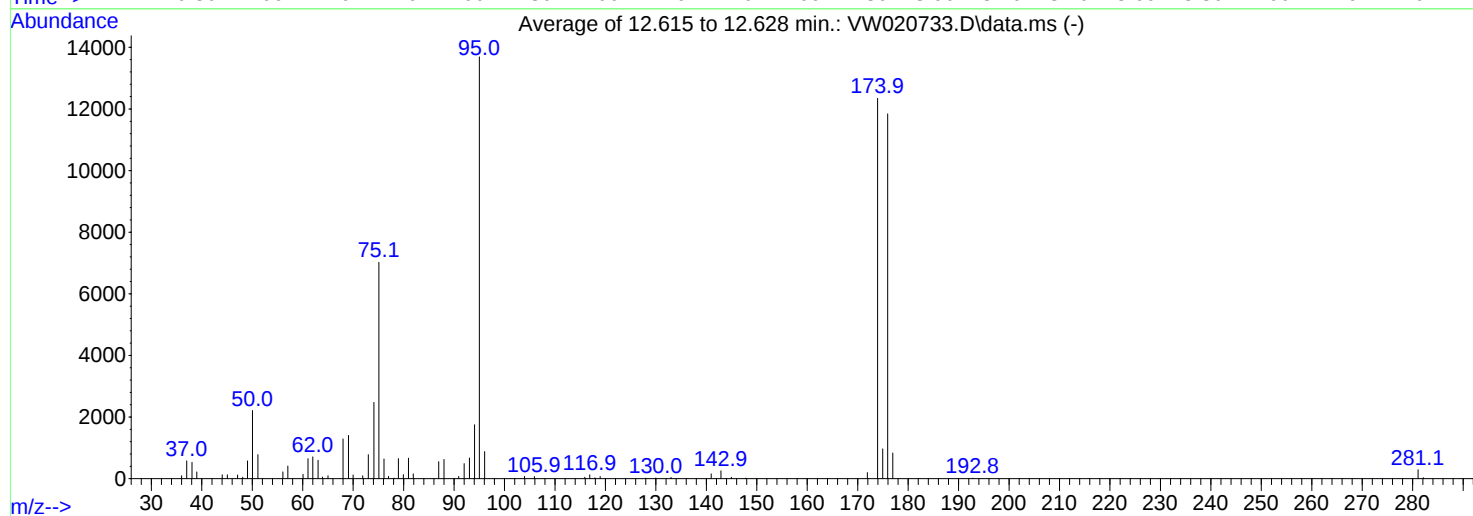


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110121\
 Data File : VW020733.D
 Acq On : 01 Nov 2021 13:38
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W110121S.M
 Title : SW846 8260
 Last Update : Tue Nov 02 04:55:07 2021

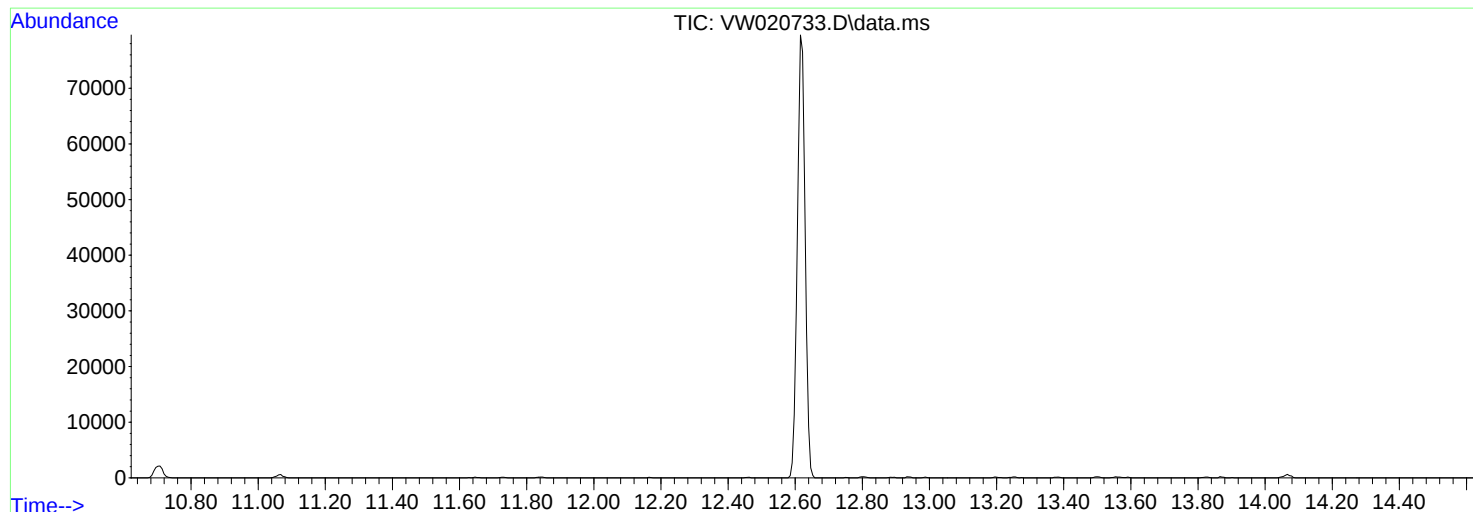

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	2215	PASS
75	95	30	60	51.3	7024	PASS
95	95	100	100	100.0	13691	PASS
96	95	5	9	6.4	877	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.2	12347	PASS
175	174	5	9	7.8	967	PASS
176	174	95	101	95.9	11844	PASS
177	176	5	9	7.0	833	PASS