


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110220\
 Data File : VW017036.D
 Acq On : 02 Nov 2020 08:53
 Operator : SY/VA
 Sample : BFB26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB26

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM102220S.M
 Title : VOC Analysis
 Last Update : Tue Nov 03 04:48:47 2020

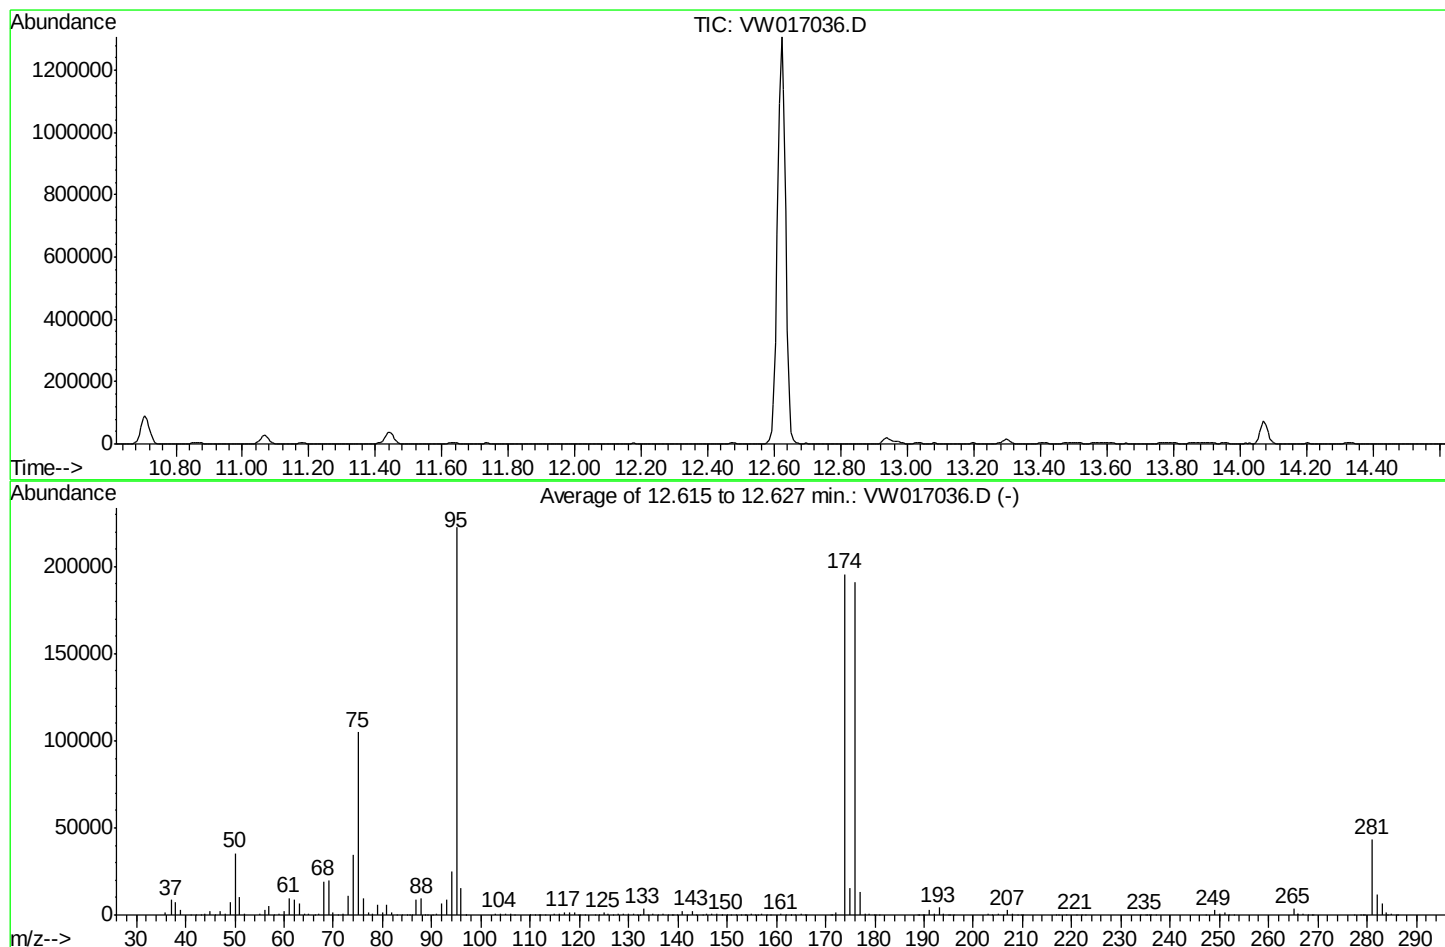

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	35376	PASS
75	95	30	80	47.2	105024	PASS
95	95	100	100	100.0	222464	PASS
96	95	5	9	6.9	15324	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.9	195648	PASS
175	174	5	9	7.8	15286	PASS
176	174	95	101	97.6	190912	PASS
177	176	5	9	7.1	13567	PASS

m/z	Abundance
35.90	1249.0
37.00	8091.0
38.00	7140.0
39.00	2804.0
40.00	206.0
40.90	52.0
43.00	231.0
44.00	1287.0
45.00	2111.0
46.00	184.0
47.00	2016.0
47.90	1048.0
49.00	7339.0
50.00	33232.0
51.00	9715.0
51.90	424.0
55.00	534.0
56.00	2376.0
57.00	4995.0
57.90	253.0
59.00	668.0
60.00	1904.0
61.00	9102.0
62.00	8215.0
63.00	6239.0
64.00	1049.0
65.10	637.0
66.10	128.0
67.00	593.0
68.00	17592.0
69.00	19200.0
70.00	1421.0
71.00	193.0
72.10	1006.0
73.00	11943.0
74.00	32088.0
75.00	95888.0
76.00	8612.0
77.00	1205.0
77.90	966.0
78.90	5115.0
80.00	1574.0
80.90	5866.0
81.90	1143.0
83.00	205.0
83.90	105.0
85.00	158.0
86.00	254.0
86.90	8555.0
88.00	8747.0
88.70	358.0
89.10	333.0
90.00	54.0
91.00	766.0
92.00	5731.0
93.00	8482.0
94.00	21960.0
95.00	199552.0
96.00	14697.0
96.90	467.0
102.90	1070.0
103.90	1094.0
105.00	624.0
105.90	956.0
106.90	207.0
109.90	506.0
111.00	502.0
111.90	376.0
113.00	157.0
114.80	614.0
115.90	660.0
116.90	1487.0
118.00	1365.0
118.90	1707.0
119.80	188.0
121.10	273.0
124.00	184.0
124.90	1666.0
125.80	600.0
126.90	90.0
127.90	770.0
128.90	369.0
129.90	767.0
130.90	396.0
133.00	5648.0
134.80	792.0
135.80	101.0
136.90	362.0
139.10	61.0
139.90	117.0
140.80	1779.0
141.90	301.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

143.00	1837.0
143.90	183.0
145.00	396.0
145.90	278.0
146.90	762.0
148.00	496.0
148.80	405.0
150.00	273.0
150.80	89.0
151.80	100.0
152.90	163.0
153.70	84.0
154.90	425.0
155.70	168.0
156.90	368.0
158.10	92.0
158.80	321.0
160.90	495.0
162.00	153.0
162.90	808.0
163.70	115.0
165.00	711.0
165.90	125.0
171.00	107.0
172.00	1229.0
173.90	164160.0
174.90	13186.0
175.90	156544.0
177.00	11860.0
177.90	736.0
179.00	1116.0
180.10	234.0
180.80	150.0
189.00	477.0
189.80	244.0
191.00	4735.0
192.10	1236.0
193.00	5566.0
194.00	968.0
194.90	447.0
196.00	92.0
202.90	651.0
203.90	82.0
205.00	1054.0
206.00	345.0
207.00	4059.0
208.10	849.0
209.00	413.0
209.90	71.0
217.30	74.0
218.90	152.0
221.00	243.0
222.10	77.0
222.70	52.0
234.00	59.0
234.90	584.0
236.00	207.0
236.90	177.0
247.10	184.0
249.00	4062.0
250.00	1024.0
251.00	1964.0
252.00	371.0
253.10	255.0
265.10	4783.0
265.90	1251.0
267.00	1084.0
268.00	261.0
269.00	149.0
277.30	102.0
279.10	418.0
281.00	55416.0
282.00	15951.0
283.10	9672.0
284.00	2070.0
285.00	671.0
285.90	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
36.00	1748.0
37.00	9404.0
38.00	8500.0
39.00	2967.0
39.90	204.0
41.00	91.0
42.10	66.0
42.90	153.0
44.00	1390.0
45.00	2064.0
45.90	246.0
46.90	2649.0
48.00	1163.0
49.00	8824.0
50.00	39120.0
51.00	12268.0
52.00	408.0
55.00	556.0
56.00	3564.0
57.00	5792.0
58.00	201.0
58.90	363.0
60.00	1906.0
61.00	10674.0
62.00	10175.0
63.00	7226.0
64.10	837.0
65.00	707.0
66.20	63.0
67.00	475.0
68.00	22056.0
69.00	22440.0
70.00	1697.0
71.10	103.0
71.90	1226.0
73.00	12710.0
74.00	38184.0
75.00	117256.0
76.00	10459.0
77.10	1320.0
78.00	1005.0
78.90	6531.0
79.90	1987.0
80.90	6925.0
81.90	1398.0
82.90	202.0
83.80	67.0
85.00	59.0
85.60	302.0
86.90	9987.0
87.90	10098.0
90.10	73.0
90.90	1148.0
92.00	6821.0
93.00	9840.0
94.00	28384.0
95.00	250176.0
96.00	16832.0
97.10	596.0
103.00	950.0
103.80	1113.0
104.90	460.0
105.90	956.0
106.80	199.0
110.10	334.0
111.10	324.0
111.70	223.0
112.00	215.0
113.00	167.0
114.90	479.0
115.90	948.0
116.90	1817.0
118.00	1283.0
118.90	1685.0
120.00	82.0
120.90	71.0
123.10	54.0
124.00	114.0
125.00	1053.0
125.90	364.0
126.90	135.0
128.00	933.0
128.90	557.0
129.90	840.0
131.00	448.0
131.80	155.0
133.00	3455.0
133.80	892.0
134.90	800.0
135.90	97.0
136.90	415.0
137.90	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

138.70	75.0
139.80	205.0
140.90	2143.0
142.90	2660.0
143.90	261.0
145.00	507.0
145.90	484.0
146.90	574.0
147.80	701.0
149.00	395.0
150.00	297.0
150.90	110.0
151.90	165.0
152.80	267.0
153.90	188.0
154.90	587.0
156.10	237.0
157.00	495.0
157.90	203.0
158.90	378.0
160.90	573.0
162.00	88.0
163.10	705.0
163.80	114.0
164.90	484.0
166.10	93.0
172.00	1047.0
174.00	218624.0
174.90	16832.0
175.90	206144.0
176.90	15522.0
177.90	770.0
178.90	882.0
179.80	71.0
188.90	381.0
190.00	218.0
191.00	3522.0
192.00	803.0
193.00	4460.0
194.00	803.0
194.90	650.0
203.00	460.0
203.90	107.0
205.00	853.0
206.10	272.0
207.00	2510.0
208.00	577.0
209.00	333.0
209.80	60.0
210.10	52.0
216.80	68.0
218.90	129.0
221.00	198.0
222.70	70.0
235.00	411.0
237.00	101.0
247.20	90.0
249.00	2954.0
249.90	734.0
251.00	1174.0
251.90	382.0
253.00	171.0
265.00	3428.0
266.10	1082.0
267.00	1015.0
267.90	156.0
268.70	58.0
278.60	81.0
279.40	184.0
281.10	49144.0
282.00	12701.0
283.00	6318.0
284.00	1656.0
285.00	550.0
286.10	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
36.00	1430.0
37.00	8219.0
38.00	6837.0
39.00	2776.0
40.00	221.0
40.80	60.0
43.10	164.0
43.90	1072.0
45.00	1623.0
47.00	2021.0
47.90	1054.0
49.00	7028.0
50.00	33776.0
51.00	10015.0
52.00	368.0
54.90	541.0
56.00	2540.0
57.00	5037.0
58.00	270.0
58.90	181.0
60.00	1904.0
61.00	8994.0
62.00	8698.0
63.00	7030.0
64.00	758.0
64.90	409.0
67.10	708.0
68.00	18648.0
69.00	17784.0
70.00	1374.0
71.10	112.0
72.00	1114.0
73.00	9280.0
74.00	32768.0
75.00	101928.0
76.00	9206.0
77.00	1431.0
77.90	1078.0
78.90	6021.0
79.90	1670.0
80.90	5866.0
82.00	1320.0
83.10	253.0
86.00	209.0
86.90	8865.0
87.90	8995.0
91.00	898.0
92.00	6405.0
93.00	8940.0
94.00	24552.0
95.00	217664.0
96.00	14445.0
97.00	373.0
102.80	391.0
103.90	827.0
104.80	339.0
105.90	792.0
107.00	179.0
110.00	142.0
110.90	314.0
112.10	222.0
112.80	151.0
114.90	239.0
115.90	723.0
116.90	1555.0
117.90	952.0
118.90	1187.0
119.70	50.0
121.10	68.0
123.10	74.0
124.00	168.0
124.90	696.0
125.80	249.0
126.90	98.0
127.90	860.0
128.90	420.0
130.00	876.0
130.80	375.0
132.20	79.0
133.00	1570.0
134.80	484.0
135.80	67.0
136.90	558.0
138.70	55.0
140.80	2075.0
141.90	344.0
142.90	2401.0
143.80	160.0
145.10	219.0
145.90	540.0
147.00	407.0
148.00	637.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

148.80	312.0
149.90	305.0
151.90	143.0
152.90	169.0
153.80	170.0
154.90	471.0
155.80	175.0
156.90	544.0
157.90	178.0
158.80	305.0
160.90	431.0
163.00	361.0
163.80	76.0
165.10	292.0
166.00	78.0
171.20	192.0
171.90	1158.0
173.90	204160.0
175.00	15841.0
175.90	210048.0
177.00	13320.0
178.00	533.0
178.90	662.0
179.90	130.0
188.70	93.0
189.10	149.0
190.00	143.0
191.00	1715.0
191.90	362.0
193.00	2521.0
194.10	348.0
195.10	240.0
202.80	227.0
205.00	467.0
206.20	179.0
206.90	1504.0
208.10	249.0
208.90	136.0
216.80	54.0
220.90	152.0
235.20	208.0
235.70	75.0
249.10	1679.0
250.00	578.0
251.00	669.0
252.00	144.0
265.00	2151.0
266.00	536.0
267.00	614.0
268.10	77.0
268.80	75.0
279.30	133.0
281.00	25184.0
282.10	6231.0
283.00	4096.0
284.20	572.0
285.00	231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

Scan 1749 (12.566 min): VW017036.D
BFB26

m/z	Abundance
40.00	219.0
40.90	55.0
43.00	51.0
44.00	246.0
57.10	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26