
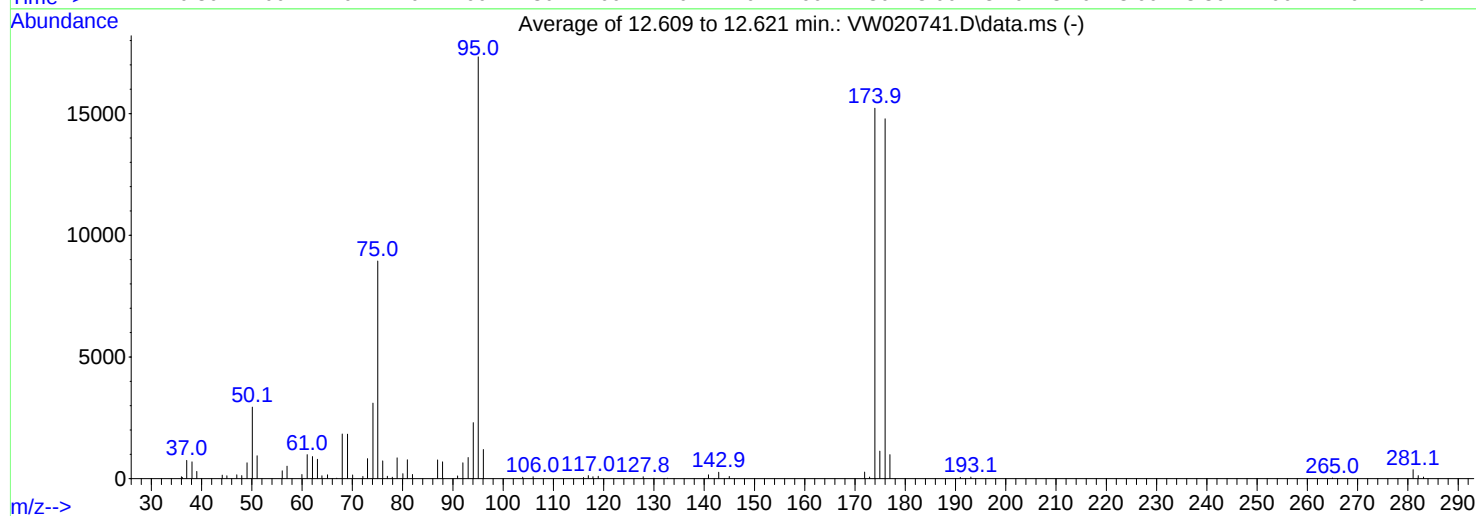


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110221\
 Data File : VW020741.D
 Acq On : 02 Nov 2021 11:54
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W110121S.M
 Title : SW846 8260
 Last Update : Thu Nov 04 15:37:33 2021

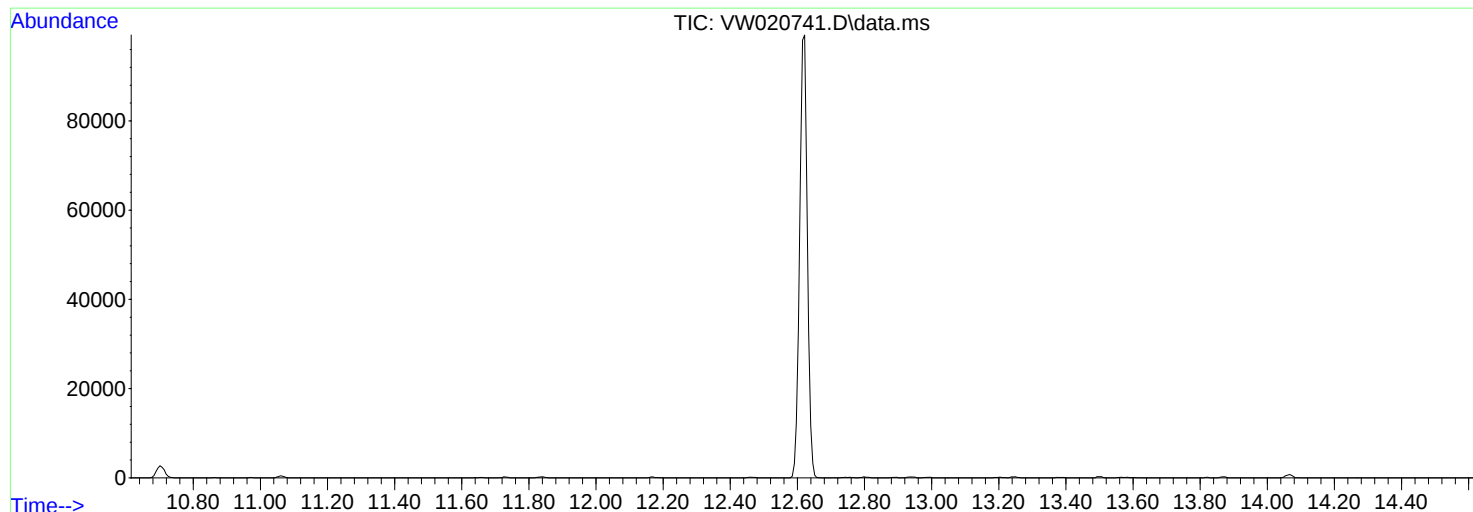

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	2938	PASS
75	95	30	60	51.6	8940	PASS
95	95	100	100	100.0	17332	PASS
96	95	5	9	6.9	1200	PASS
173	174	0.00	2	0.4	63	PASS
174	95	50	100	87.8	15221	PASS
175	174	5	9	7.4	1132	PASS
176	174	95	101	97.2	14790	PASS
177	176	5	9	6.7	987	PASS