


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW110318\
 Data File : VW006574.D
 Acq On : 01 Nov 2018 22:34
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
 Title : SW846 8260
 Last Update : Thu Nov 01 03:48:08 2018

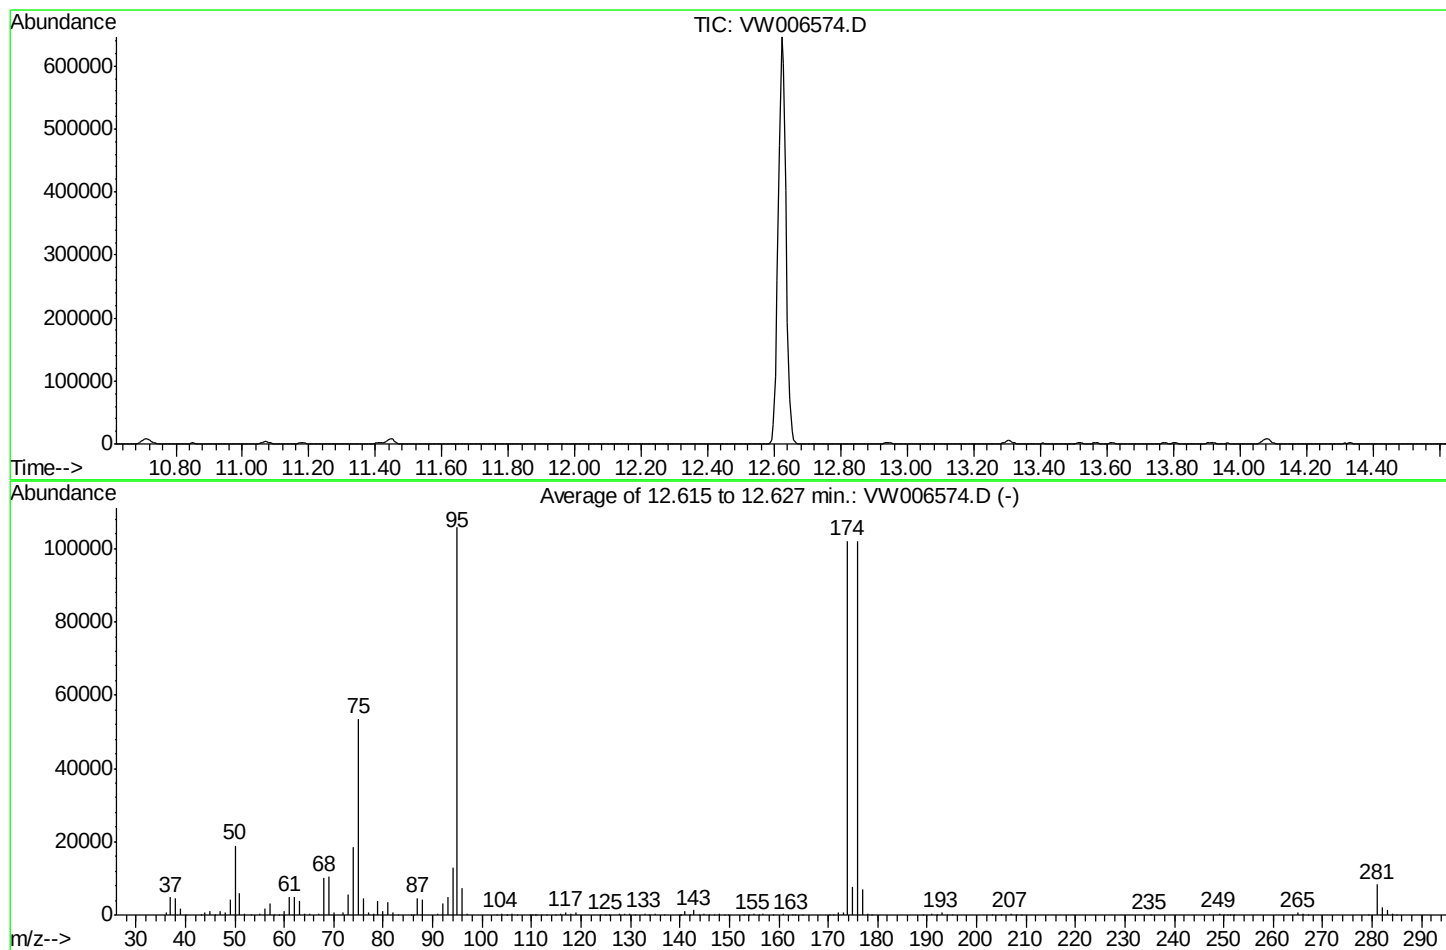

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	18909	PASS
75	95	30	60	50.6	53506	PASS
95	95	100	100	100.0	105832	PASS
96	95	5	9	6.9	7268	PASS
173	174	0.00	2	0.8	777	PASS
174	95	50	100	96.6	102218	PASS
175	174	5	9	7.5	7625	PASS
176	174	95	101	99.8	102037	PASS
177	176	5	9	6.8	6902	PASS