
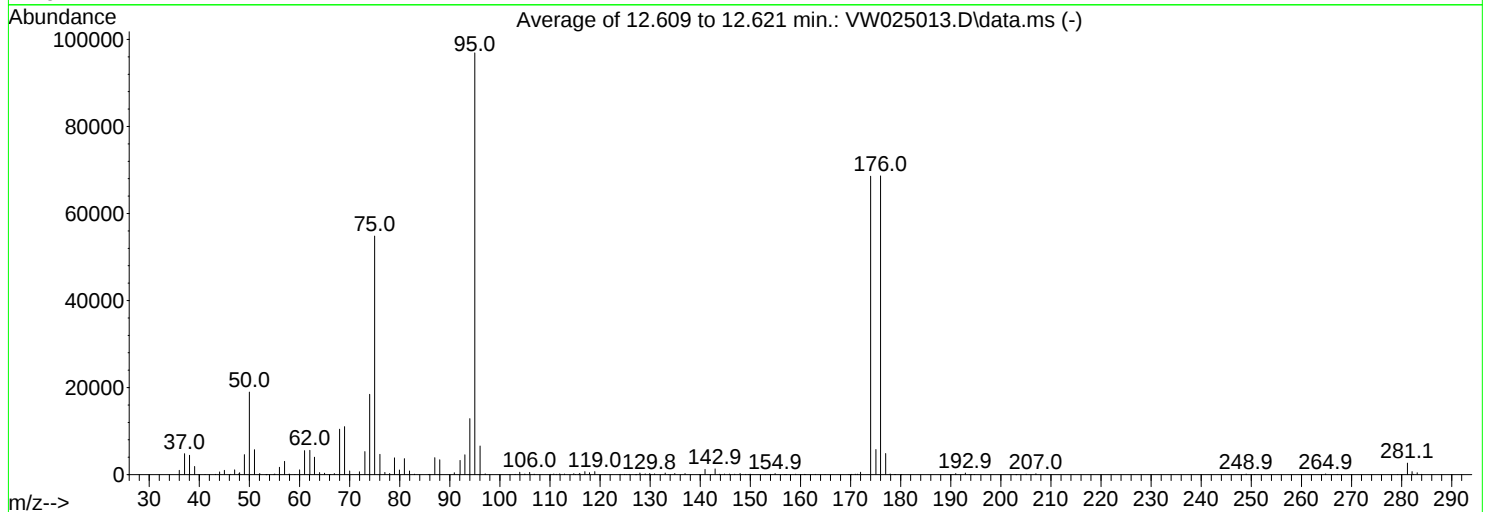


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110322\
 Data File : VW025013.D
 Acq On : 03 Nov 2022 07:00
 Operator : SY/VA
 Sample : BFB450
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB450

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Title : SFAM01.0
 Last Update : Fri Nov 04 04:15:36 2022

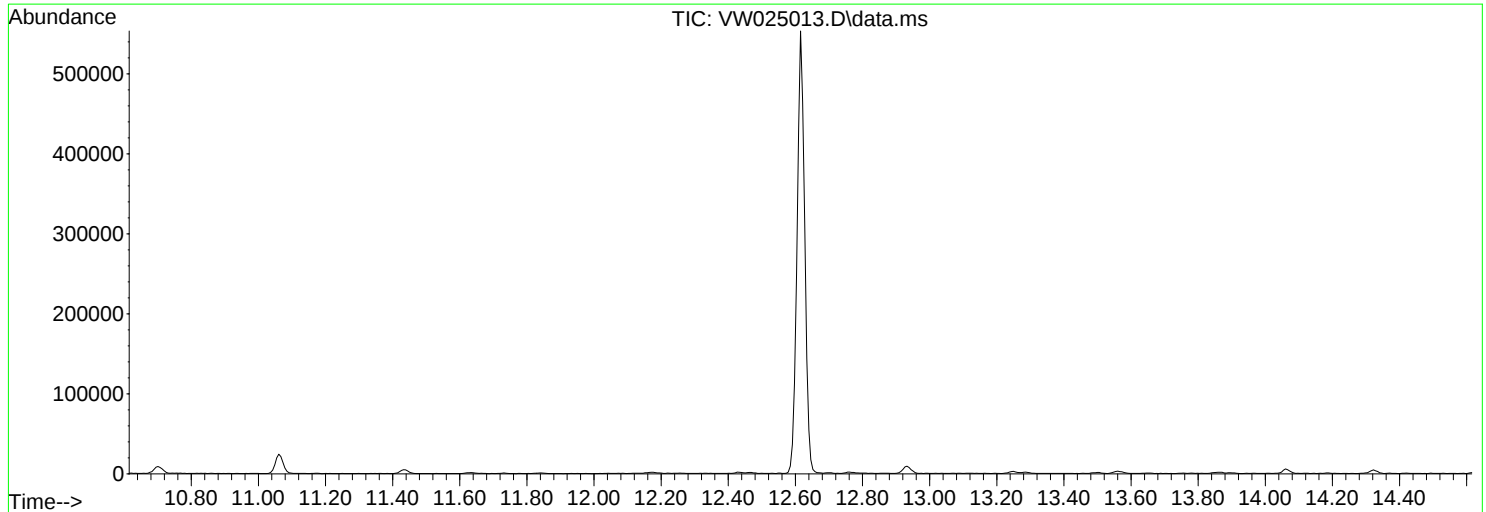

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	18957	PASS
75	95	30	80	56.6	54811	PASS
95	95	100	100	100.0	96917	PASS
96	95	5	9	6.8	6567	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.7	68565	PASS
175	174	5	9	8.4	5775	PASS
176	174	95	105	100.1	68621	PASS
177	176	5	10	7.1	4851	PASS

m/z	Abundance
35.90	139.0
38.10	52.0
39.90	315.0
44.10	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	1155.0
37.00	4867.0
38.10	4478.0
39.10	1822.0
40.00	306.0
41.10	53.0
43.20	85.0
44.00	661.0
45.00	1087.0
46.10	121.0
47.10	1013.0
47.90	632.0
49.00	4281.0
50.00	18248.0
51.00	5688.0
52.10	190.0
54.90	277.0
56.00	1546.0
57.00	3027.0
58.00	114.0
59.10	83.0
60.00	992.0
61.00	5281.0
62.00	5231.0
63.00	3904.0
64.00	621.0
65.10	334.0
66.10	63.0
66.90	257.0
68.00	9219.0
69.00	10428.0
70.00	867.0
72.00	480.0
73.00	5050.0
74.00	16824.0
75.00	49816.0
76.00	4296.0
77.00	526.0
78.00	426.0
78.90	3575.0
80.00	978.0
81.00	3456.0
81.90	713.0
83.00	62.0
85.80	141.0
87.00	3313.0
88.00	2801.0
91.00	419.0
92.10	3048.0
93.00	4200.0
94.00	11723.0
95.00	87656.0
96.00	6043.0
97.00	229.0
103.00	159.0
104.00	557.0
105.10	138.0
106.00	484.0
106.90	109.0
110.10	131.0
110.70	141.0
111.90	168.0
112.90	110.0
114.70	129.0
115.10	72.0
115.80	380.0
117.00	626.0
117.90	360.0
118.90	736.0
121.00	92.0
124.10	114.0
124.80	73.0
125.20	137.0
125.80	91.0
127.90	288.0
129.00	113.0
129.80	306.0
130.90	150.0
133.00	530.0
133.70	139.0
134.90	198.0
137.00	249.0
141.00	1008.0
142.90	1277.0
143.90	95.0
144.90	154.0
145.80	88.0
146.90	111.0
147.90	244.0
149.10	80.0
149.70	76.0
150.10	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

154.10	66.0
154.90	209.0
156.80	157.0
159.10	68.0
161.20	58.0
163.00	146.0
164.90	74.0
170.90	113.0
172.00	451.0
174.00	53992.0
175.00	5077.0
176.00	55600.0
177.00	4230.0
177.90	155.0
178.80	101.0
180.00	56.0
191.00	389.0
192.90	571.0
193.80	84.0
194.70	62.0
205.00	176.0
207.10	270.0
208.00	69.0
249.00	239.0
250.70	66.0
264.80	239.0
267.20	130.0
279.20	60.0
280.00	127.0
281.10	3688.0
282.10	1189.0
283.10	596.0
284.00	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	1193.0
37.00	5179.0
38.00	4773.0
39.00	2208.0
40.10	419.0
41.20	53.0
43.20	101.0
44.10	739.0
45.00	1086.0
46.20	97.0
47.10	1307.0
48.10	721.0
49.00	5197.0
50.00	21032.0
51.00	6236.0
52.00	319.0
53.30	56.0
55.10	208.0
56.00	1805.0
57.00	3587.0
57.90	182.0
59.10	58.0
60.00	1231.0
61.00	6410.0
62.00	6360.0
63.00	4488.0
64.00	410.0
65.00	445.0
66.10	61.0
66.90	317.0
68.00	11986.0
69.00	12138.0
70.00	980.0
72.00	858.0
73.10	5695.0
74.00	21560.0
75.00	62040.0
76.10	5588.0
77.10	457.0
78.90	4445.0
80.00	1228.0
80.90	4124.0
82.00	996.0
83.00	105.0
86.00	123.0
87.00	4529.0
88.00	3940.0
90.80	532.0
92.00	3476.0
93.00	5127.0
94.00	14788.0
95.00	112000.0
96.10	7609.0
97.10	249.0
103.90	575.0
105.00	140.0
106.00	517.0
106.80	92.0
110.10	103.0
110.80	165.0
111.20	137.0
112.00	227.0
112.90	224.0
114.70	237.0
116.00	477.0
116.90	772.0
118.00	498.0
118.90	837.0
123.90	65.0
124.90	121.0
125.80	91.0
127.10	57.0
127.90	387.0
129.10	241.0
130.10	333.0
130.80	215.0
133.00	388.0
134.00	58.0
134.90	302.0
137.00	289.0
139.90	70.0
140.90	1574.0
142.10	151.0
143.00	1403.0
143.90	84.0
144.80	134.0
145.90	203.0
146.80	187.0
147.90	286.0
149.10	58.0
149.90	134.0
153.00	74.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

154.00	108.0
155.00	326.0
157.00	172.0
159.00	168.0
160.80	215.0
162.90	74.0
169.70	68.0
170.20	120.0
171.00	202.0
171.40	210.0
172.10	625.0
174.00	79528.0
175.10	6611.0
176.00	80680.0
177.00	5511.0
177.90	125.0
179.00	106.0
191.10	176.0
192.90	382.0
194.10	152.0
203.00	50.0
205.10	122.0
206.90	189.0
248.90	258.0
250.70	56.0
264.90	235.0
267.10	80.0
281.20	2881.0
282.10	902.0
283.10	446.0
284.00	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.10	1008.0
37.10	4389.0
38.10	4291.0
39.10	1600.0
40.00	396.0
44.00	749.0
45.00	755.0
47.00	1036.0
48.00	608.0
49.00	4268.0
50.00	17592.0
51.00	5282.0
52.00	304.0
55.00	260.0
56.00	1742.0
57.00	2496.0
57.90	106.0
60.00	1123.0
61.00	4905.0
62.10	5203.0
63.00	3659.0
64.00	367.0
64.90	187.0
67.00	258.0
68.00	10093.0
69.00	10499.0
70.00	737.0
71.90	686.0
73.00	5122.0
74.00	17000.0
75.00	52576.0
76.00	4143.0
77.10	571.0
78.00	368.0
79.00	3588.0
79.90	1055.0
80.90	3438.0
81.90	859.0
82.90	122.0
86.00	126.0
87.00	3840.0
88.00	3567.0
90.90	429.0
92.00	3268.0
93.00	4393.0
94.00	12078.0
95.00	91096.0
96.00	6049.0
97.00	92.0
103.10	97.0
103.90	484.0
104.90	160.0
105.90	591.0
106.80	108.0
110.20	52.0
110.80	148.0
111.30	69.0
112.00	152.0
112.90	128.0
114.80	267.0
115.90	424.0
116.90	718.0
117.80	439.0
119.00	582.0
123.90	80.0
124.80	86.0
128.00	399.0
128.90	212.0
129.90	353.0
131.00	167.0
132.90	213.0
134.00	93.0
134.90	231.0
136.90	200.0
140.90	1006.0
142.90	1342.0
143.90	130.0
144.90	149.0
145.90	116.0
147.00	64.0
148.00	264.0
149.00	100.0
150.00	141.0
152.90	72.0
154.00	77.0
155.00	250.0
157.20	144.0
159.10	95.0
161.00	114.0
169.70	74.0
170.20	91.0
171.20	113.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

171.90	634.0
174.00	72176.0
175.00	5638.0
176.00	69584.0
177.00	4811.0
177.90	170.0
190.90	184.0
192.80	139.0
205.00	53.0
207.00	197.0
264.80	103.0
281.10	1365.0
282.30	264.0
283.10	323.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450