

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110323\
 Data File : VW027533.D
 Acq On : 03 Nov 2023 13:58
 Operator : SY/MD
 Sample : 05174-08
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Nov 04 00:17:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 04 00:15:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	365349	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	328710	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	167130	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	112857	20.241	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.960%
7) Chloroethane-d5	2.899	69	93252	23.292	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.160%
11) 1,1-Dichloroethene-d2	4.021	65	58069	20.784	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.120%
21) 2-Butanone-d5	7.081	46	65119	35.137	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.280%
24) Chloroform-d	7.648	84	249701	22.931	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.720%
26) 1,2-Dichloroethane-d4	8.307	65	125535	21.461	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.840%
32) Benzene-d6	8.276	84	520376	23.399	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	9.276	67	161524	23.779	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.120%
41) Toluene-d8	10.325	98	449469	22.287	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.160%
43) trans-1,3-Dichloroprop...	10.581	79	52530	16.961	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.840%
47) 2-Hexanone-d5	10.922	63	46537	33.113	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.220%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	103560	20.434	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.720%
66) 1,2-Dichlorobenzene-d4	13.848	152	133212	21.995	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.960%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	18032	2.696	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110323\
Data File : VW027533.D
Acq On : 03 Nov 2023 13:58
Operator : SY/MD
Sample : 05174-08
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002


Quant Time: Nov 04 00:17:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 04 00:15:46 2023
Response via : Initial Calibration

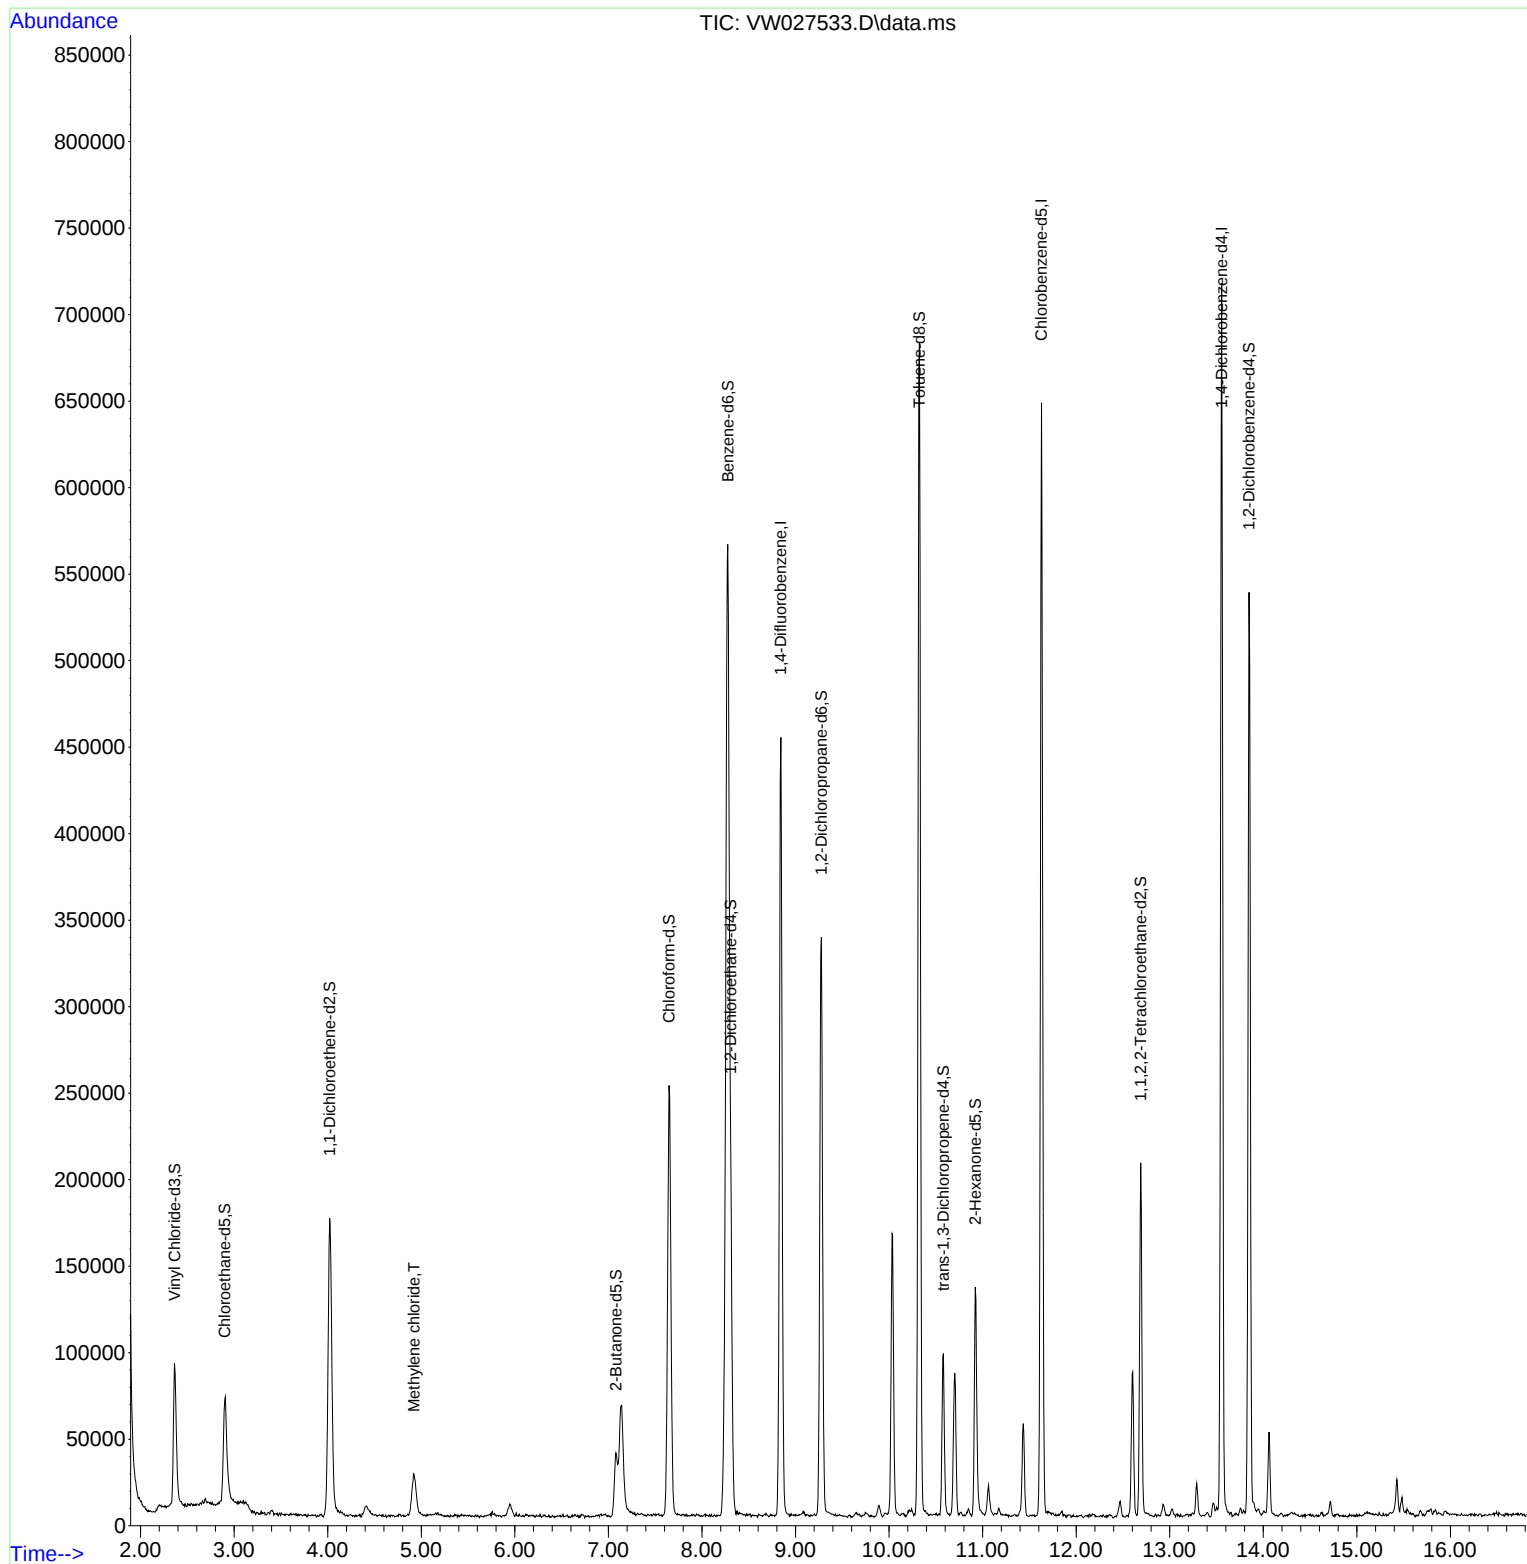

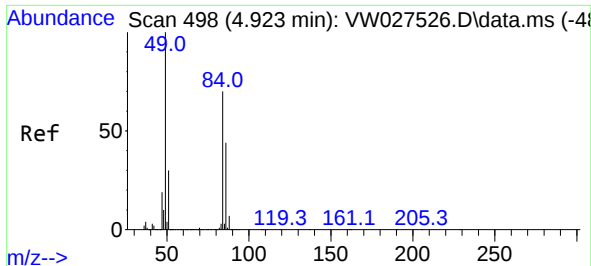

#16
Methylene chloride
Concen: 2.696 ug/L
RT: 4.923 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW027533.D
Acq: 03 Nov 2023 13:58

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

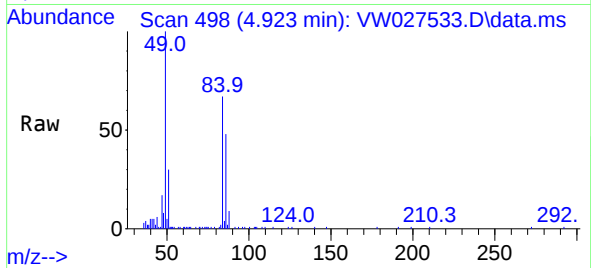

Tgt Ion: 84 Resp: 18032
Ion Ratio Lower Upper
84 100
86 71.5 41.3 76.7
49 149.8 92.8 172.4

