

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW110518\
 Data File : VW006627.D
 Acq On : 05 Nov 2018 11:13
 Operator : SY/AP
 Sample : VW1105SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW1105SBL01

Quant Time: Nov 05 14:55:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 01 03:48:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	285743	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	397101	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	357323	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	186249	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	113146	46.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.12%	
35) Dibromofluoromethane	7.88	113	126483	50.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.50%	
50) Toluene-d8	10.33	98	488272	51.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.94%	
62) 4-Bromofluorobenzene	12.62	95	162405	47.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.44%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW110518\
Data File : VW006627.D
Acq On : 05 Nov 2018 11:13
Operator : SY/AP
Sample : VW1105SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW1105SBL01

Quant Time: Nov 05 14:55:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W110218S.M
Quant Title : SW846 8260
QLast Update : Thu Nov 01 03:48:08 2018
Response via : Initial Calibration

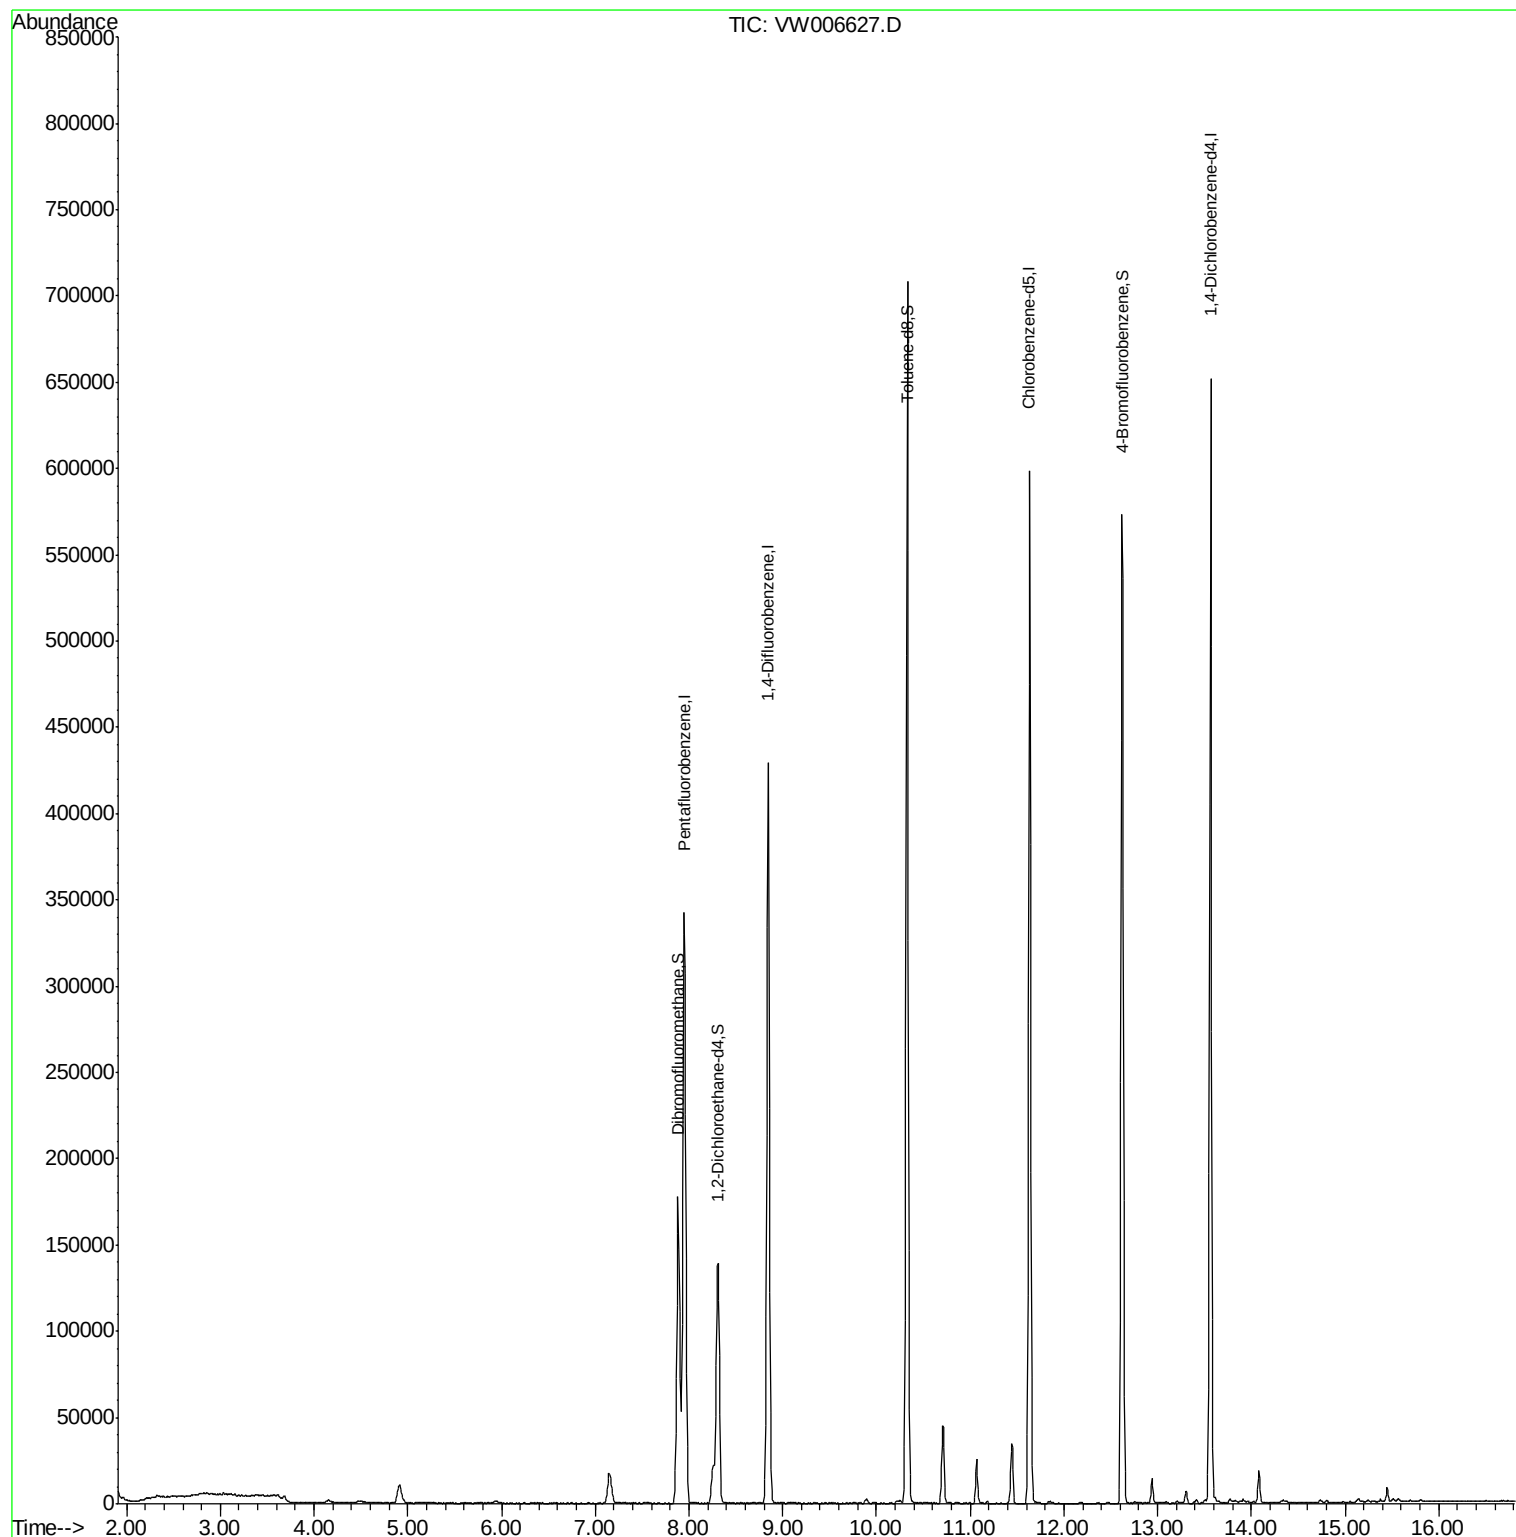

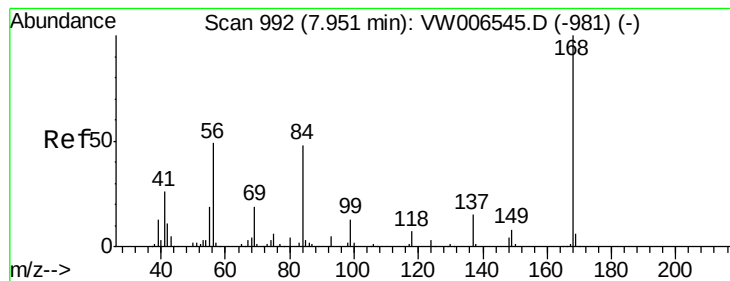

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.00 min

Lab File: VW006627.D

Acq: 05 Nov 2018 11:13

Instrument :

MSVOA_W

ClientSampleId :


VW1105SBL01

Tot Ion:168 Resp: 285743

Ion Ratio Lower Upper

168 100

99 47.2 37.4 56.0

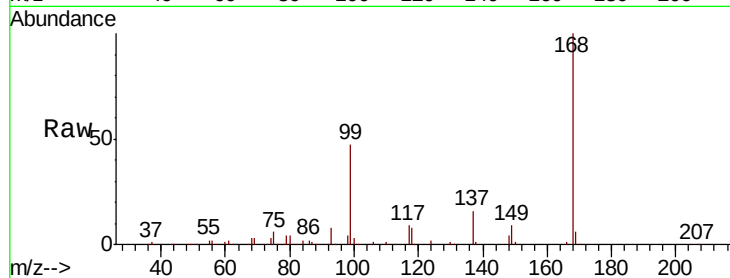

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95



150000

100000

50000

0

Time-->

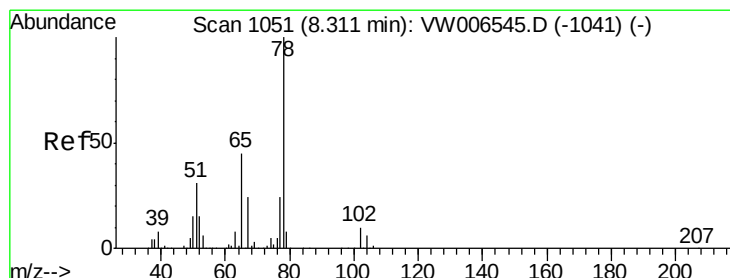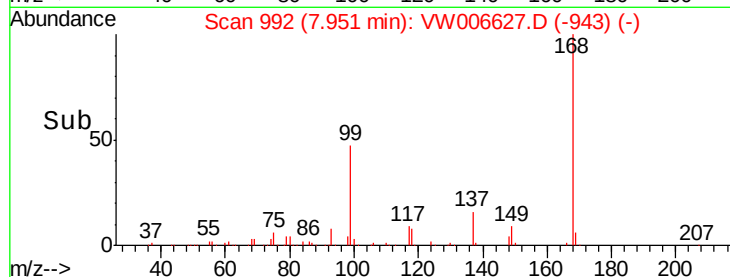

#33

1,2-Dichloroethane-d4

Concen: 46.065 ug/l

RT: 8.30 min Scan# 1050

Delta R.T. -0.01 min

Lab File: VW006627.D


Acq: 05 Nov 2018 11:13

Tgt Ion: 65 Resp: 113146

Ion Ratio Lower Upper

65 100

67 52.3 0.0 104.4

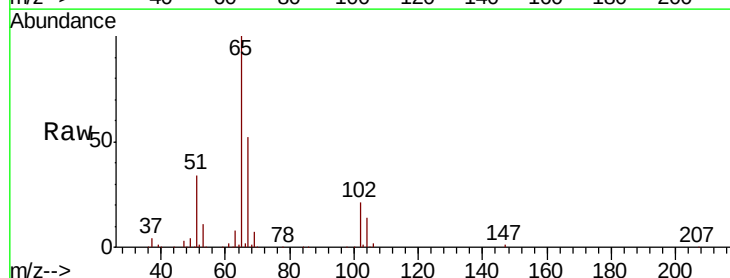

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.30

60000

50000

40000


30000


20000

10000

0

Time-->

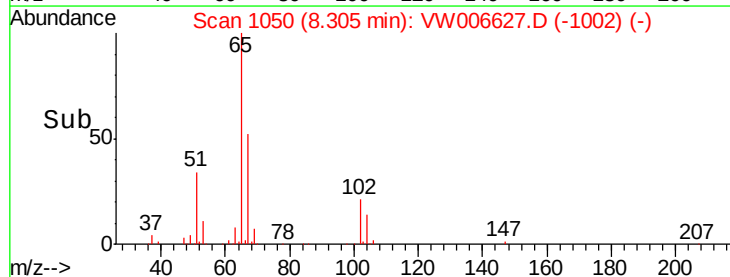

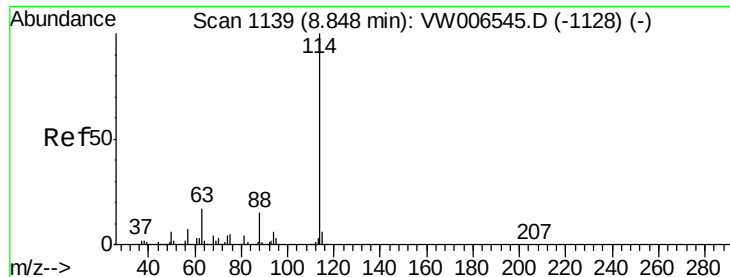

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.85 min Scan# 1139

Delta R.T. -0.00 min

Lab File: VW006627.D

Acq: 05 Nov 2018 11:13

Instrument :

MSVOA_W

ClientSampleId :

VW1105SBL01


Tot Ion:114 Resp: 397101

Ion Ratio Lower Upper

114 100

63 16.9 0.0 34.4

88 14.1 0.0 29.0

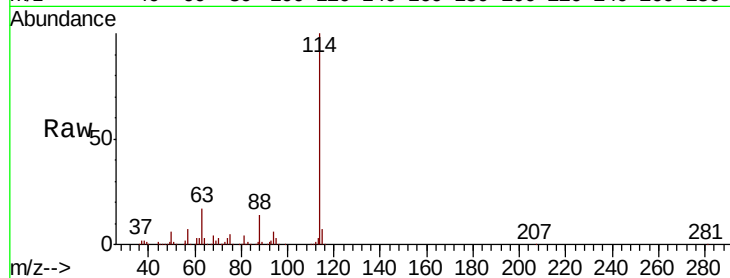

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

250000

200000

150000

100000



50000

0

8.80

8.90

Time-->

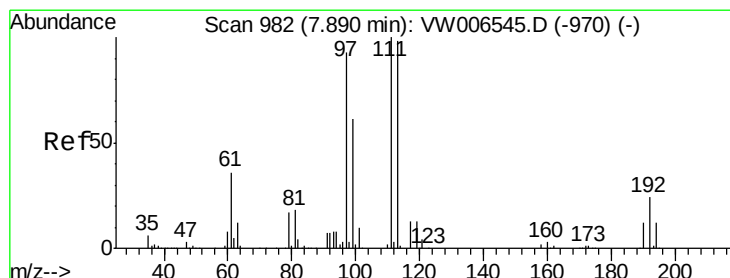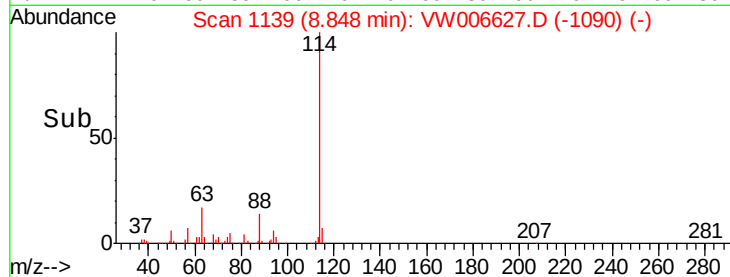

#35

Dibromofluoromethane

Concen: 50.753 ug/l

RT: 7.88 min Scan# 981

Delta R.T. -0.01 min

Lab File: VW006627.D

Acq: 05 Nov 2018 11:13


Tgt Ion:113 Resp: 126483

Ion Ratio Lower Upper

113 100

111 102.5 82.2 123.2

192 24.0 19.0 28.6

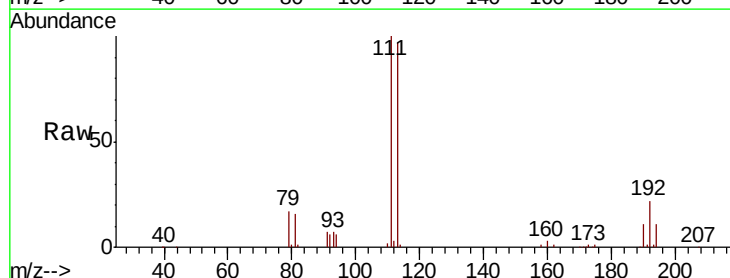

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

60000

40000


20000


0

7.80

7.90

Time-->

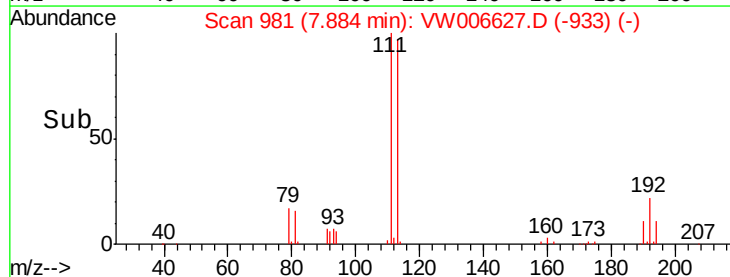

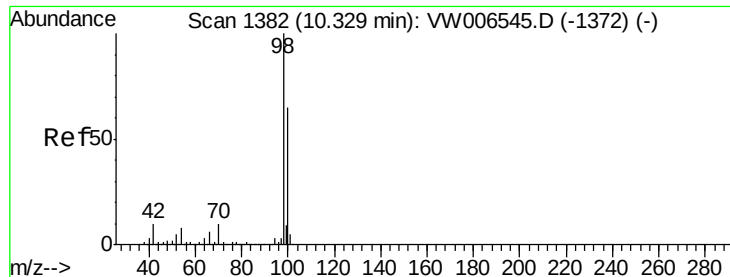

#50

Toluene-d8

Concen: 51.467 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. -0.00 min

Lab File: VW006627.D

Acq: 05 Nov 2018 11:13

Instrument :

MSVOA_W

ClientSampleId :





VW1105SBL01

Tot Ion: 98 Resp: 488272

Ion Ratio Lower Upper

98 100

100 64.6 51.6 77.4

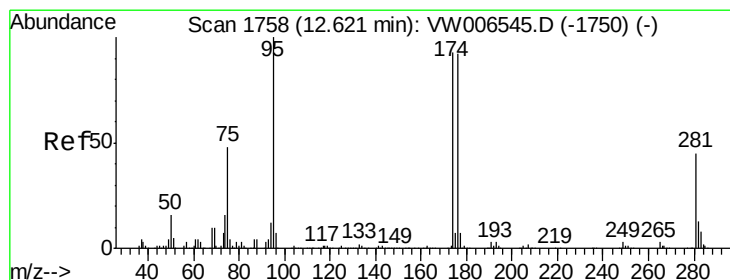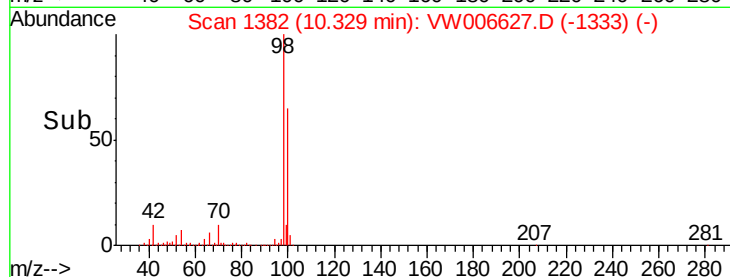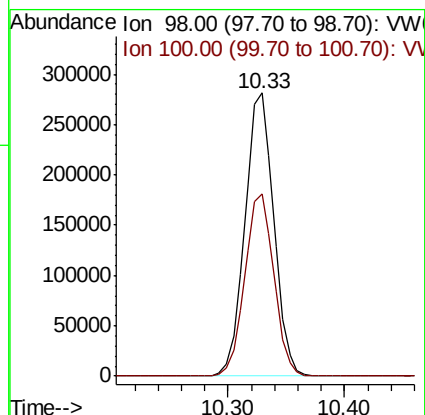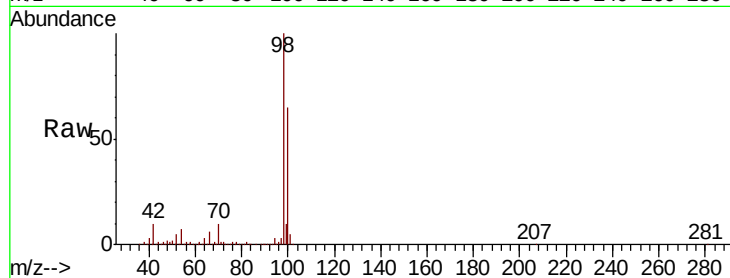

#62

4-Bromofluorobenzene

Concen: 47.219 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW006627.D

Acq: 05 Nov 2018 11:13




Tgt Ion: 95 Resp: 162405


Ion Ratio Lower Upper

95 100

174 98.6 0.0 192.4

176 95.9 0.0 187.4


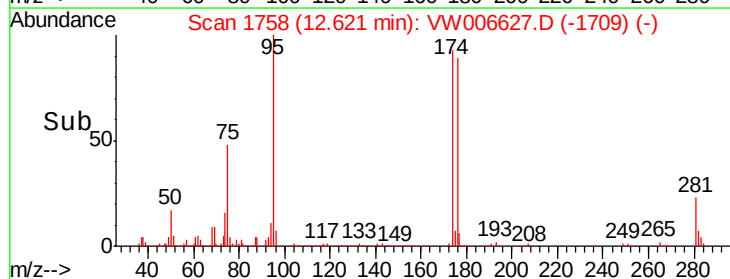
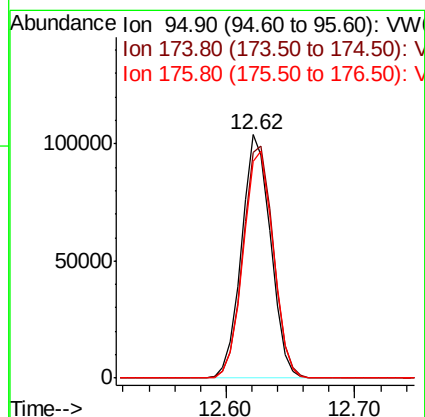
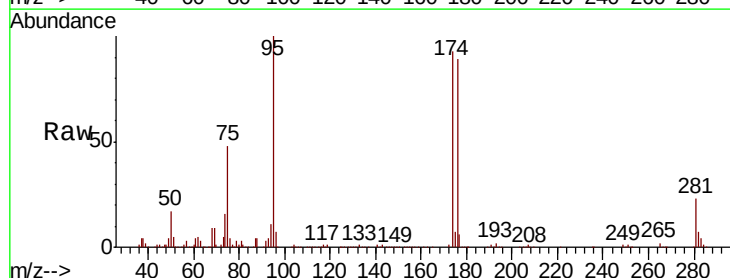


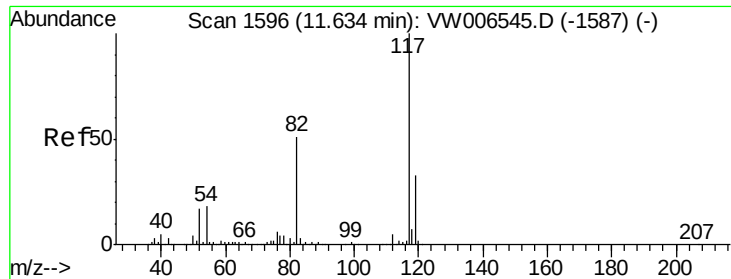

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW006627.D
Acq: 05 Nov 2018 11:13

Instrument :
MSVOA_W
ClientSampleId :
VW1105SBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	51.5	40.8	61.2
119	32.7	26.1	39.1

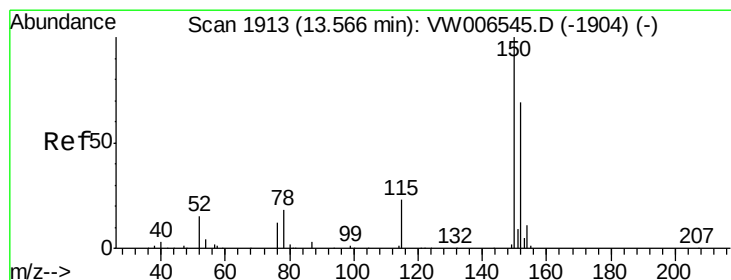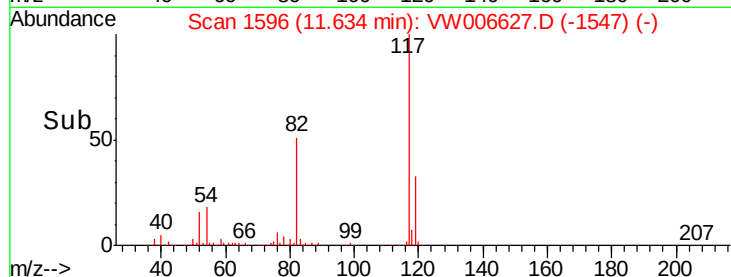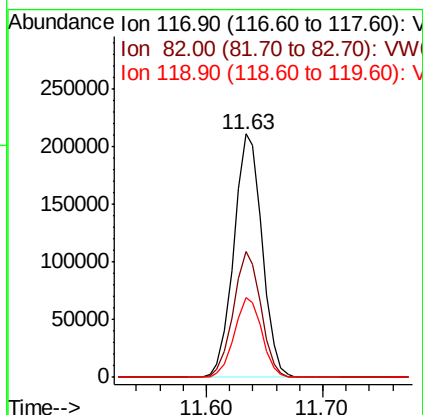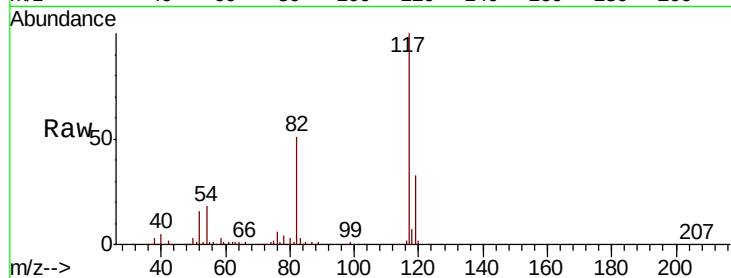

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1913
Delta R.T. -0.00 min
Lab File: VW006627.D
Acq: 05 Nov 2018 11:13

Tgt Ion	Ratio	Lower	Upper
152	100		
115	53.2	26.6	79.8
150	156.3	0.0	344.6

